

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111325\
 Data File : PD091146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2025 12:44
 Operator : AR\AJ
 Sample : Q3609-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-713-COMP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 22:02:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.874	38784594	404.0E6	12.454	13.566
28)	SA Decachlor...	9.066	8.059	52413414	394.0E6	11.204	13.006
Target Compounds							
11)	B alpha-Chl...	6.022	5.179	4734418	21638758	0.766	0.502 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111325\
Data File : PD091146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2025 12:44
Operator : AR\AJ
Sample : Q3609-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 22:02:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

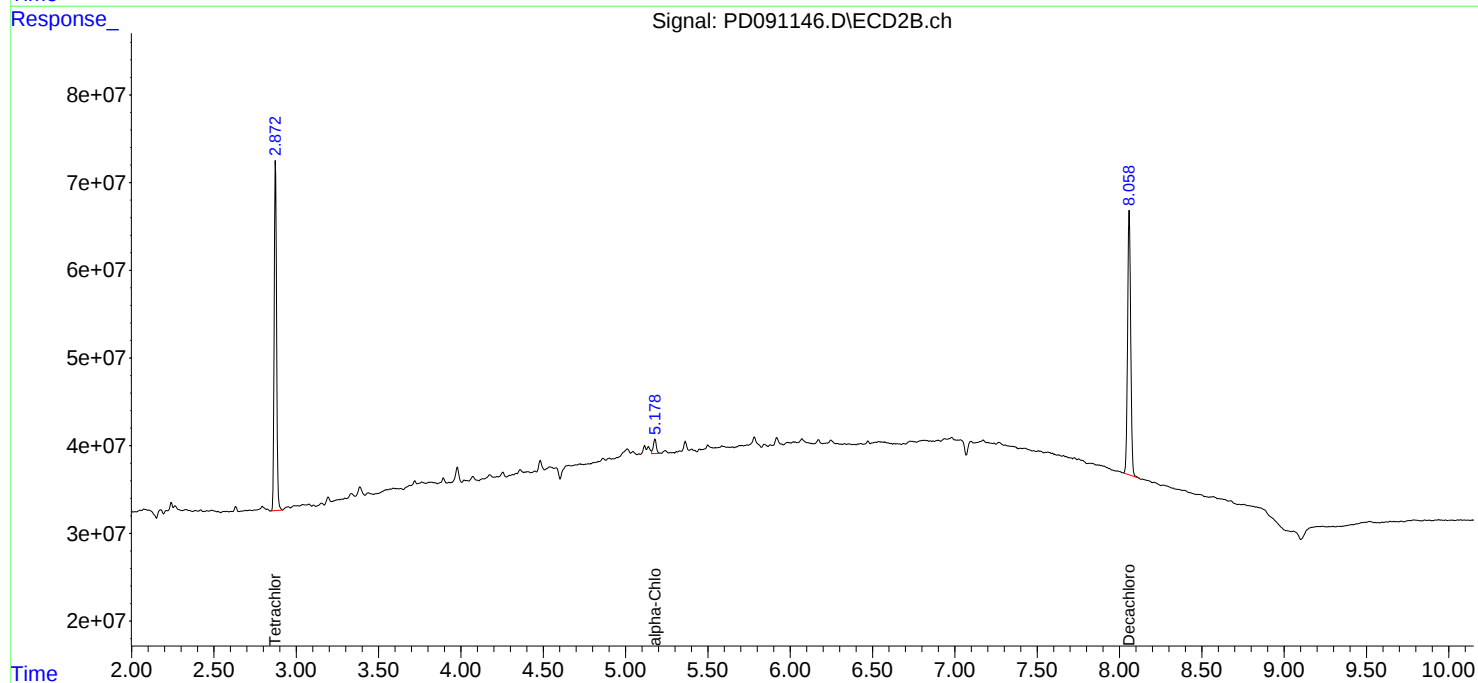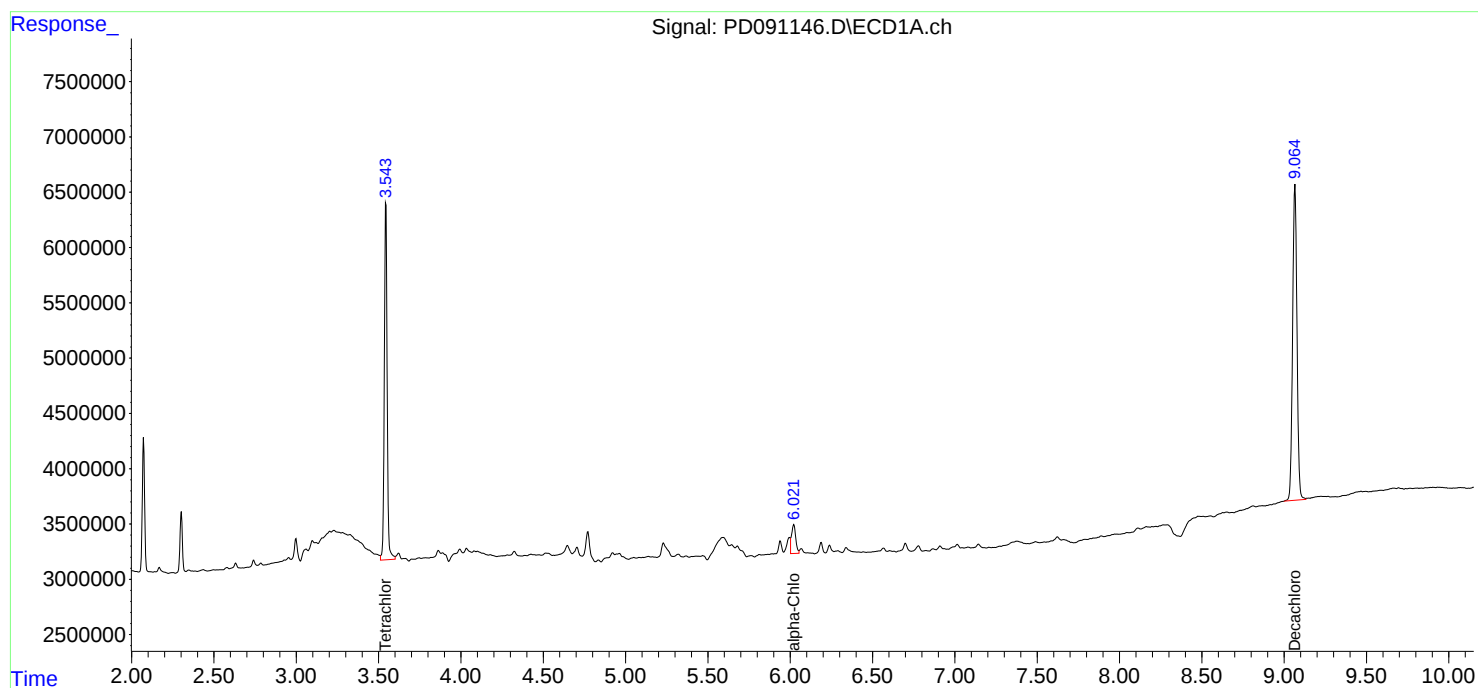


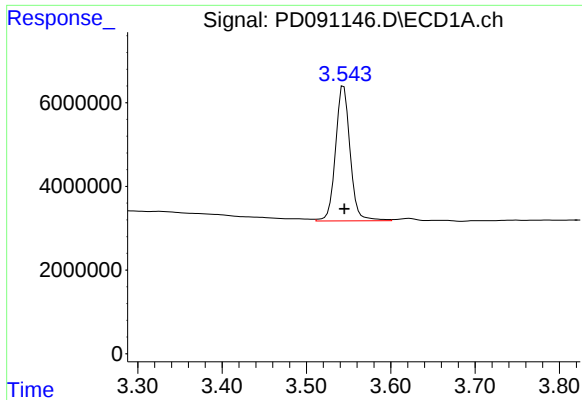

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 38784594
Conc: 12.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-01

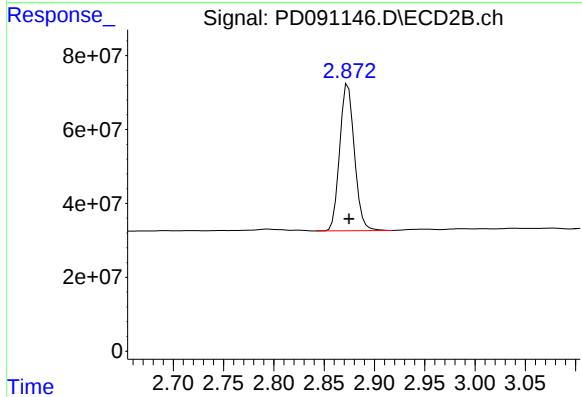


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 403962091
Conc: 13.57 ng/ml

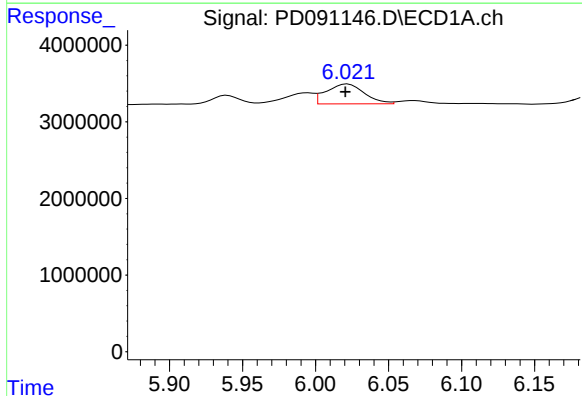


#11 alpha-Chlordane

R.T.: 6.022 min
Delta R.T.: 0.002 min
Response: 4734418
Conc: 0.77 ng/ml

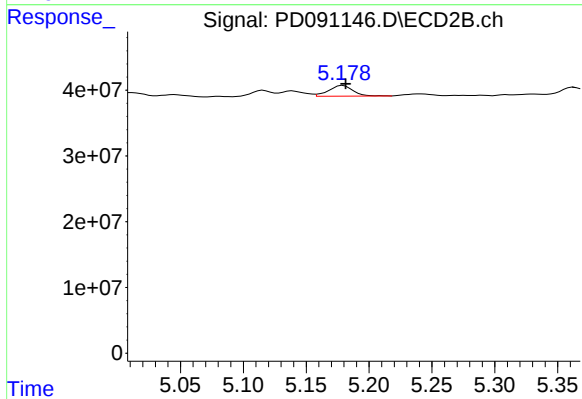

#11 alpha-Chlordane


R.T.: 5.179 min
Delta R.T.: -0.002 min
Response: 21638758
Conc: 0.50 ng/ml

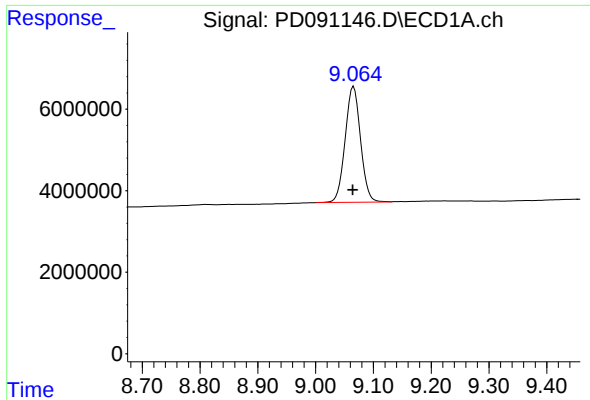

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.002 min
Response: 52413414
Conc: 11.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-01

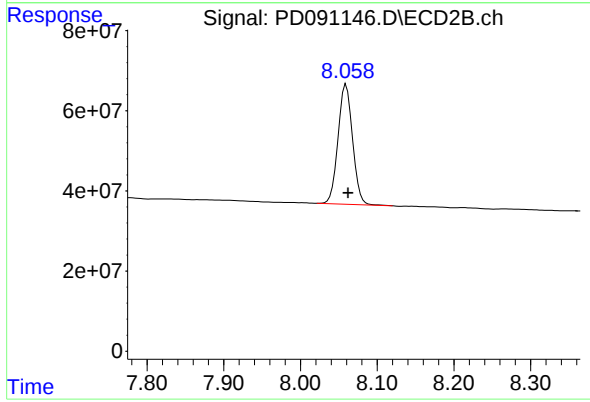

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.002 min
Response: 393972961
Conc: 13.01 ng/ml