

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111325\
 Data File : PD091148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2025 13:11
 Operator : AR\AJ
 Sample : Q3609-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-713-COMP-03

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/14/2025
 Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 22:03:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.872	40074313	439.9E6	12.868m	14.773m
28) SA Decachlor...	9.064	8.059	53035857	377.9E6	11.337m	12.474
Target Compounds						
8) B Heptachlo...	5.681	4.863	1921.1E6	9942.4E6	331.851m	233.176 #
10) B gamma-Chl...	5.940	5.109	8694.4E6	38948.7E6	1465.887	866.512m#
11) B alpha-Chl...	6.021	5.183	11871.7E6	36102.9E6	1920.901	836.922 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111325\
Data File : PD091148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2025 13:11
Operator : AR\AJ
Sample : Q3609-07
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 22:03:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

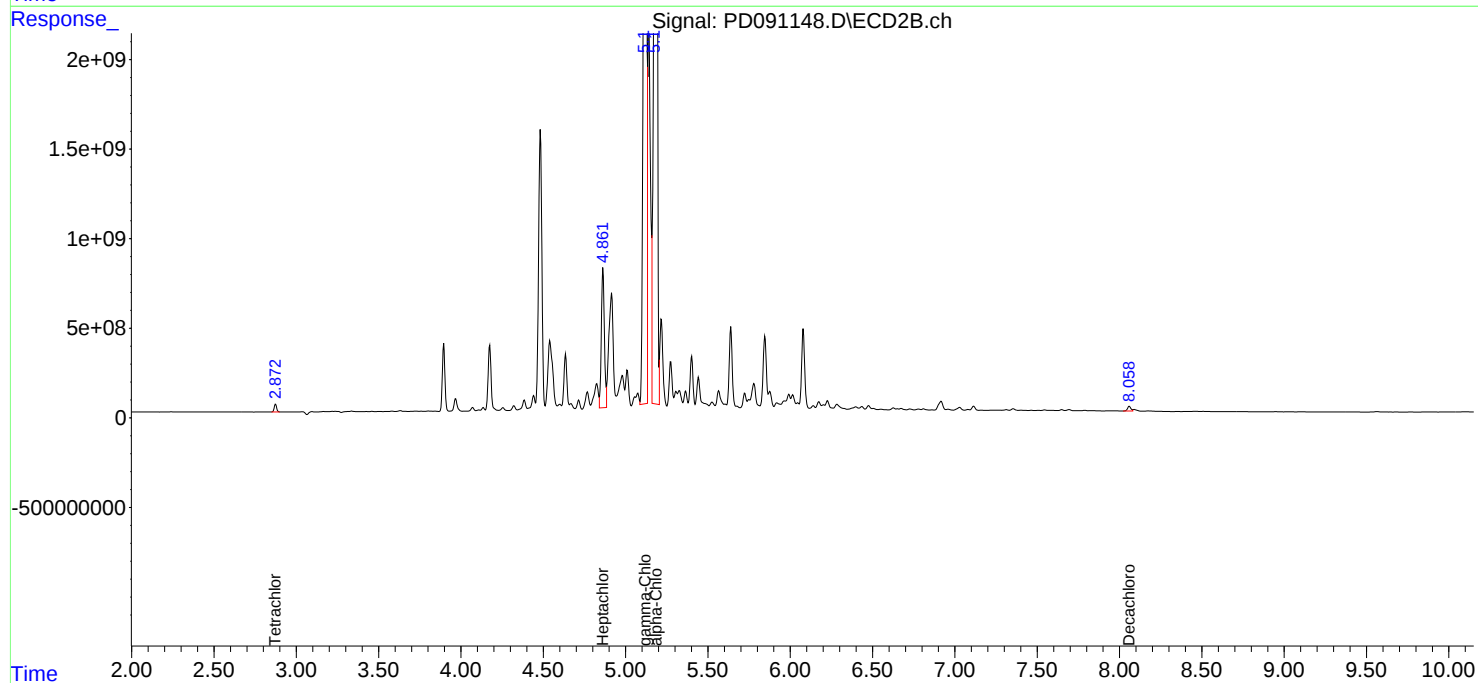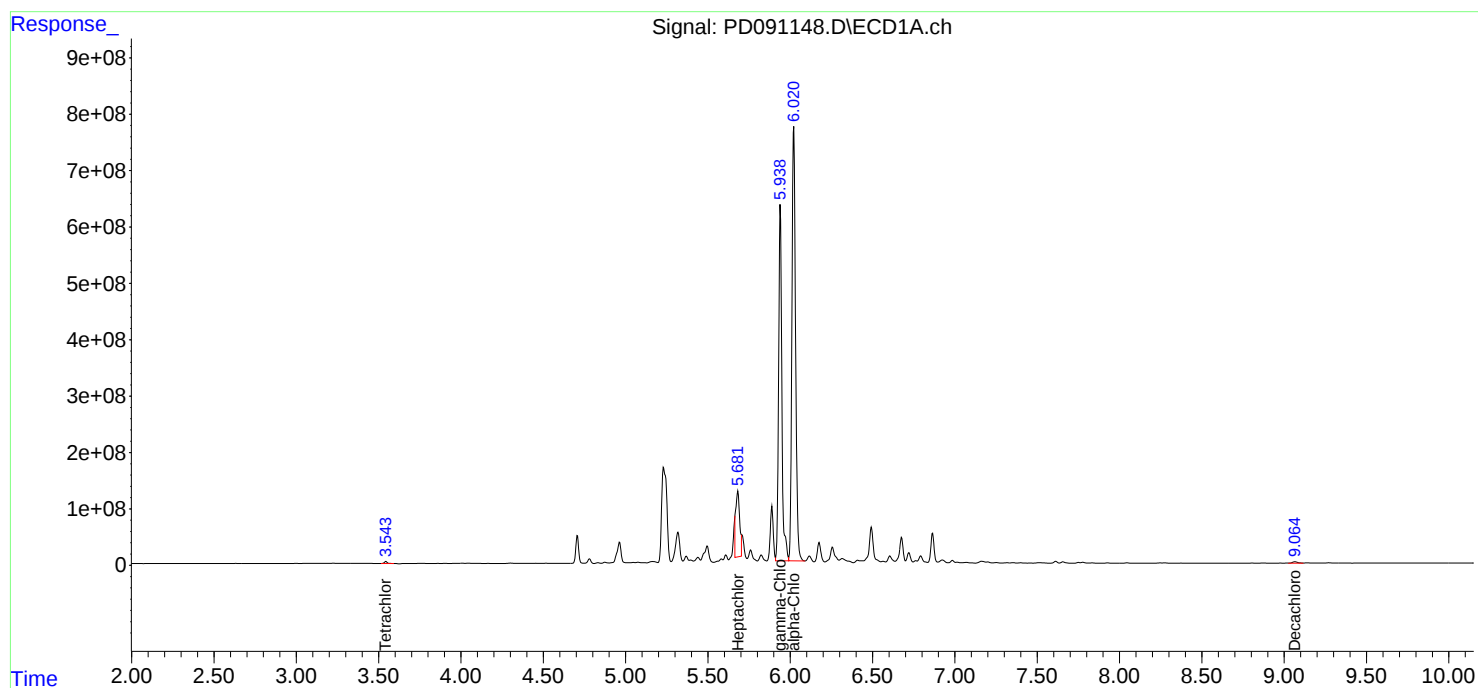

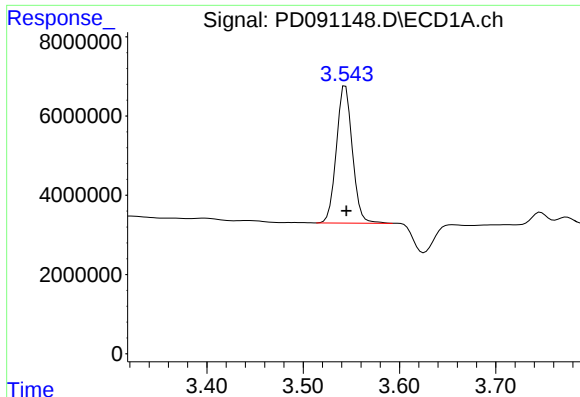


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 40074313
Conc: 12.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

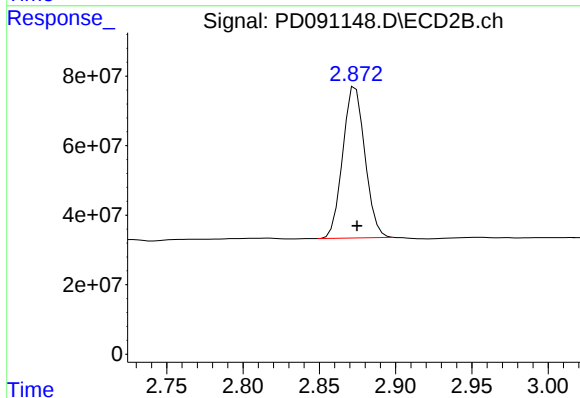


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.002 min
Response: 439910444
Conc: 14.77 ng/ml m

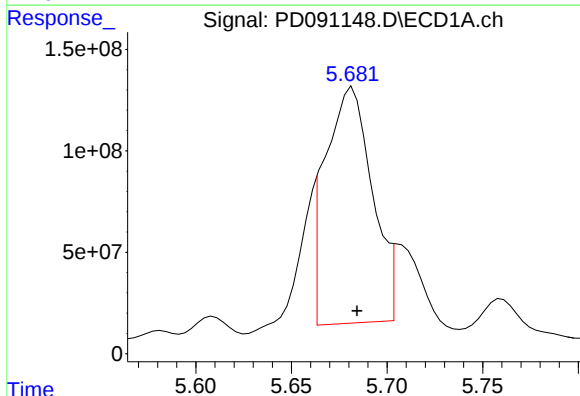


#8 Heptachlor epoxide

R.T.: 5.681 min
Delta R.T.: -0.004 min
Response: 1921108604
Conc: 331.85 ng/ml m

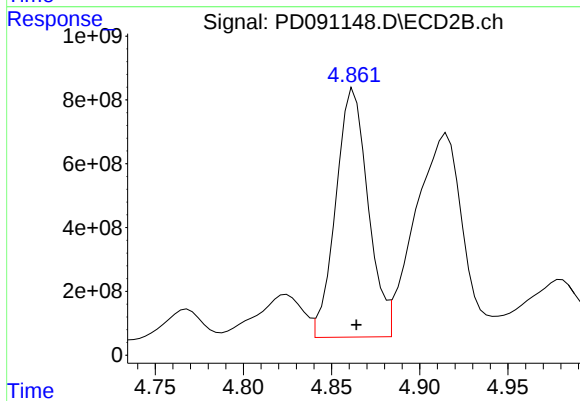

#8 Heptachlor epoxide

R.T.: 4.863 min
Delta R.T.: -0.001 min
Response: 9942373479
Conc: 233.18 ng/ml

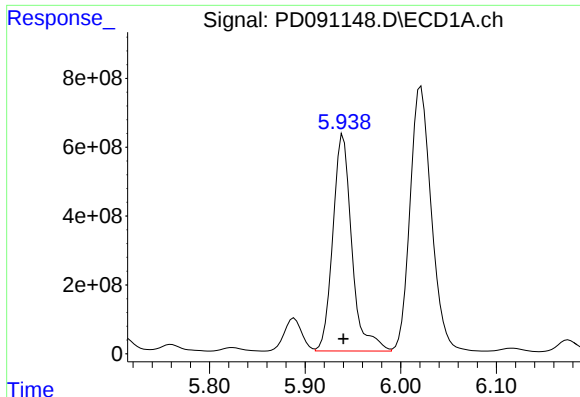


#10 gamma-Chlordane

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 8694436856
Conc: 1465.89 ng/m

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

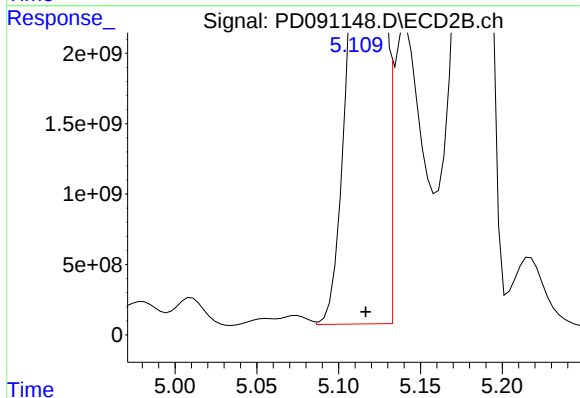


#10 gamma-Chlordane

R.T.: 5.109 min
Delta R.T.: -0.007 min
Response: 38948736773
Conc: 866.51 ng/ml m

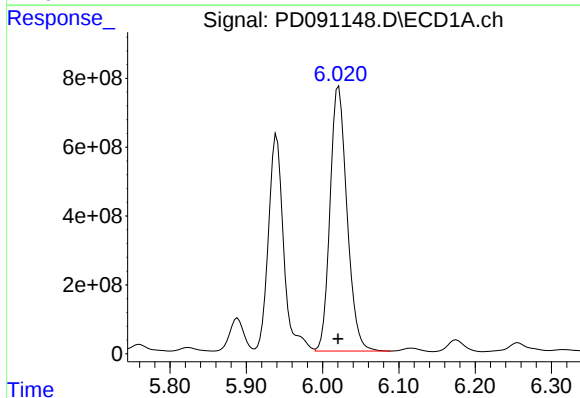


#11 alpha-Chlordane

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 11871658492
Conc: 1920.90 ng/ml

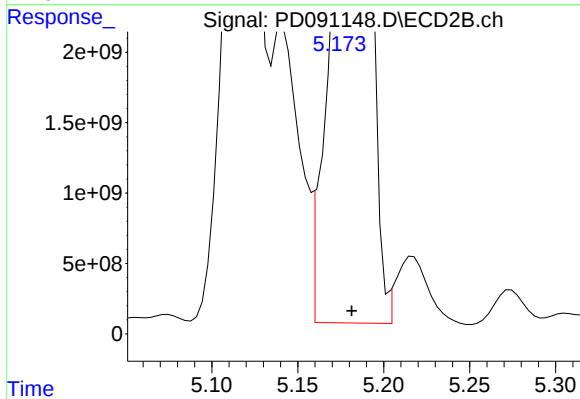

#11 alpha-Chlordane

R.T.: 5.183 min
Delta R.T.: 0.002 min
Response: 36102921699
Conc: 836.92 ng/ml

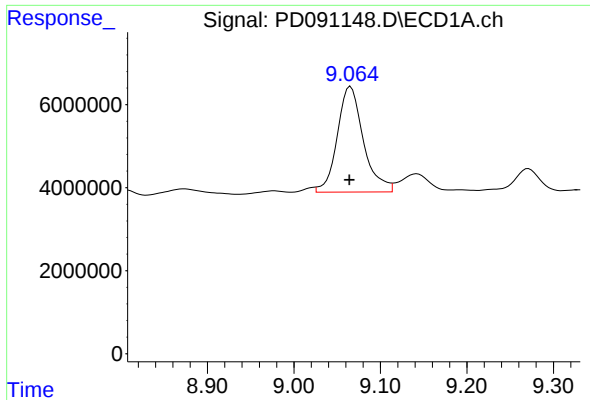


#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.000 min
Response: 53035857
Conc: 11.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

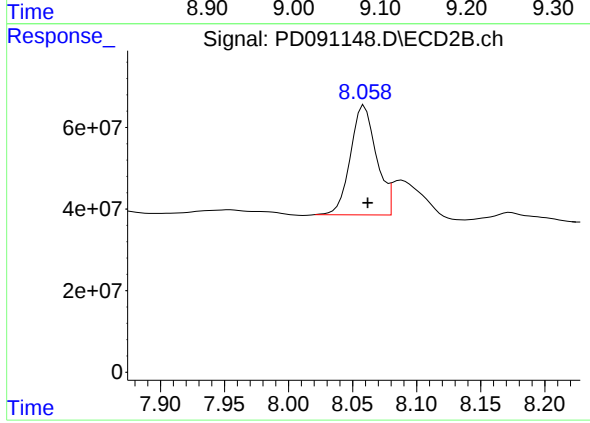

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.003 min
Response: 377864554
Conc: 12.47 ng/ml