

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
 Data File : PD055973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 09:28
 Operator : SG\AJ
 Sample : K5815-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A5460

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:54:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.962	16802239	22157019	22.320	21.143
27)	SA Decachlor...	7.965	8.997	31341658	38238396	38.451	33.674
Target Compounds							
2)	A alpha-BHC	0.000	4.386f	0	1616879	N.D.	1.135
3)	MA gamma-BHC...	0.000	4.595f	0	448078	N.D.	0.318


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
Data File : PD055973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 09:28
Operator : SG\AJ
Sample : K5815-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
A5460

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:54:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

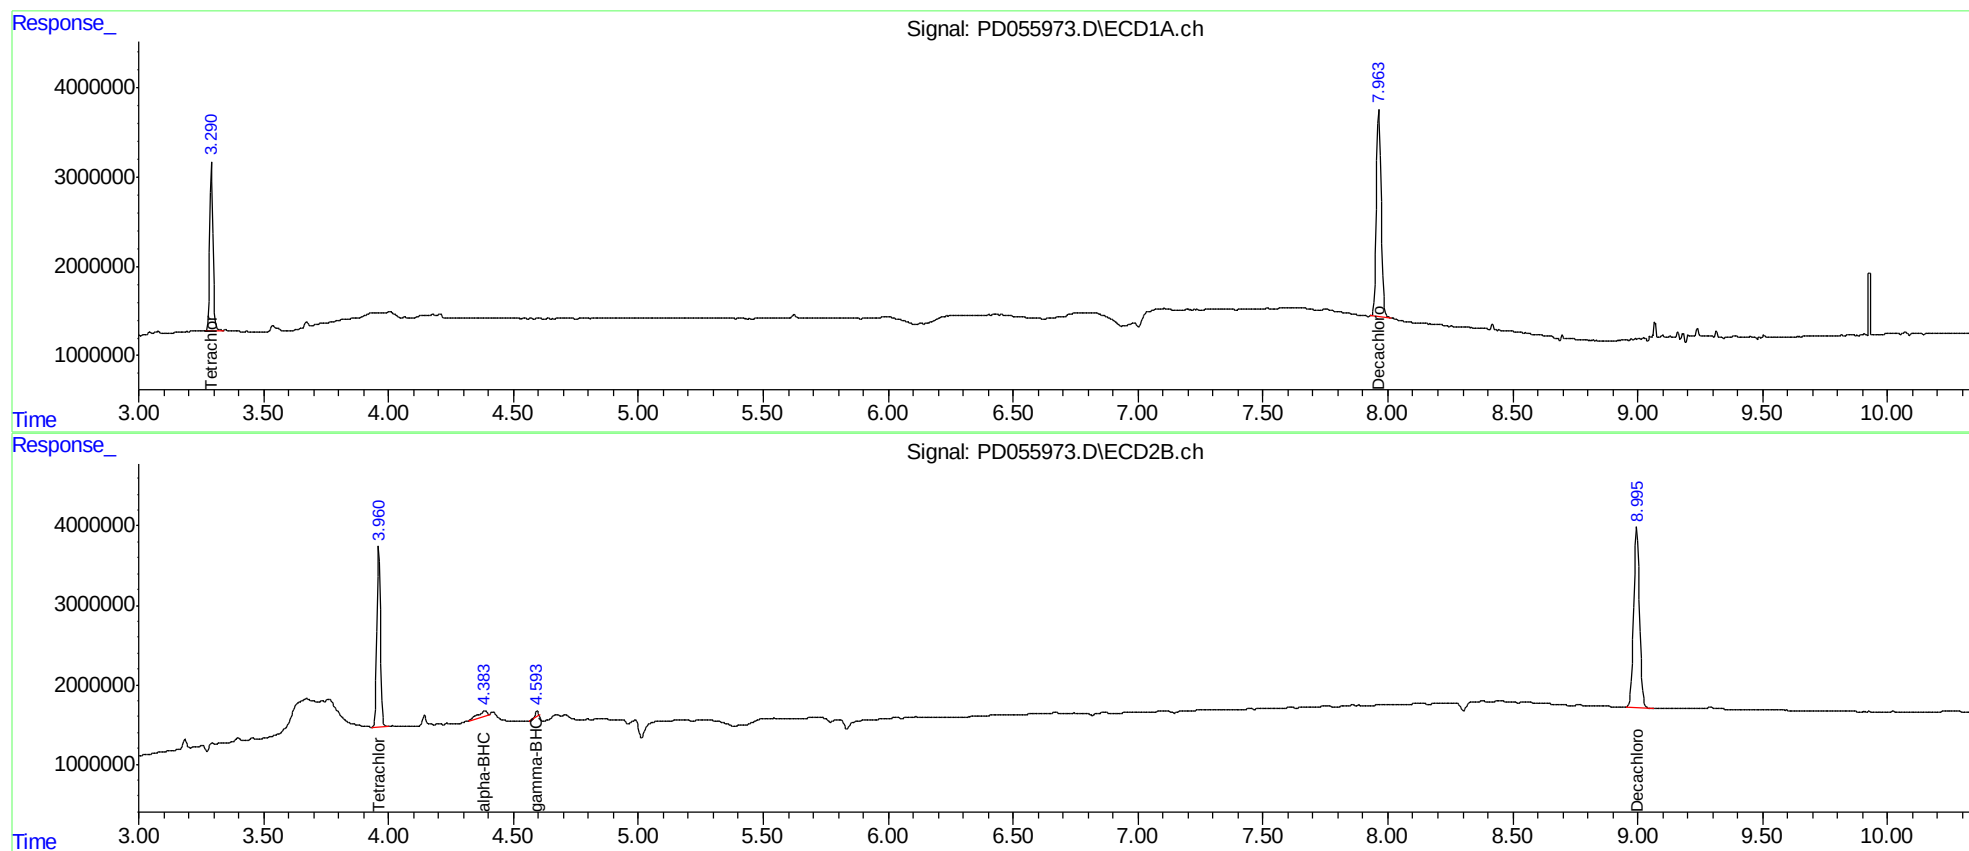


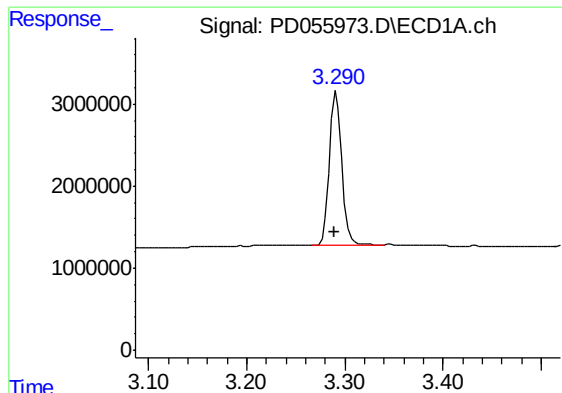

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.003 min
Response: 16802239
Conc: 22.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
A5460

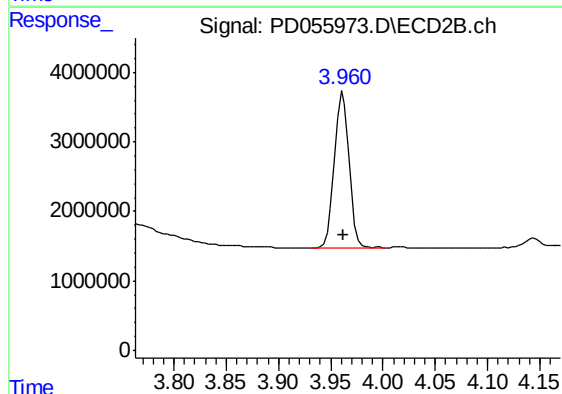


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 22157019
Conc: 21.14 ng/ml

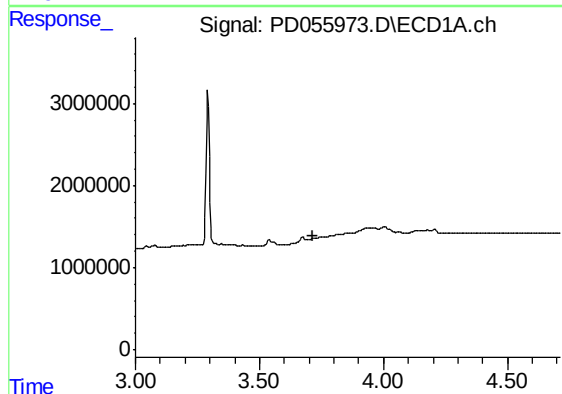


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.716 min
Response: 0
Conc: N.D.

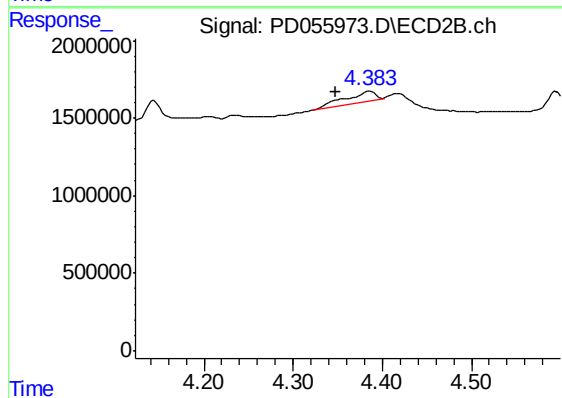

#2 alpha-BHC


R.T.: 4.386 min
Delta R.T.: 0.038 min
Response: 1616879
Conc: 1.13 ng/ml

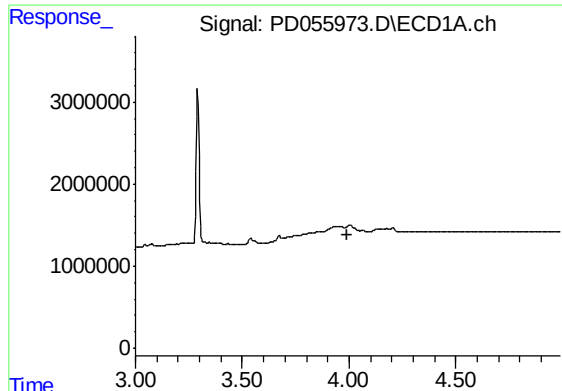

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.991 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
A5460

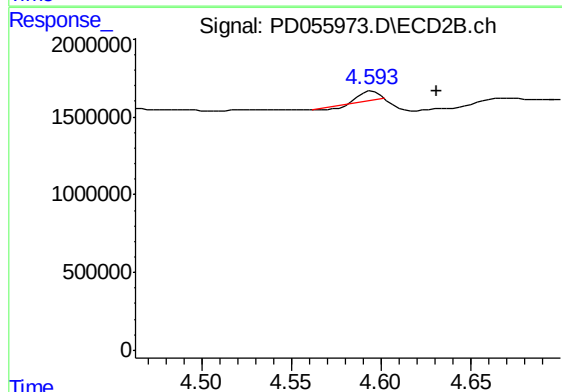


#3 gamma-BHC (Lindane)

R.T.: 4.595 min
Delta R.T.: -0.036 min
Response: 448078
Conc: 0.32 ng/ml

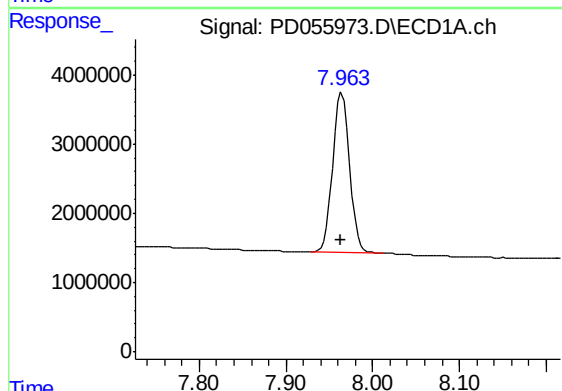

#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.001 min
Response: 31341658
Conc: 38.45 ng/ml

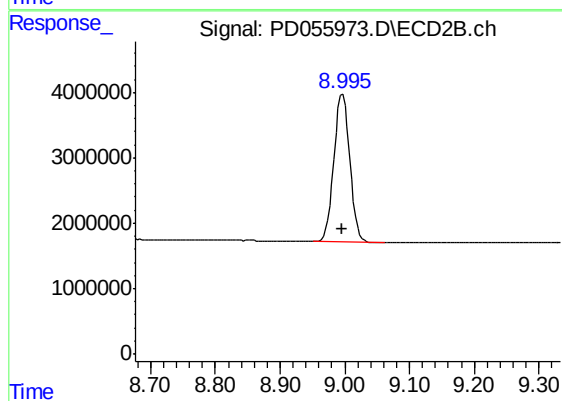

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 38238396
Conc: 33.67 ng/ml