

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
 Data File : PD055978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 10:38
 Operator : SG\AJ
 Sample : K5629-02MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AG1MS

Manual Integrations
 APPROVED

Ankita
 11/15/2019 11:23:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:55:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.961	17351790	22553324	23.050	21.521
27)	SA Decachlor...	7.961	8.995	31536960	39598732	38.690	34.871
Target Compounds							
3)	MA gamma-BHC...	3.991	4.631	59478836	76715932	58.150	54.452
4)	MA Heptachlor	4.276	5.137	52710888	75607990	55.672	51.988
5)	MB Aldrin	4.515	5.440	52723520	71533861	56.908	52.134
8)	B Heptachlo...	4.952	5.819	3063090	8077735	3.431	5.986 #
9)	A Endosulfan I	5.269	6.156	2782571	3487906	3.320m	2.679m
10)	B trans-Chl...	5.172	6.054	1702148	3534914	1.877m	2.478m#
11)	B cis-Chlor...	5.229	6.128	3247367	4604088	3.667m	3.280m
13)	MA Dieldrin	5.522	6.434	130.4E6	182.5E6	138.604	129.107
14)	MA Endrin	5.775	6.651	95355366	129.3E6	118.863	112.335
15)	B Endosulfa...	6.043	6.861	455837	1856459	0.541m	1.434m#
17)	MA 4,4'-DDT	6.145	7.071	79377862	115.5E6	122.492	106.203
21)	B Endrin ke...	6.911	7.673	4024338	6315981	4.544	4.788

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
Data File : PD055978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 10:38
Operator : SG\AJ
Sample : K5629-02MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:55:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

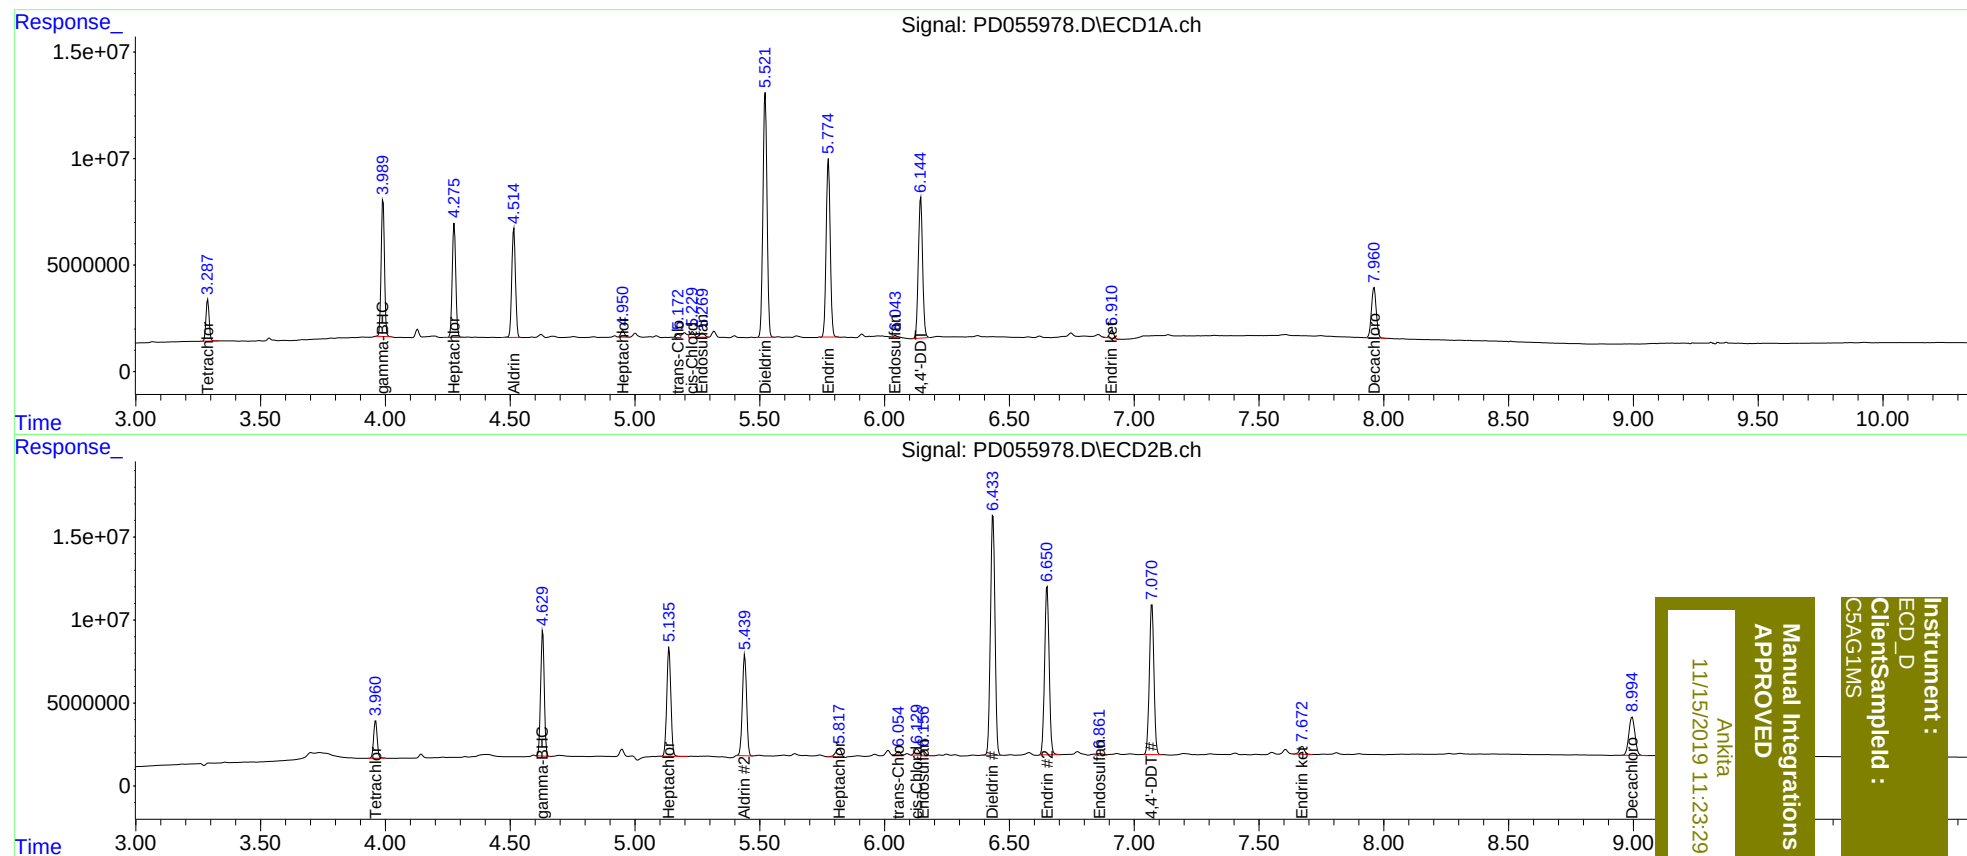

Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

Instrument :
ECD_D
Client Sampled :
CSAG1MS

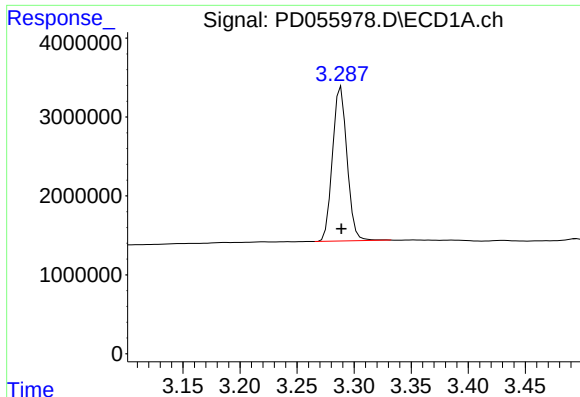


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 17351790
Conc: 23.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

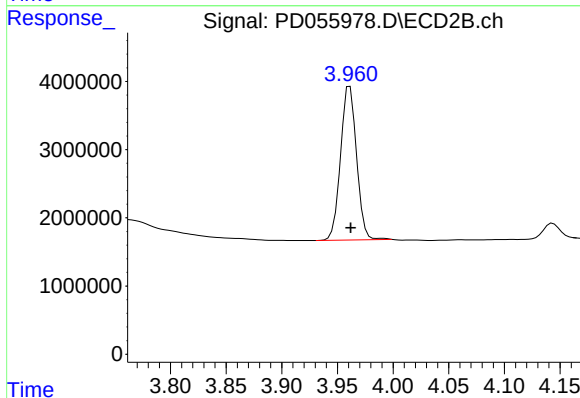


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 22553324
Conc: 21.52 ng/ml

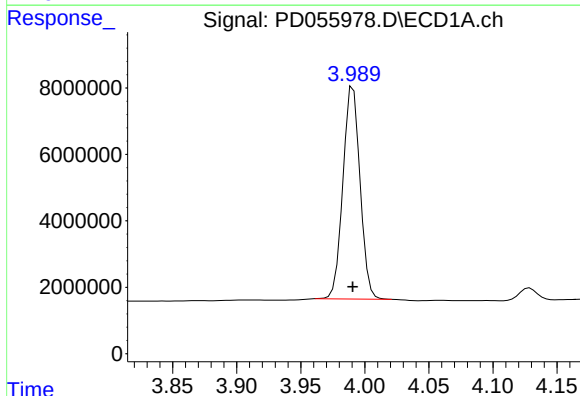


#3 gamma-BHC (Lindane)

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 59478836
Conc: 58.15 ng/ml

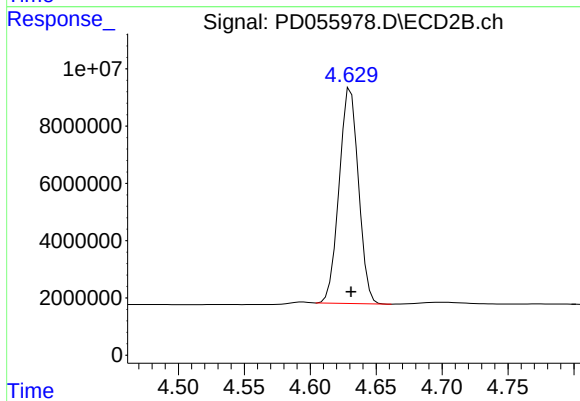

#3 gamma-BHC (Lindane)

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 76715932
Conc: 54.45 ng/ml

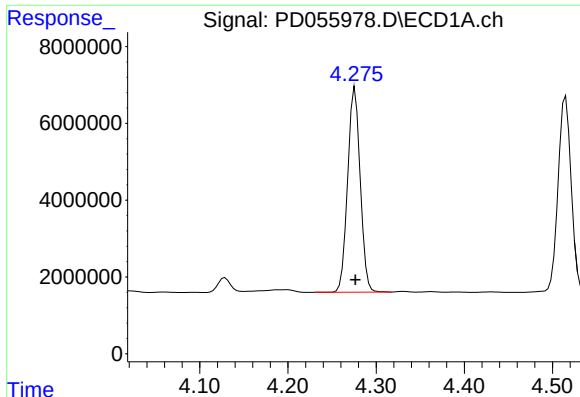


#4 Heptachlor

R.T.: 4.276 min
Delta R.T.: 0.000 min
Response: 52710888
Conc: 55.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

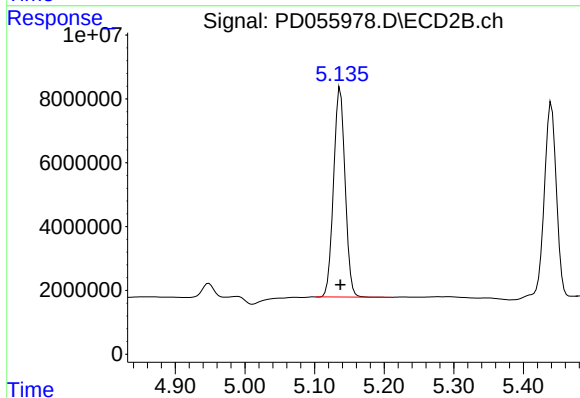


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 75607990
Conc: 51.99 ng/ml

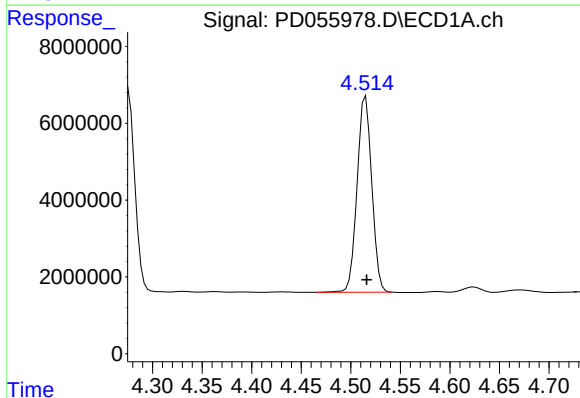


#5 Aldrin

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 52723520
Conc: 56.91 ng/ml

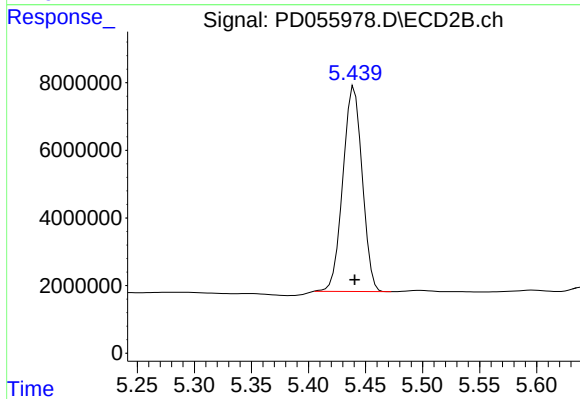

#5 Aldrin

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 71533861
Conc: 52.13 ng/ml

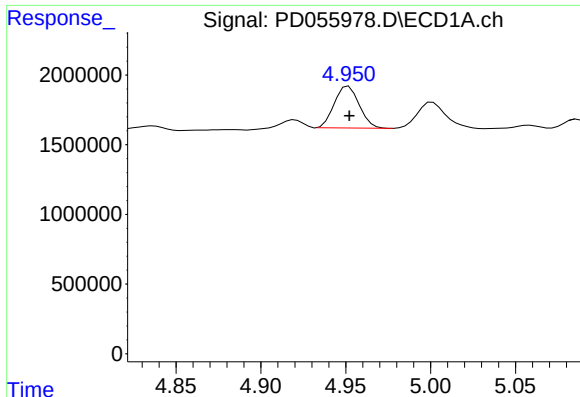


#8 Heptachlor epoxide

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 3063090
Conc: 3.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

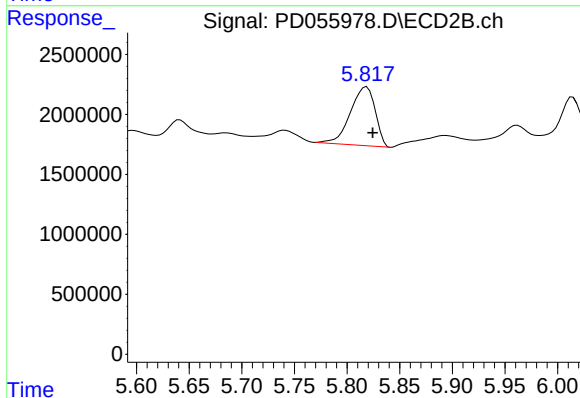


#8 Heptachlor epoxide

R.T.: 5.819 min
Delta R.T.: -0.006 min
Response: 8077735
Conc: 5.99 ng/ml

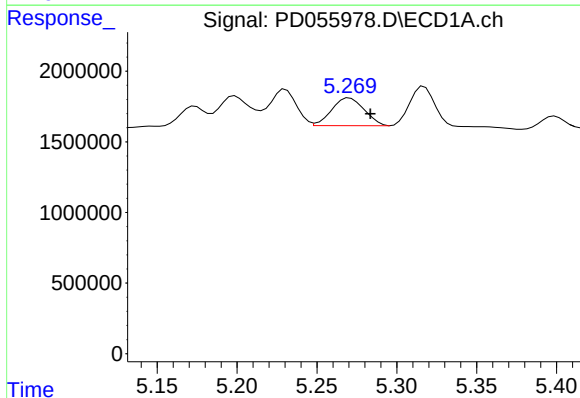


#9 Endosulfan I

R.T.: 5.269 min
Delta R.T.: -0.014 min
Response: 2782571
Conc: 3.32 ng/ml m

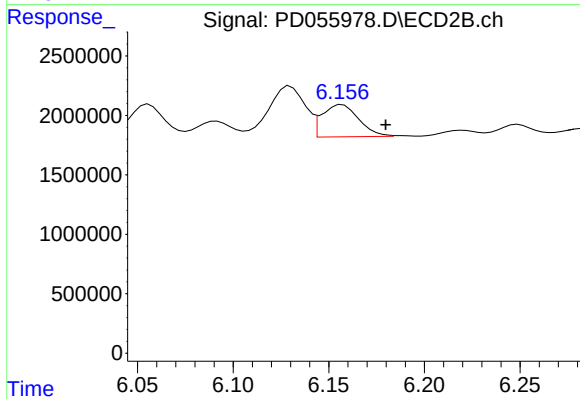

#9 Endosulfan I

R.T.: 6.156 min
Delta R.T.: -0.024 min
Response: 3487906
Conc: 2.68 ng/ml m

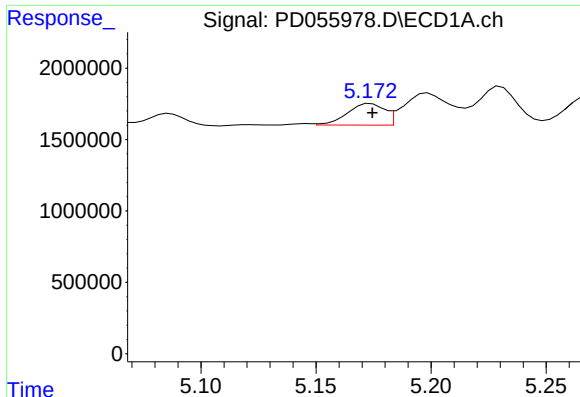


#10 trans-Chlordane

R.T.: 5.172 min
Delta R.T.: -0.002 min
Response: 1702148
Conc: 1.88 ng/ml m

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

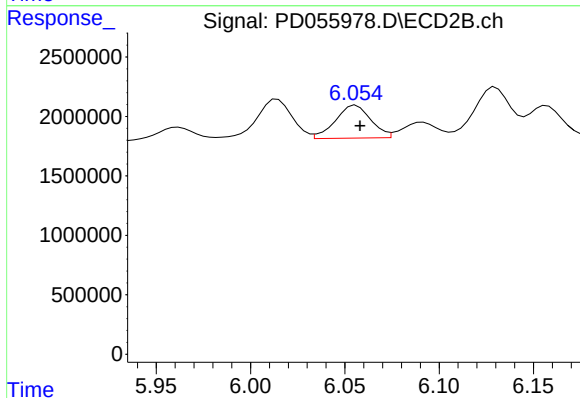


#10 trans-Chlordane

R.T.: 6.054 min
Delta R.T.: -0.003 min
Response: 3534914
Conc: 2.48 ng/ml m

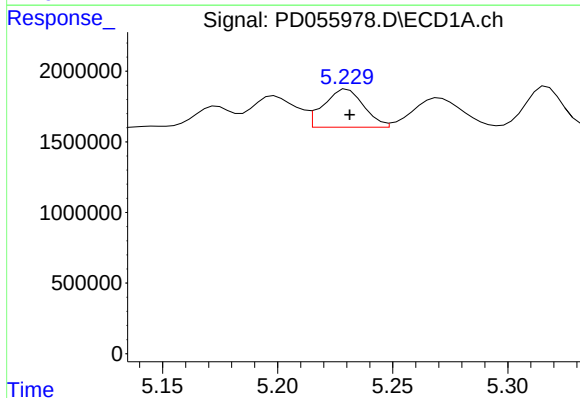


#11 cis-Chlordane

R.T.: 5.229 min
Delta R.T.: -0.002 min
Response: 3247367
Conc: 3.67 ng/ml m

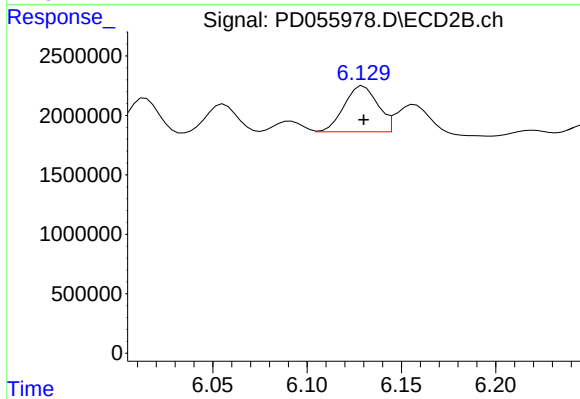

#11 cis-Chlordane

R.T.: 6.128 min
Delta R.T.: -0.002 min
Response: 4604088
Conc: 3.28 ng/ml m

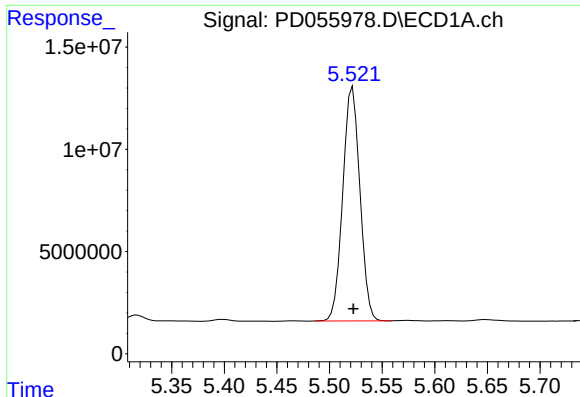


#13 Dieldrin

R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 130371475
Conc: 138.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

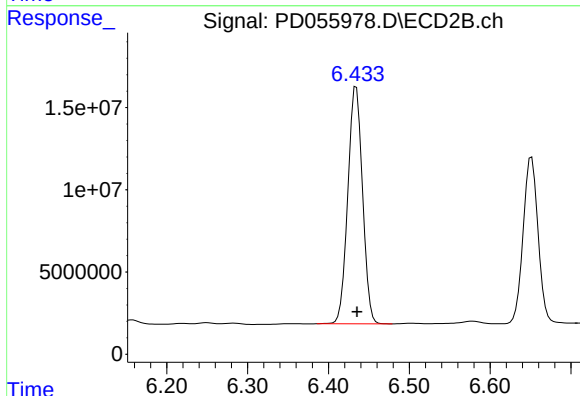


#13 Dieldrin

R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 182503014
Conc: 129.11 ng/ml

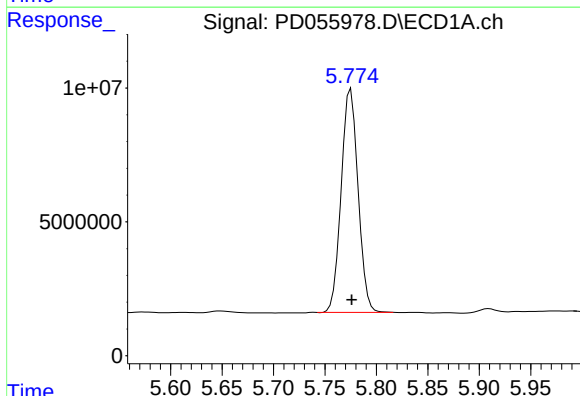


#14 Endrin

R.T.: 5.775 min
Delta R.T.: -0.001 min
Response: 95355366
Conc: 118.86 ng/ml

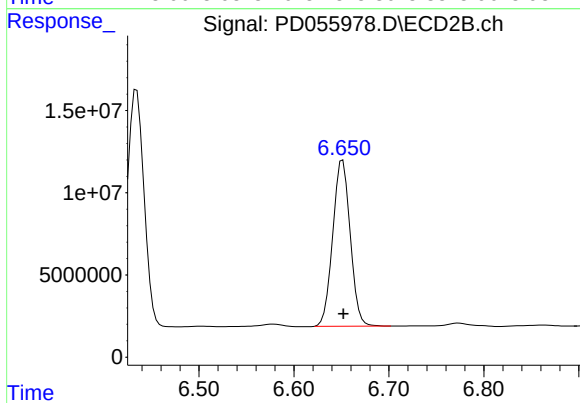

#14 Endrin

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 129329877
Conc: 112.33 ng/ml

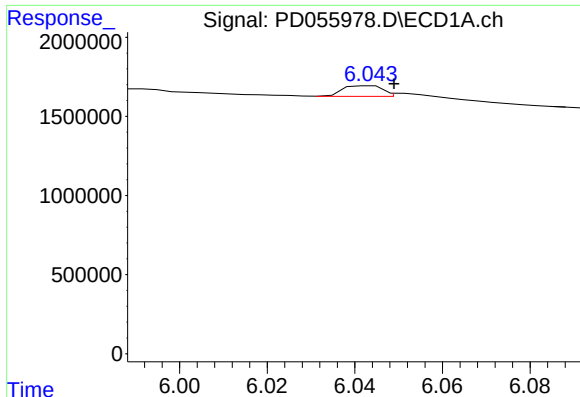


#15 Endosulfan II

R.T.: 6.043 min
Delta R.T.: -0.006 min
Response: 455837
Conc: 0.54 ng/ml m

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

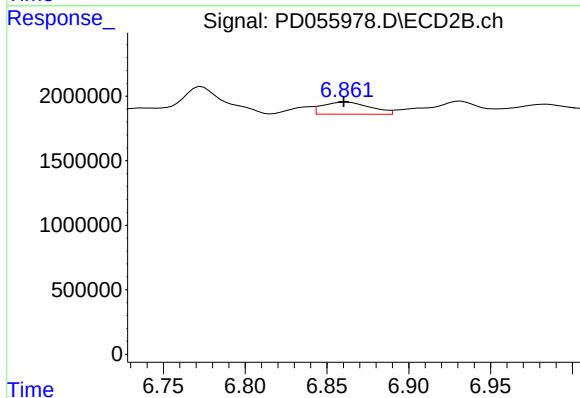


#15 Endosulfan II

R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 1856459
Conc: 1.43 ng/ml m

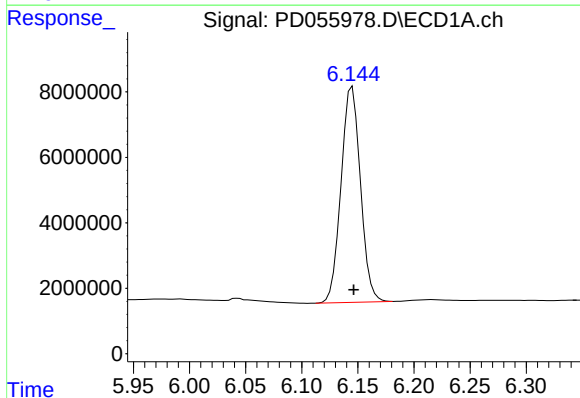


#17 4,4'-DDT

R.T.: 6.145 min
Delta R.T.: -0.001 min
Response: 79377862
Conc: 122.49 ng/ml

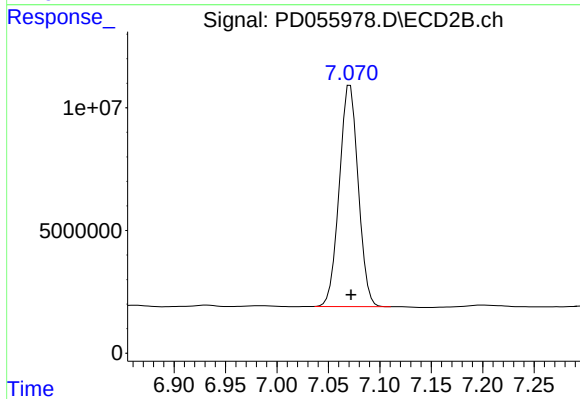

#17 4,4'-DDT

R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 115483325
Conc: 106.20 ng/ml

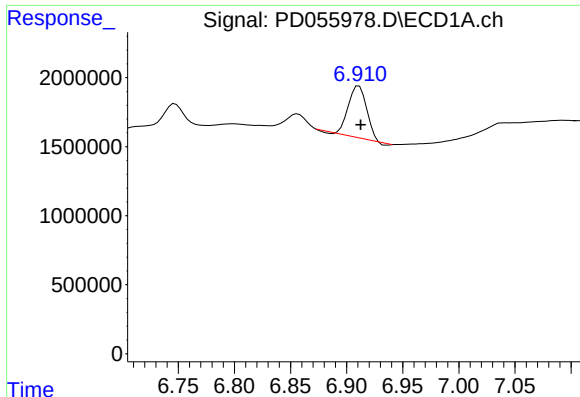


#21 Endrin ketone

R.T.: 6.911 min
Delta R.T.: -0.002 min
Response: 4024338
Conc: 4.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AG1MS


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:29 AM

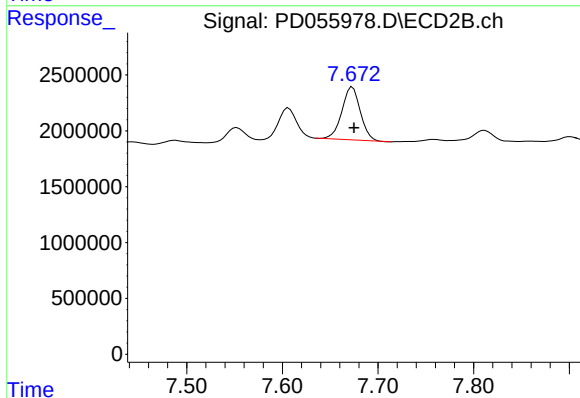


#21 Endrin ketone

R.T.: 7.673 min
Delta R.T.: -0.002 min
Response: 6315981
Conc: 4.79 ng/ml

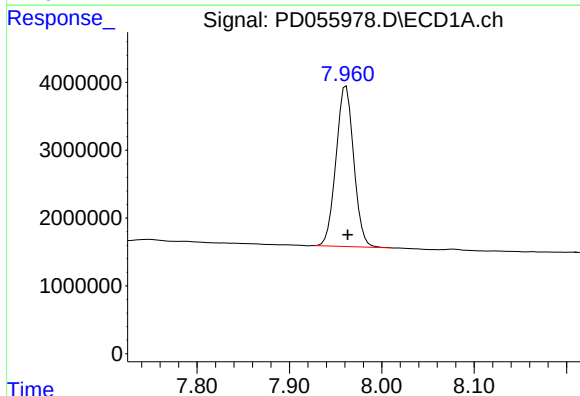

#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.002 min
Response: 31536960
Conc: 38.69 ng/ml

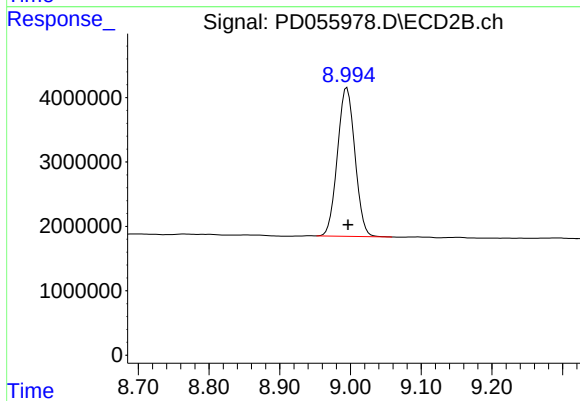

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.002 min
Response: 39598732
Conc: 34.87 ng/ml