

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
 Data File : PD055987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 13:24
 Operator : SG\AJ
 Sample : K5776-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AS8

Manual Integrations
 APPROVED

Ankita
 11/15/2019 11:23:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:57:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	9103274	11042674	12.093	10.537
2)	SA Decachlor...	7.961	8.993	16780394	22687618	20.587	19.979m
Target Compounds							
3)	MA gamma-BHC...	3.997	4.610	3005252	3625721	2.938	2.574m


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111419\
Data File : PD055987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 13:24
Operator : SG\AJ
Sample : K5776-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:57:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

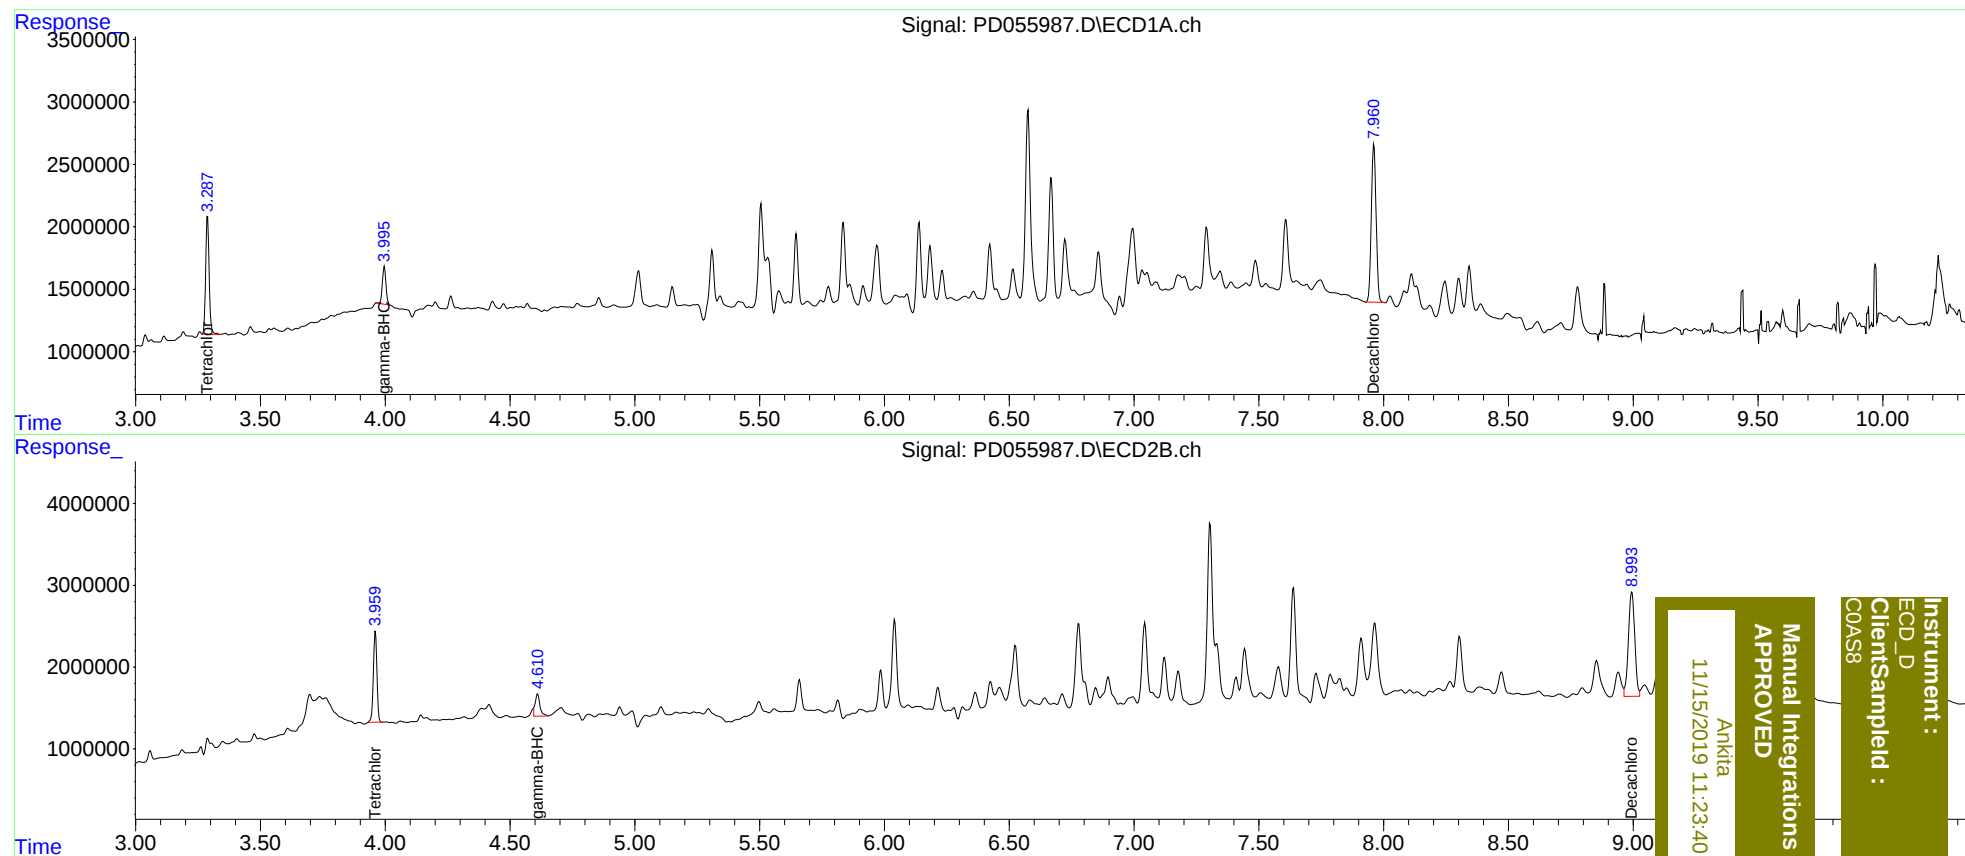

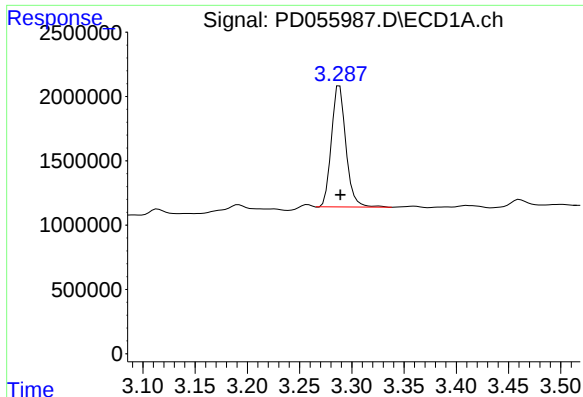


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 9103274
Conc: 12.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS8


Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:40 AM

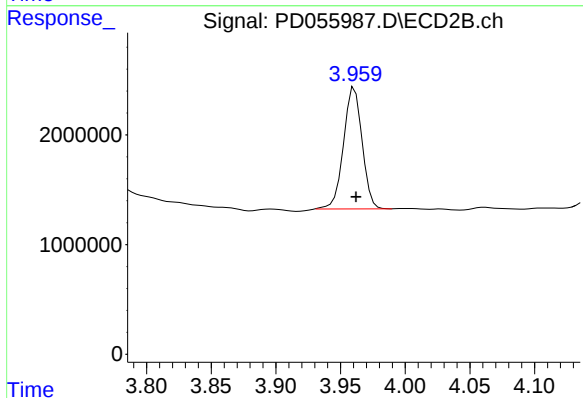


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 11042674
Conc: 10.54 ng/ml

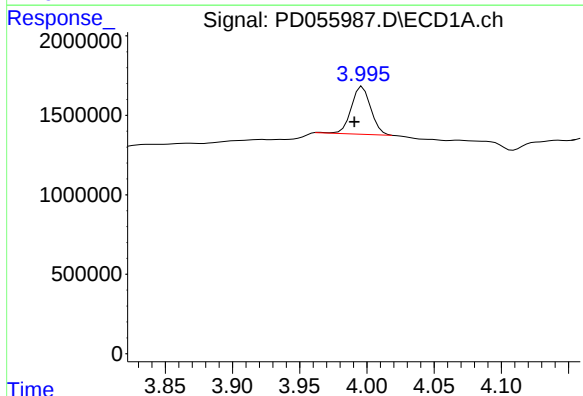


#3 gamma-BHC (Lindane)

R.T.: 3.997 min
Delta R.T.: 0.006 min
Response: 3005252
Conc: 2.94 ng/ml

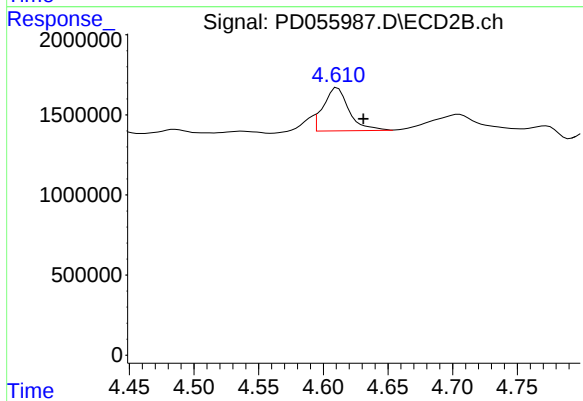

#3 gamma-BHC (Lindane)

R.T.: 4.610 min
Delta R.T.: -0.021 min
Response: 3625721
Conc: 2.57 ng/ml m

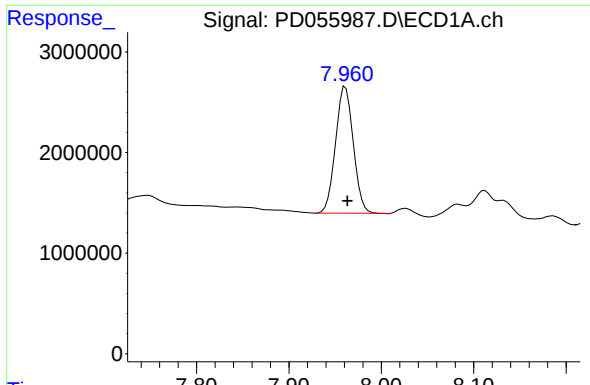


#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.002 min
Response: 16780394
Conc: 20.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS8

Manual Integrations
APPROVED

Ankita
11/15/2019 11:23:40 AM

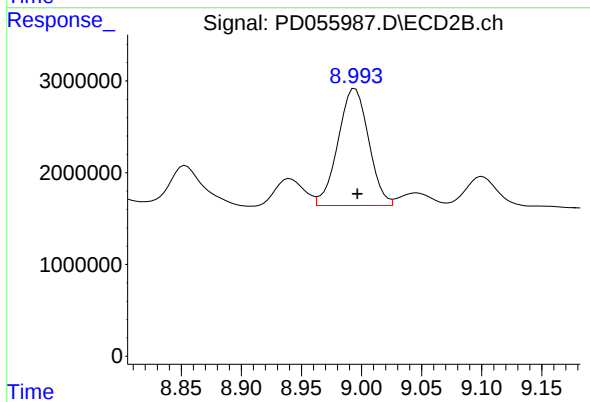

#27 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: -0.003 min
Response: 22687618
Conc: 19.98 ng/ml m