

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
 Data File : PD072975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 15:52
 Operator : AR\AJ
 Sample : PB148936BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS936

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/15/2022
 Supervised By : Ankita Jodhani 11/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:34:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.461	39375843	864.2E6	16.872	19.825
27)	SA Decachlor...	7.828	8.910	81047357	464.7E6	35.681	44.151
Target Compounds							
2)	A alpha-BHC	3.202	3.924	13250704	299.6E6	3.754	5.295 #
3)	MA gamma-BHC...	3.533	4.258	13061535	252.4E6	4.018	5.639 #
4)	MA Heptachlor	3.865	4.824	13348682	174.1E6	4.063	5.655 #
5)	MB Aldrin	4.142	5.162	13537284	152.5E6	4.184m	5.814 #
6)	B beta-BHC	3.834	4.473	6399286	94005594	4.196	5.315 #
7)	B delta-BHC	4.062	4.716	13031121	192.5E6	3.747m	5.371 #
8)	B Heptachlo...	4.648	5.593	12644636	134.9E6	4.220	6.096m#
9)	A Endosulfan I	5.017	5.979	12214902	108.6E6	4.414	5.628 #
10)	B trans-Chl...	4.897	5.848	13100854	114.4E6	4.431	5.542 #
11)	B cis-Chlor...	4.960	5.923	13949442	114.8E6	4.617	5.505
12)	B 4,4'-DDE	5.148	6.097	24037571	206.8E6	8.332	10.806 #
13)	MA Dieldrin	5.283	6.256	24003815	236.4E6	8.007	11.916 #
14)	MA Endrin	5.559	6.487	21382701	120.8E6	7.998m	7.312
15)	B Endosulfa...	5.858	6.717	21865778	179.5E6	8.421	11.272 #
16)	A 4,4'-DDD	5.706	6.621	18916673	168.9E6	7.999	11.515 #
17)	MA 4,4'-DDT	5.955	6.929	17818070	157.5E6	7.710	11.069 #
18)	B Endrin al...	6.040	6.849	18556324	142.7E6	8.893	11.441 #
19)	B Endosulfa...	6.263	7.081	20685582	153.3E6	8.500	11.171 #
20)	A Methoxychlor	6.539	7.407	56423922	370.2E6	43.931	58.440m#
21)	B Endrin ke...	6.772	7.570	24323105	179.4E6	8.606m	11.937 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
Data File : PD072975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 15:52
Operator : AR\AJ
Sample : PB148936BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:34:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

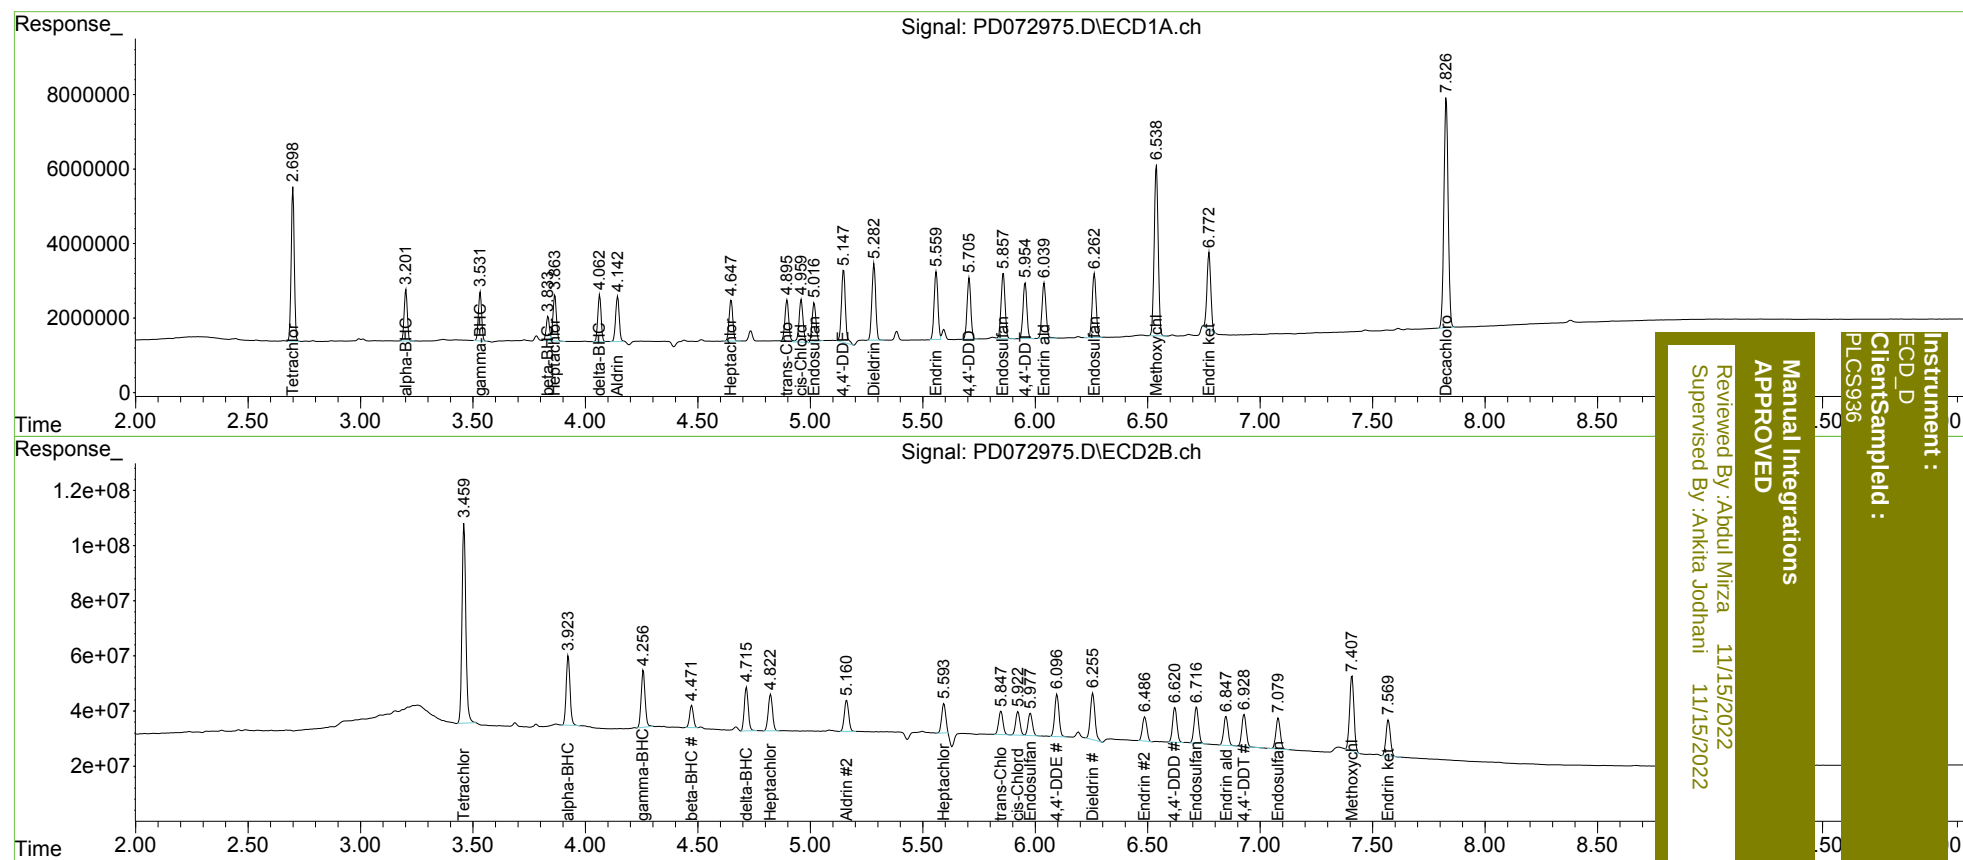

Instrument :
ECD_D
ClientSampled :
PLCS936

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/15/2022
Supervised By :Ankita Jodhani 11/15/2022