

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
 Data File : PD072979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 17:16
 Operator : AR\AJ
 Sample : N5541-02MS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0KX8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:35:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.462	38596354	1048.5E6	16.538	24.053 #
2)	SA Decachlor...	7.827	8.910	65861404	368.3E6	28.995	34.990
Target Compounds							
2)	A alpha-BHC	3.203	3.924	133.1E6	2201.8E6	37.725	38.910
3)	MA gamma-BHC...	3.533	4.258	132.4E6	1827.6E6	40.730	40.826
4)	MA Heptachlor	3.865	4.824	130.4E6	1188.0E6	39.678	38.586
5)	MB Aldrin	4.144	5.162	130.9E6	1075.1E6	40.460	40.985
6)	B beta-BHC	3.835	4.473	61012899	755.6E6	40.005	42.721
7)	B delta-BHC	4.064	4.717	11213603	152.0E6	3.224	4.240 #
8)	B Heptachlo...	4.648	5.594	126.0E6	971.1E6	42.065	43.873
9)	A Endosulfan I	5.017	5.979	115.8E6	867.3E6	41.826	44.949
10)	B trans-Chl...	4.897	5.848	125.6E6	904.1E6	42.478	43.804
11)	B cis-Chlor...	4.960	5.924	121.0E6	890.1E6	40.048	42.696
12)	B 4,4'-DDE	5.149	6.097	250.7E6	1770.2E6	86.901	92.515
13)	MA Dieldrin	5.284	6.256	264.3E6	1840.4E6	88.161	92.783
14)	MA Endrin	5.560	6.487	231.9E6	1507.8E6	86.751	91.303
15)	B Endosulfa...	5.859	6.717	216.4E6	1451.0E6	83.331	91.112
16)	A 4,4'-DDD	5.707	6.622	194.5E6	1340.3E6	82.249	91.375
17)	MA 4,4'-DDT	5.955	6.929	185.3E6	1290.9E6	80.190	90.717
18)	B Endrin al...	6.040	6.848	157.5E6	1050.5E6	75.467	84.207
19)	B Endosulfa...	6.263	7.081	132.9E6	860.7E6	54.598	62.720
20)	A Methoxychlor	6.539	7.408	526.1E6	2969.0E6	409.644	468.651
21)	B Endrin ke...	6.773	7.570	245.0E6	1419.3E6	86.699	94.457

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
Data File : PD072979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 17:16
Operator : AR\AJ
Sample : N5541-02MS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:35:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

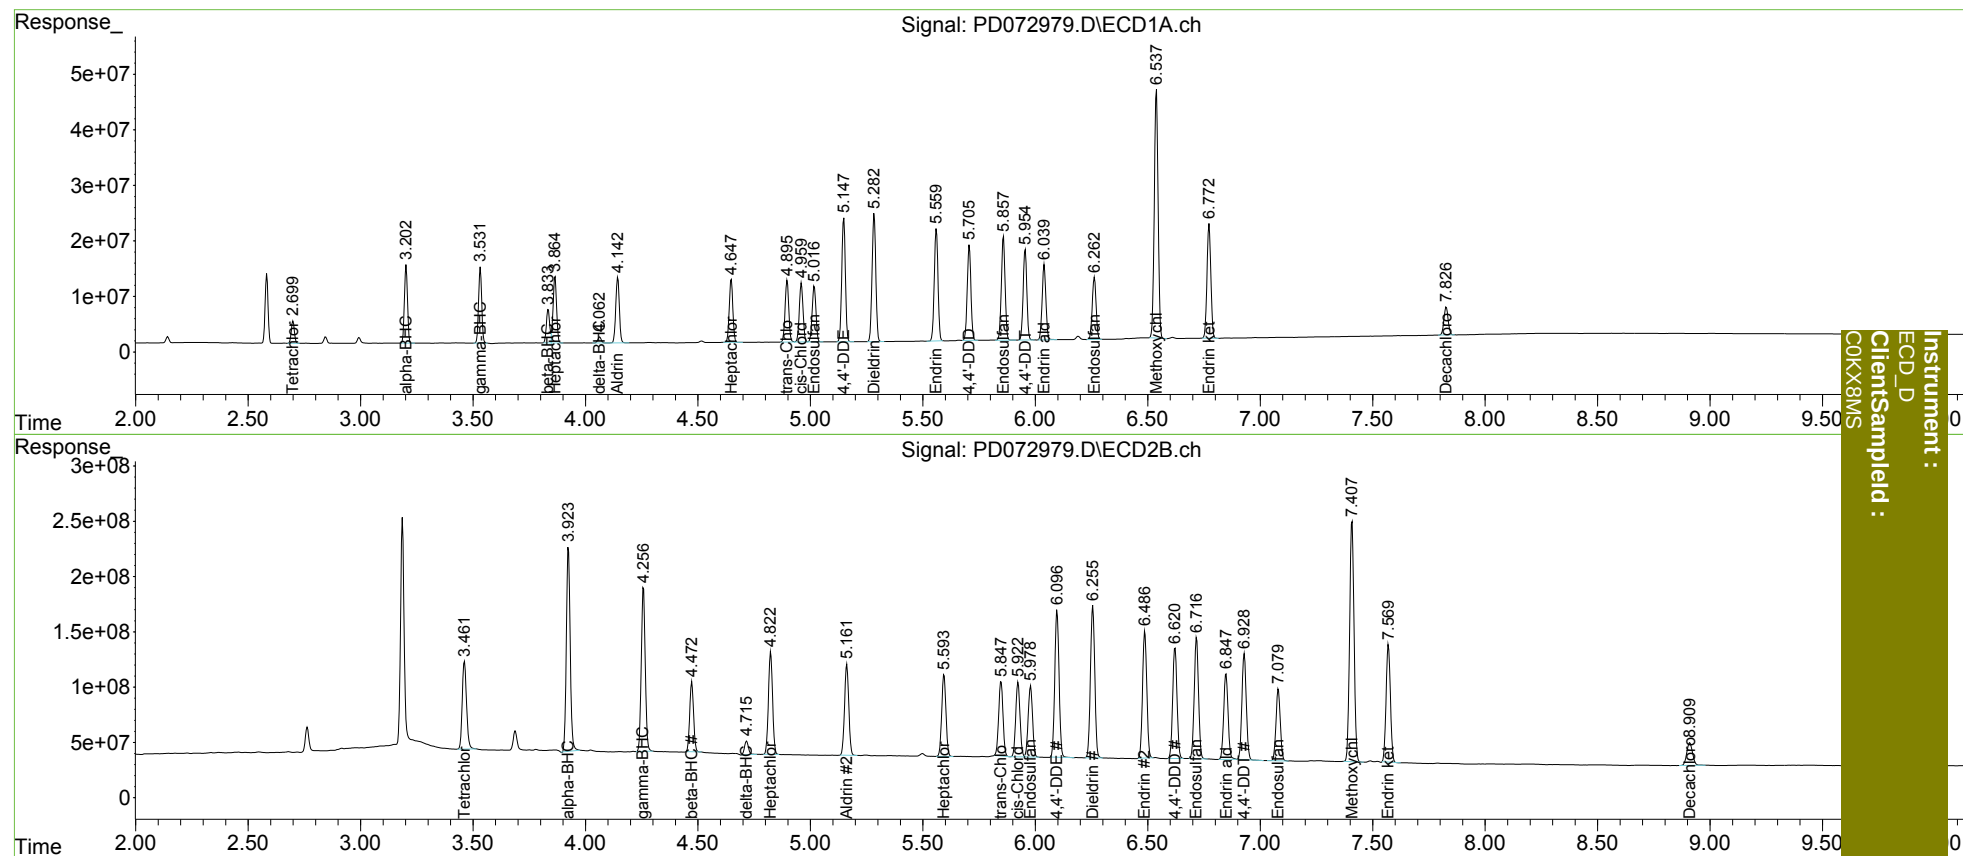

Instrument :
ECD_D
ClientSampled :
C0KX8MS