

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
 Data File : PD072980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 17:29
 Operator : AR\AJ
 Sample : N5541-03MSD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0KX8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:35:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.462	38553785	1072.2E6	16.519	24.596 #
27)	SA Decachlor...	7.828	8.911	67234815	374.4E6	29.600	35.566
Target Compounds							
2)	A alpha-BHC	3.203	3.924	133.0E6	2255.3E6	37.689	39.856
3)	MA gamma-BHC...	3.533	4.258	132.2E6	1873.9E6	40.661	41.861
4)	MA Heptachlor	3.865	4.824	130.8E6	1227.4E6	39.824	39.865
5)	MB Aldrin	4.144	5.162	132.6E6	1115.6E6	40.971	42.527
6)	B beta-BHC	3.835	4.473	60421018	778.7E6	39.617	44.030
7)	B delta-BHC	4.064	4.717	11408070	156.0E6	3.280	4.351 #
8)	B Heptachlo...	4.649	5.594	126.9E6	995.8E6	42.349	44.989
9)	A Endosulfan I	5.018	5.979	116.7E6	888.5E6	42.185	46.048
10)	B trans-Chl...	4.897	5.848	126.7E6	935.2E6	42.868	45.310
11)	B cis-Chlor...	4.961	5.923	122.8E6	915.6E6	40.647	43.920
12)	B 4,4'-DDE	5.148	6.097	253.4E6	1822.3E6	87.842	95.237
13)	MA Dieldrin	5.284	6.256	266.7E6	1883.5E6	88.960	94.957
14)	MA Endrin	5.561	6.487	232.8E6	1542.7E6	87.065	93.416
15)	B Endosulfa...	5.858	6.717	218.3E6	1480.9E6	84.071	92.991
16)	A 4,4'-DDD	5.707	6.621	197.0E6	1367.2E6	83.287	93.210
17)	MA 4,4'-DDT	5.956	6.929	186.0E6	1321.8E6	80.494	92.888
18)	B Endrin al...	6.040	6.848	159.1E6	1076.6E6	76.225	86.302
19)	B Endosulfa...	6.263	7.081	134.2E6	881.2E6	55.125	64.213
20)	A Methoxychlor	6.539	7.409	528.5E6	3024.6E6	411.474	477.435
21)	B Endrin ke...	6.773	7.570	246.4E6	1457.1E6	87.182	96.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
Data File : PD072980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 17:29
Operator : AR\AJ
Sample : N5541-03MSD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:35:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

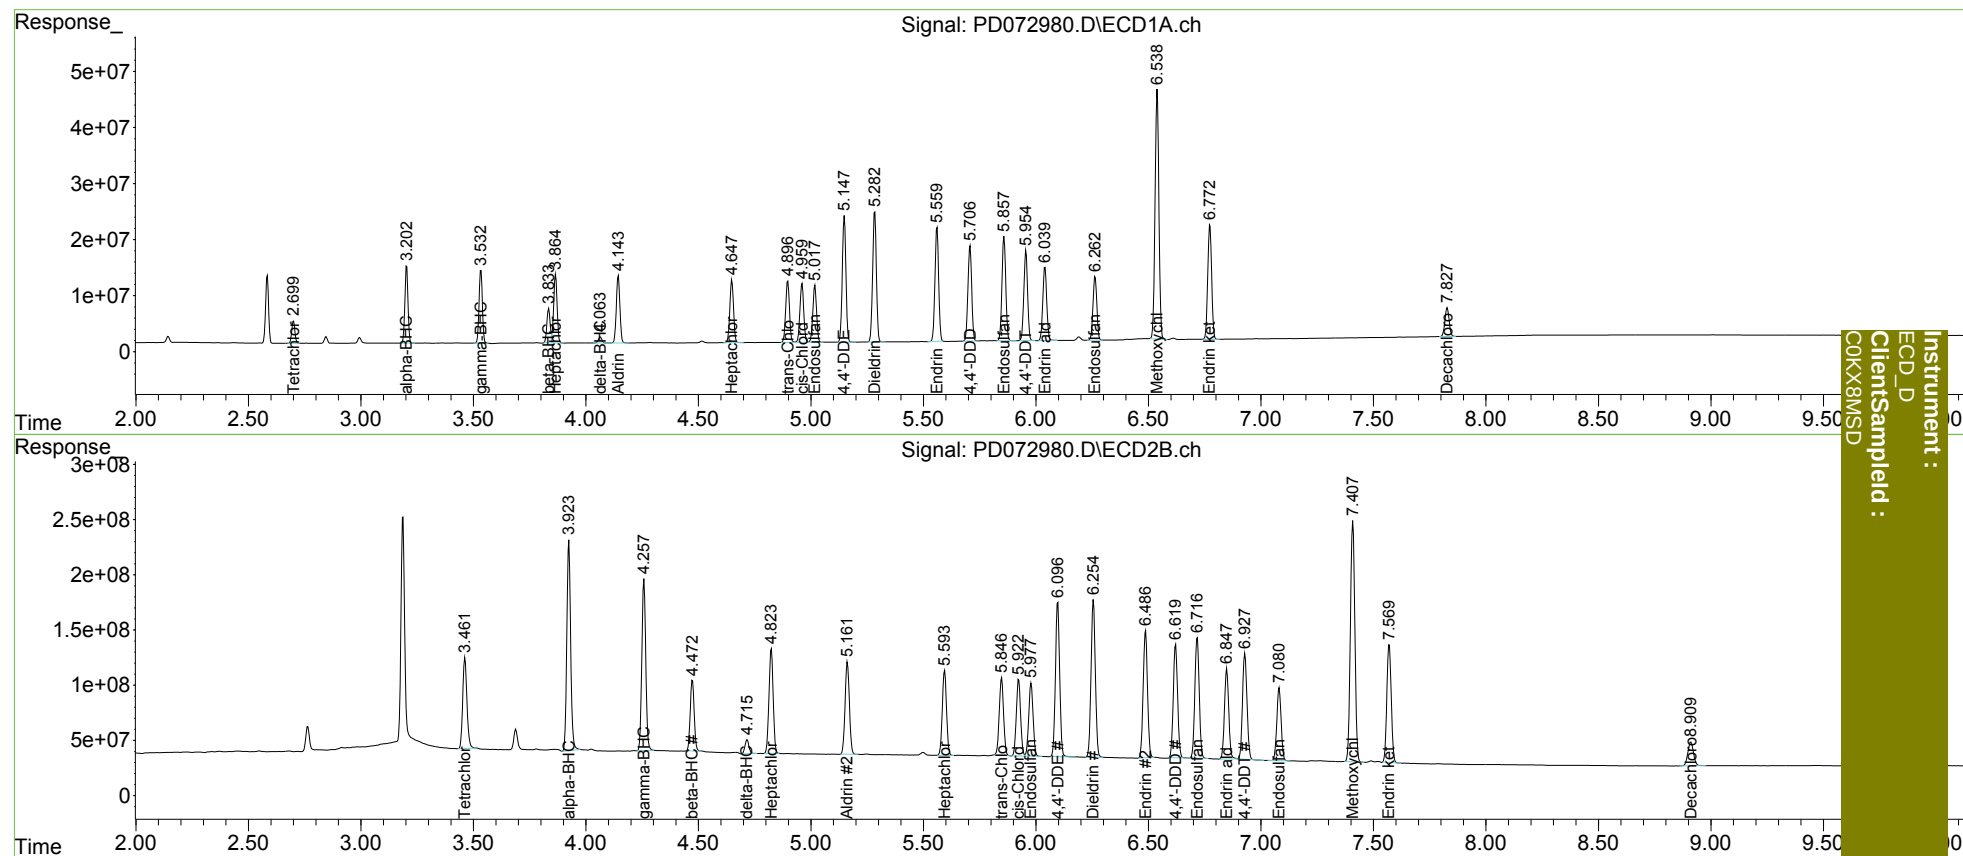

Instrument :
ECD_D
ClientSampled :
C0KX8MSD