

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
 Data File : PD072977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 16:49
 Operator : AR\AJ
 Sample : N5407-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4Y2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/15/2022
 Supervised By : Ankita Jodhani 11/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:34:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.704	3.457	47626743	1852.3E6	20.407m	42.494m#
2) SA Decachlor...	7.829	8.909	22556806	197.4E6	9.931m	18.752m#
Target Compounds						
16) A 4,4'-DDD	5.727	6.637	15793683	170.3E6	6.678m	11.609m#
18) B Endrin al...	6.024	6.849	42785756	51543845	20.504m	4.132 #
20) A Methoxychlor	6.536	7.409	18510932	86229990	14.412m	13.611m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111422\
Data File : PD072977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 16:49
Operator : AR\AJ
Sample : N5407-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:34:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

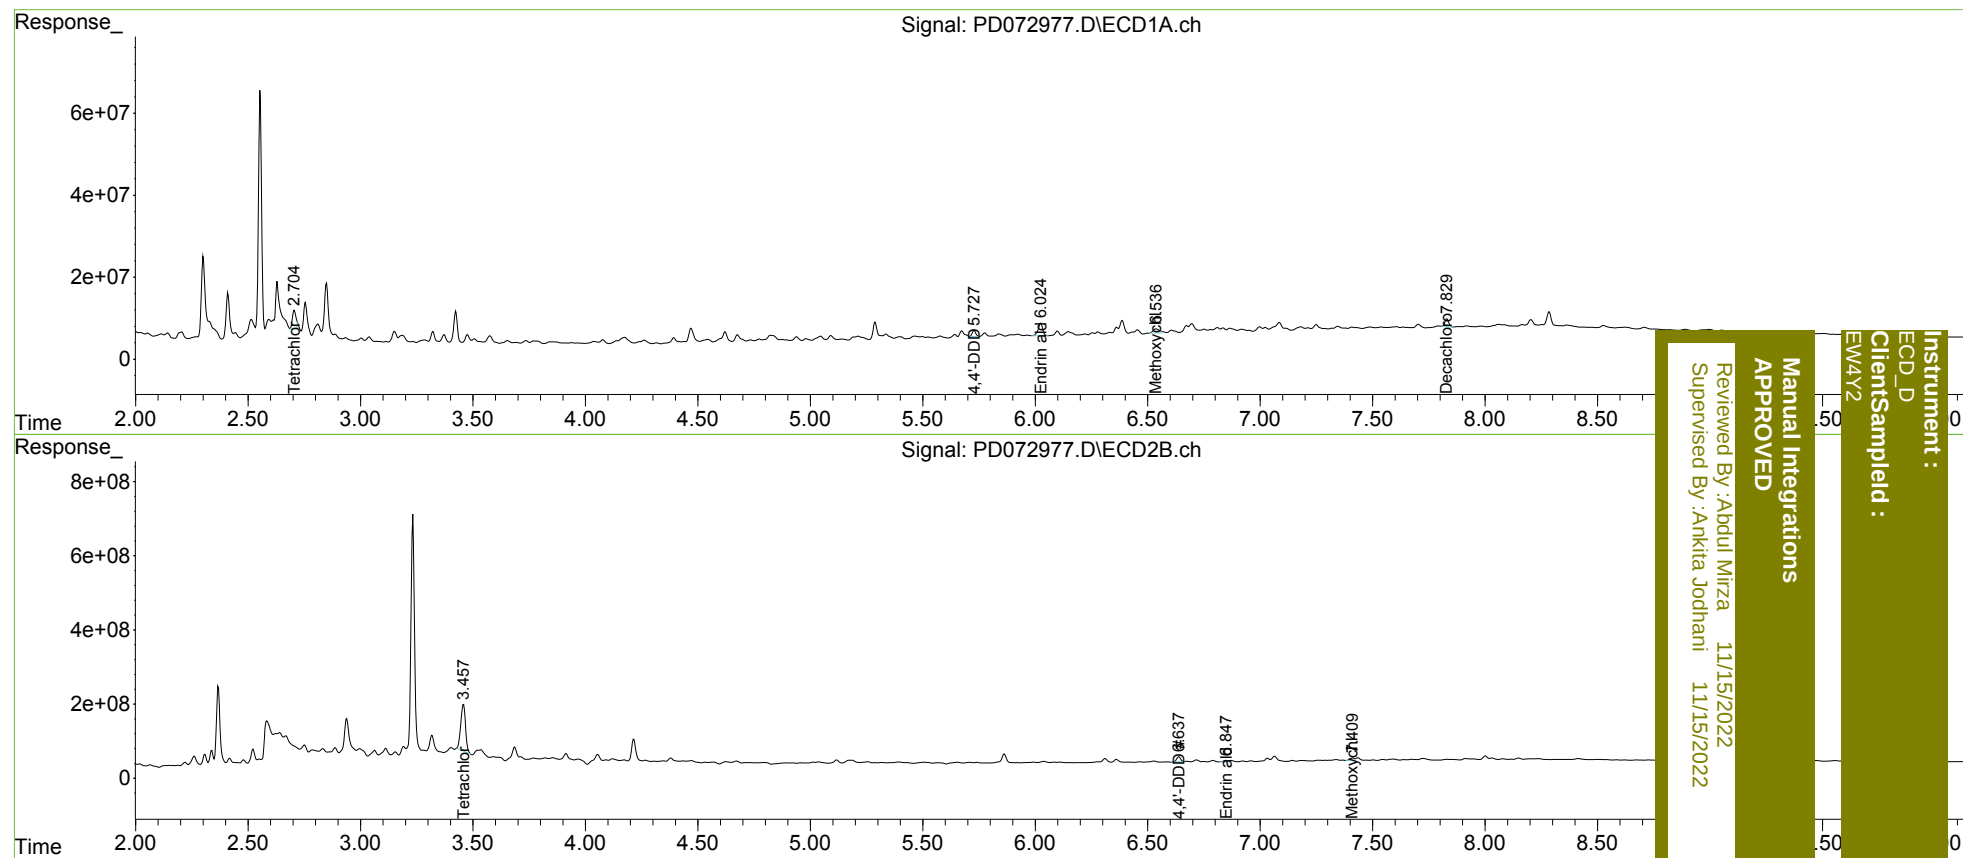

Reviewed By: Abdul Mirza 11/15/2022
Supervised By: Ankita Jodhani 11/15/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW4Y2