

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 14:32
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 02:05:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 02:04:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	15159674	109.6E6	10.181	10.578
27)	SA Decachlor...	9.087	8.089	45199169	253.2E6	20.794	21.697
Target Compounds							
2)	A alpha-BHC	4.006	3.399	26932219	167.3E6	9.559	10.334
3)	MA gamma-BHC...	4.337	3.736	26891382	157.3E6	9.653	10.387
4)	MA Heptachlor	4.938	4.093	27876255	165.8E6	9.853	10.586
9)	A Endosulfan I	6.083	5.258	23988716	138.9E6	10.041	10.477
13)	MA Dieldrin	6.356	5.525	51421847	294.1E6	19.414	20.979
14)	MA Endrin	6.583	5.801	42939207	270.5E6	19.460	21.183
16)	A 4,4'-DDD	6.714	5.942	37259848	236.2E6	19.392	21.029
17)	MA 4,4'-DDT	7.030	6.197	39037371	250.2E6	19.460	20.937
20)	A Methoxychlor	7.503	6.768	114.8E6	608.4E6	101.063	110.338


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 14:32
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 02:05:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 02:04:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

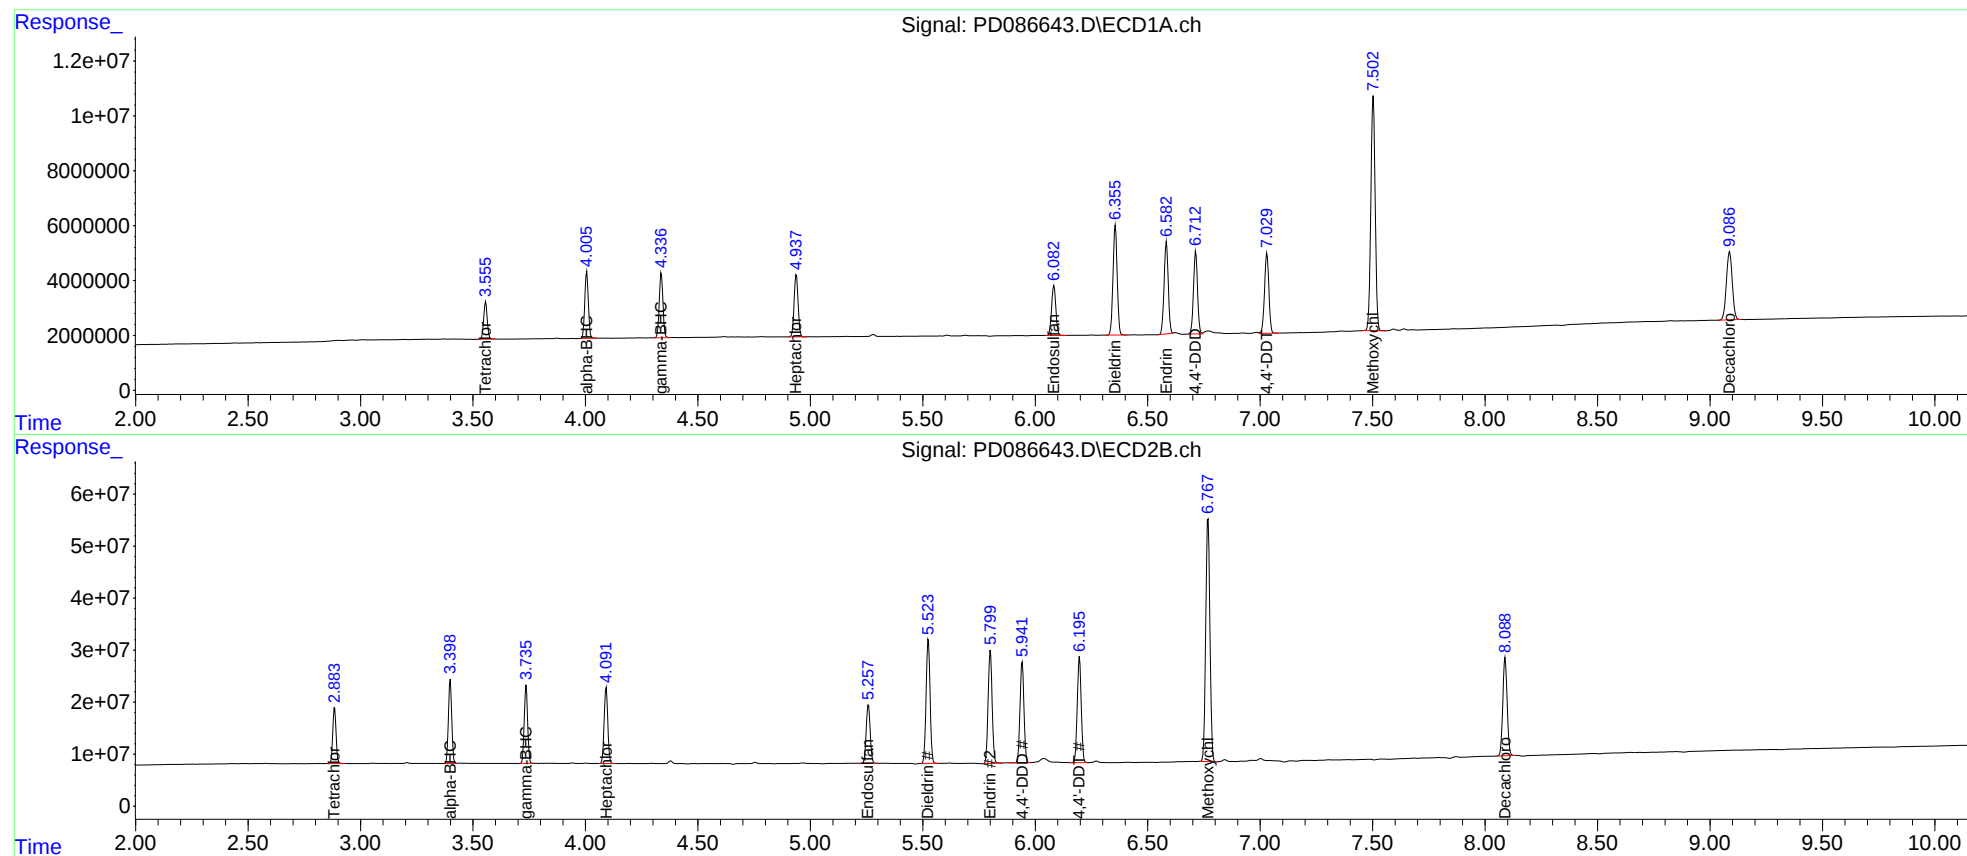

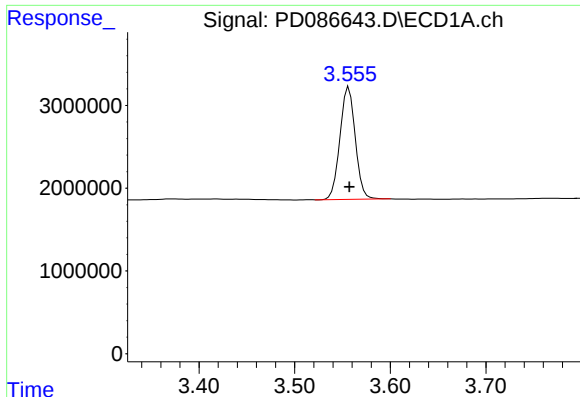


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 15159674
Conc: 10.18 ng/ml

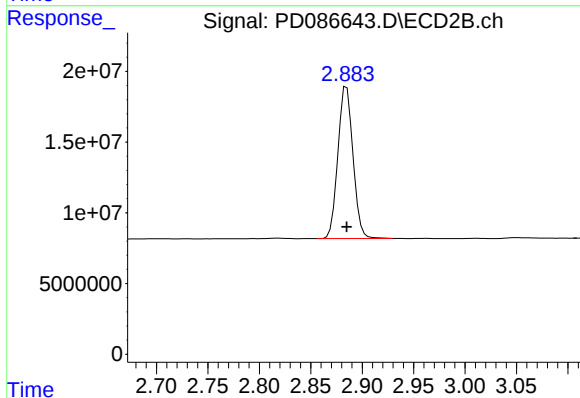


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 109612439
Conc: 10.58 ng/ml

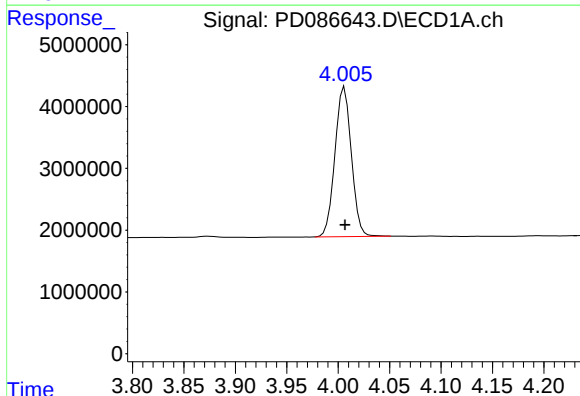


#2 alpha-BHC

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 26932219
Conc: 9.56 ng/ml

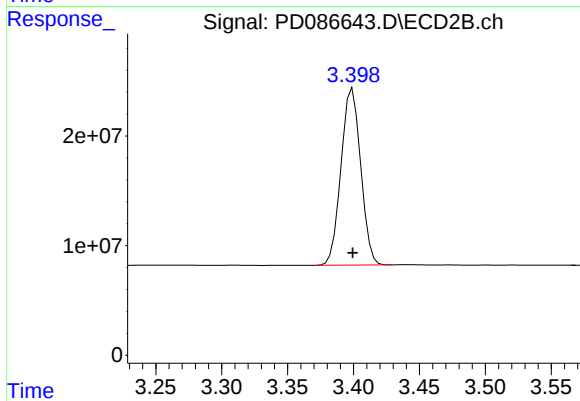


#2 alpha-BHC

R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 167290584
Conc: 10.33 ng/ml

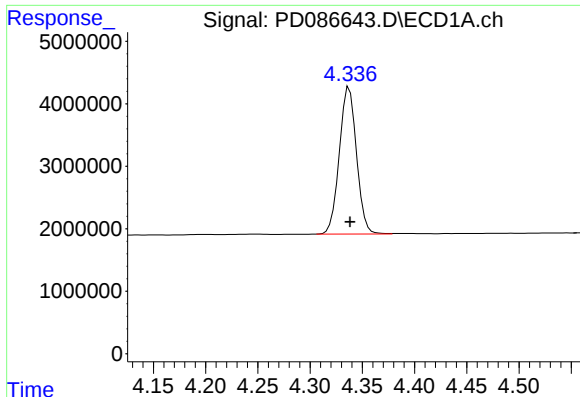


#3 gamma-BHC (Lindane)

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 26891382
Conc: 9.65 ng/ml

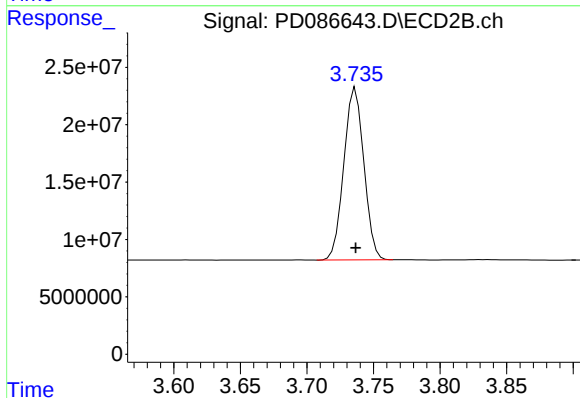


#3 gamma-BHC (Lindane)

R.T.: 3.736 min
Delta R.T.: 0.000 min
Response: 157257706
Conc: 10.39 ng/ml

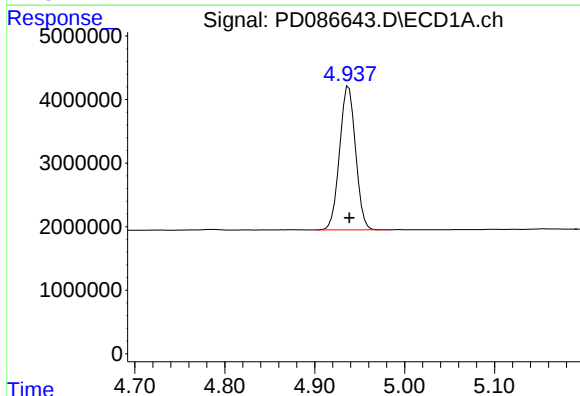


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 27876255
Conc: 9.85 ng/ml

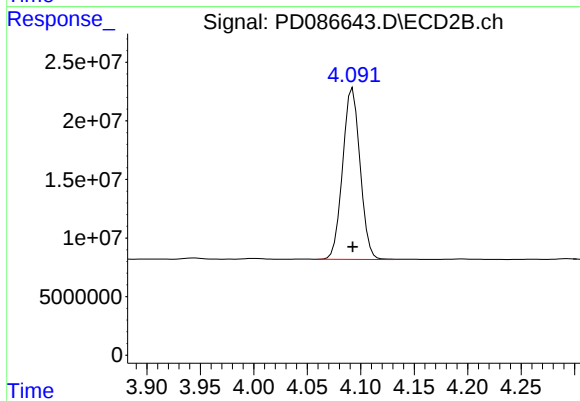


#4 Heptachlor

R.T.: 4.093 min
Delta R.T.: 0.000 min
Response: 165777442
Conc: 10.59 ng/ml

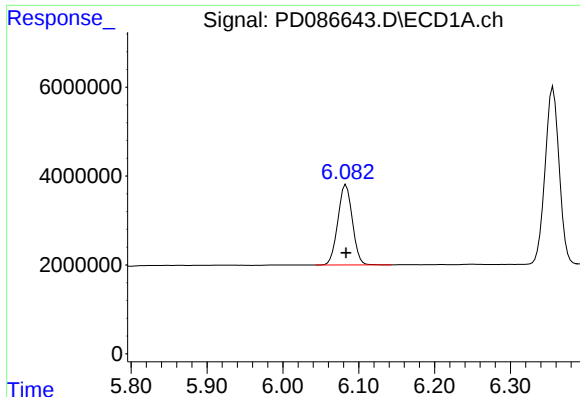


#9 Endosulfan I

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 23988716
Conc: 10.04 ng/ml

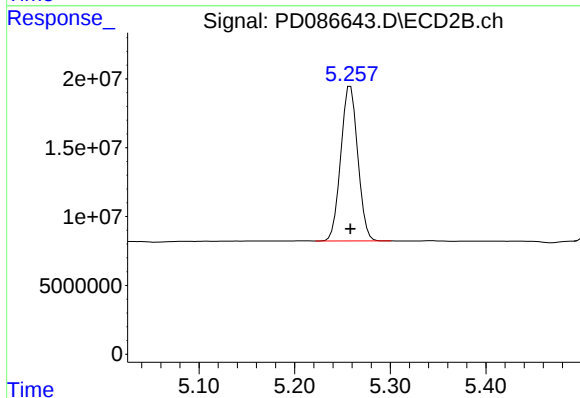


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 138897660
Conc: 10.48 ng/ml

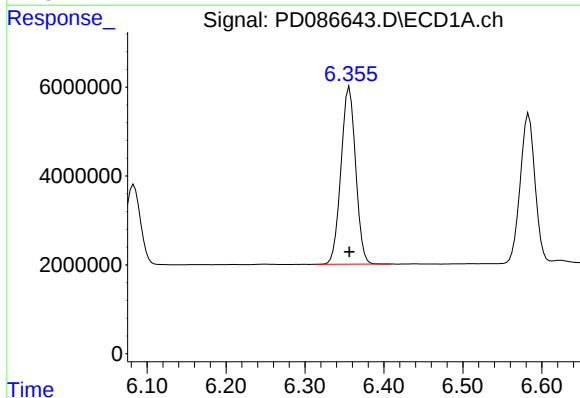


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 51421847
Conc: 19.41 ng/ml

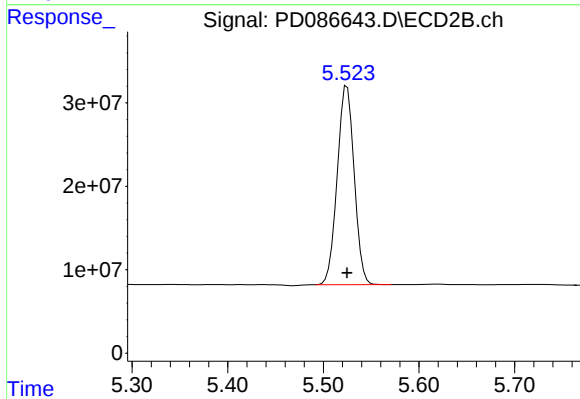


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 294061078
Conc: 20.98 ng/ml

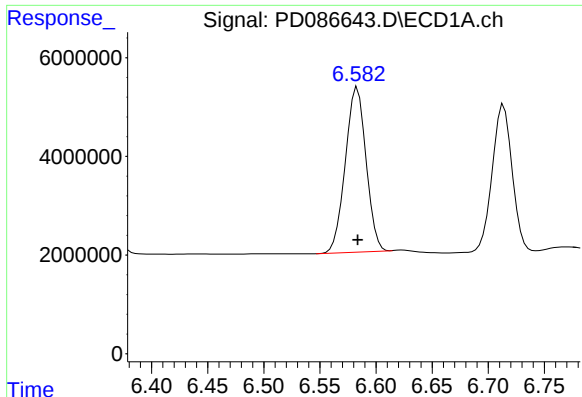


#14 Endrin

R.T.: 6.583 min
Delta R.T.: 0.000 min
Response: 42939207
Conc: 19.46 ng/ml

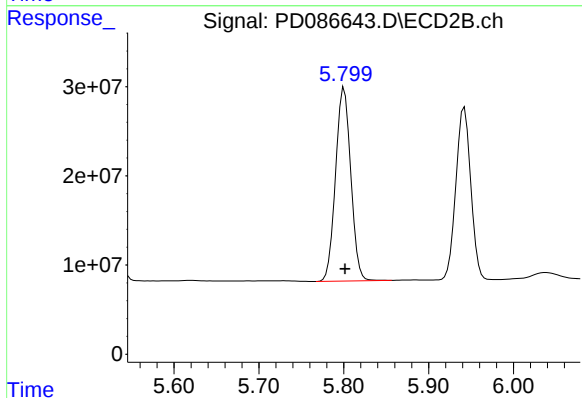


#14 Endrin

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 270462798
Conc: 21.18 ng/ml

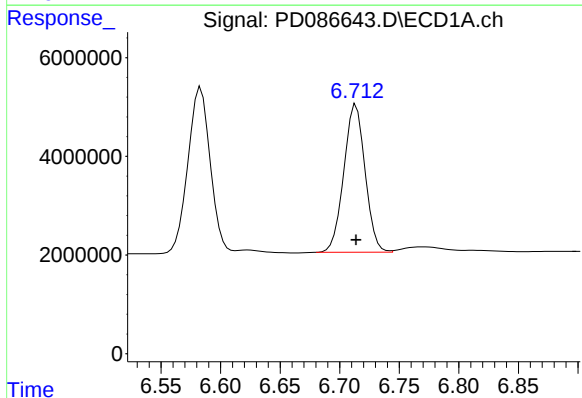


#16 4,4'-DDD

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 37259848
Conc: 19.39 ng/ml

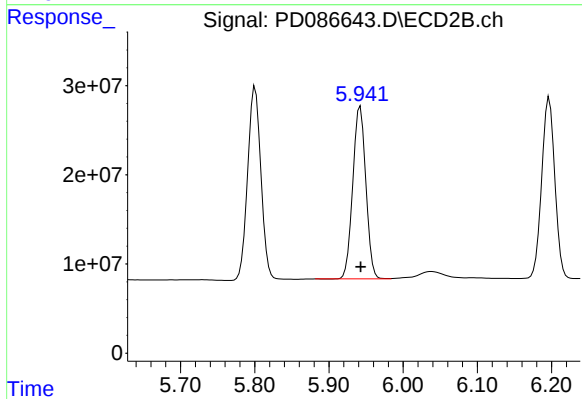


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 236248351
Conc: 21.03 ng/ml

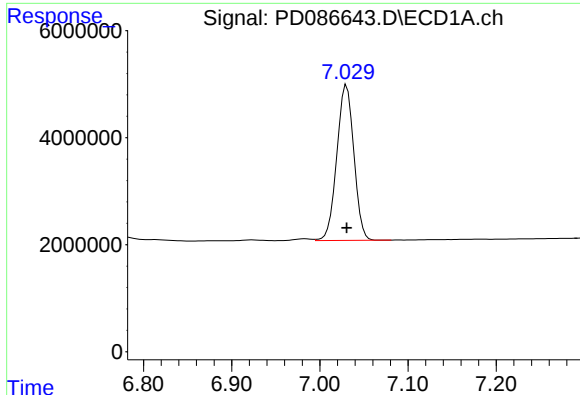


#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 39037371
Conc: 19.46 ng/ml

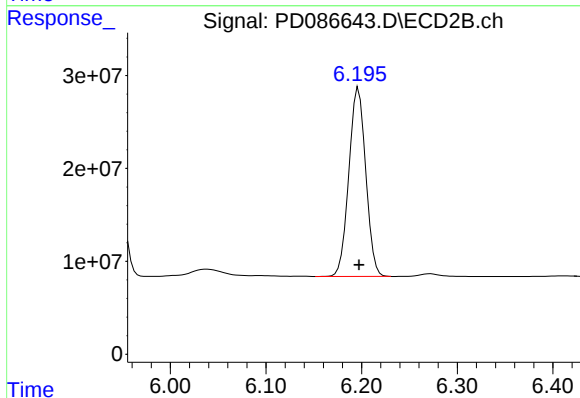


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 250224415
Conc: 20.94 ng/ml

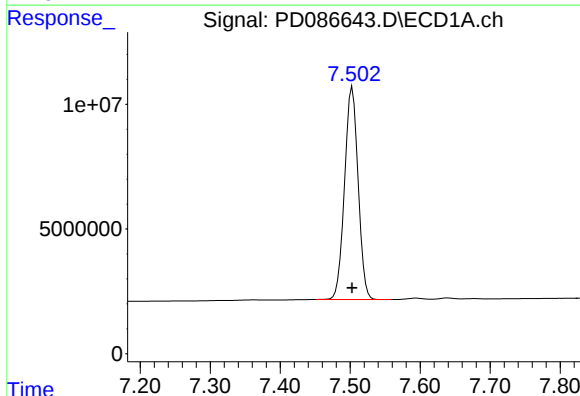


#20 Methoxychlor

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 114781681
Conc: 101.06 ng/ml

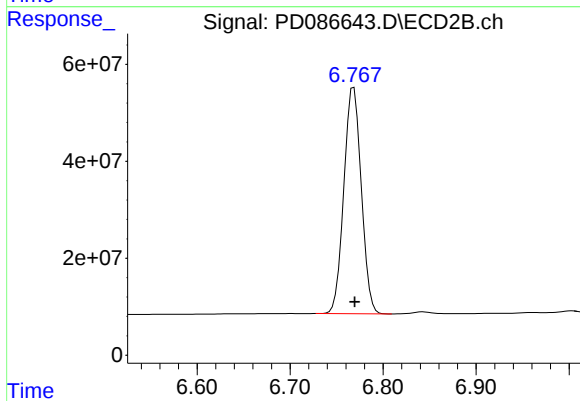


#20 Methoxychlor

R.T.: 6.768 min
Delta R.T.: -0.001 min
Response: 608372223
Conc: 110.34 ng/ml

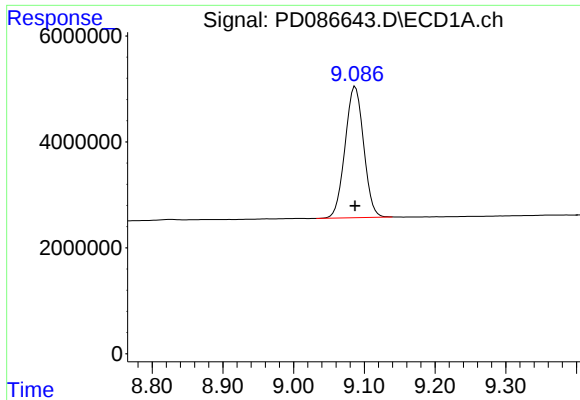

#27 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.000 min
Response: 45199169
Conc: 20.79 ng/ml

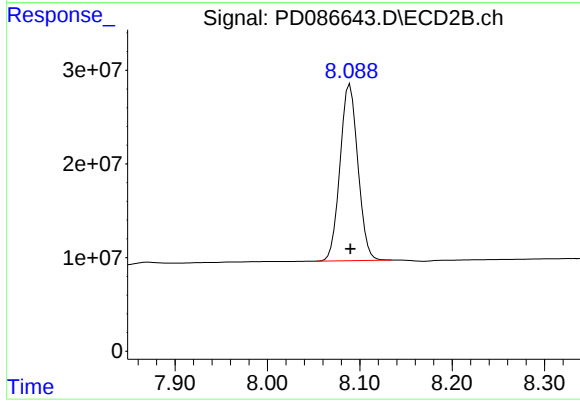

#27 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 253223494
Conc: 21.70 ng/ml