

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 15:00
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 02:06:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 02:04:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	29780798	207.2E6	20.000	20.000
27)	SA Decachlor...	9.087	8.090	86947674	466.8E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.007	3.399	56352118	323.8E6	20.000	20.000
3)	MA gamma-BHC...	4.338	3.737	55718632	302.8E6	20.000	20.000
4)	MA Heptachlor	4.939	4.093	56582070	313.2E6	20.000	20.000
9)	A Endosulfan I	6.084	5.258	47779391	265.2E6	20.000	20.000
13)	MA Dieldrin	6.356	5.525	105.9E6	560.7E6	40.000	40.000
14)	MA Endrin	6.584	5.801	88260123	510.7E6	40.000	40.000
16)	A 4,4'-DDD	6.714	5.943	76856619	449.4E6	40.000	40.000
17)	MA 4,4'-DDT	7.031	6.197	80242994	478.0E6	40.000	40.000
20)	A Methoxychlor	7.502	6.770	227.1E6	1102.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 15:00
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 02:06:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 02:04:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

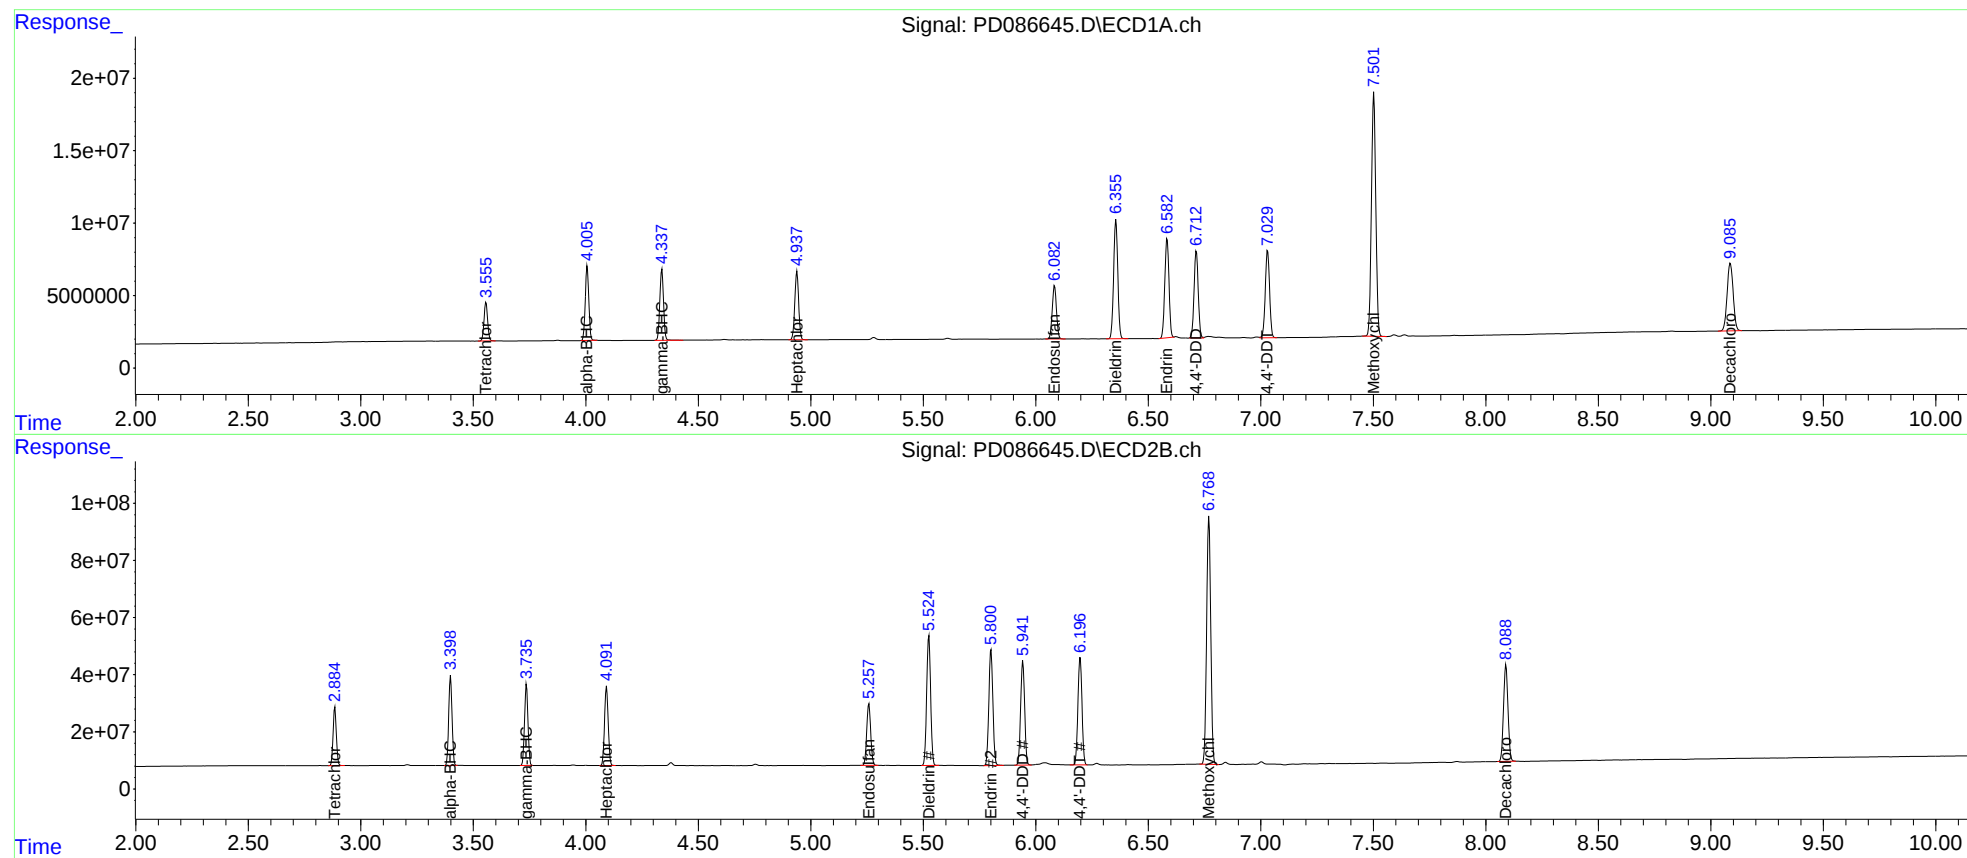

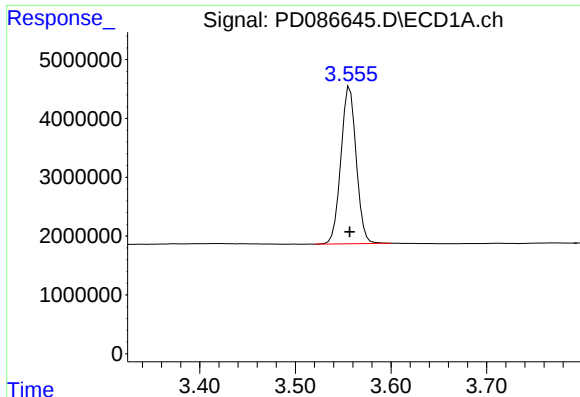


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 29780798
Conc: 20.00 ng/ml

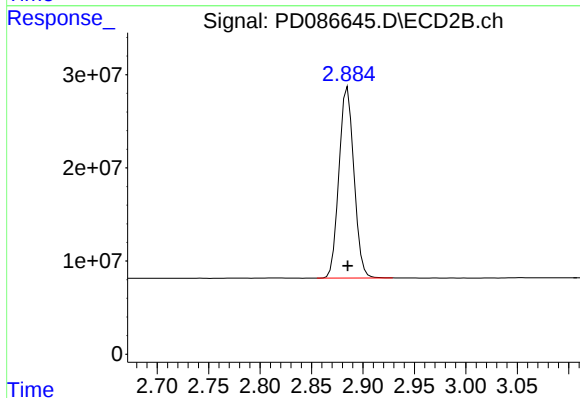


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 207242401
Conc: 20.00 ng/ml

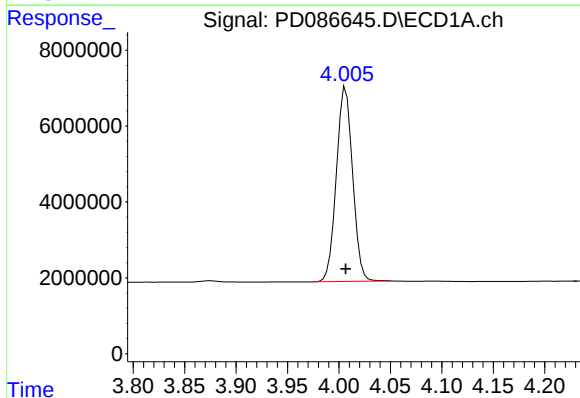


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 56352118
Conc: 20.00 ng/ml

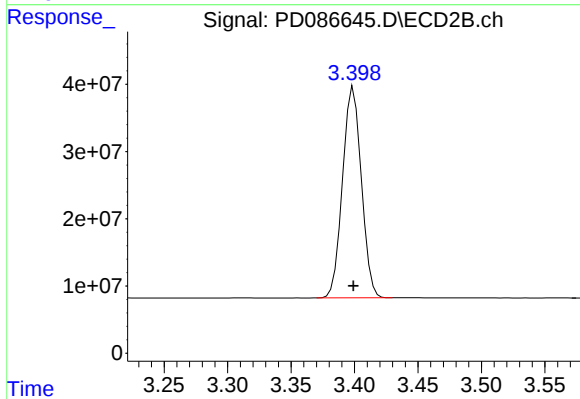


#2 alpha-BHC

R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 323778234
Conc: 20.00 ng/ml

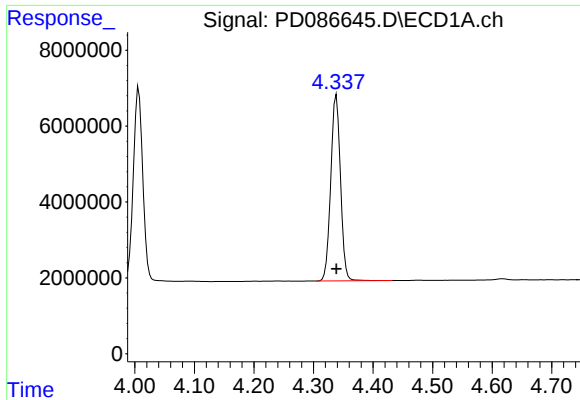


#3 gamma-BHC (Lindane)

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 55718632
Conc: 20.00 ng/ml

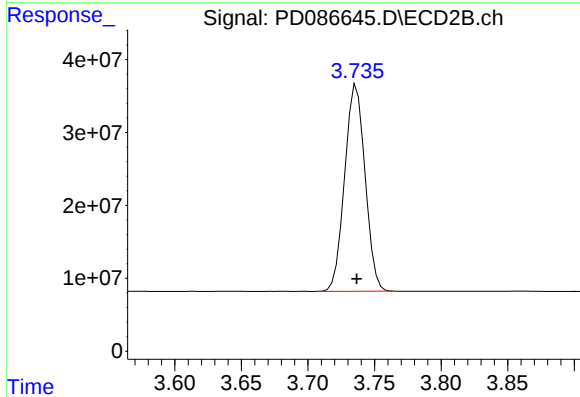


#3 gamma-BHC (Lindane)

R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 302790981
Conc: 20.00 ng/ml

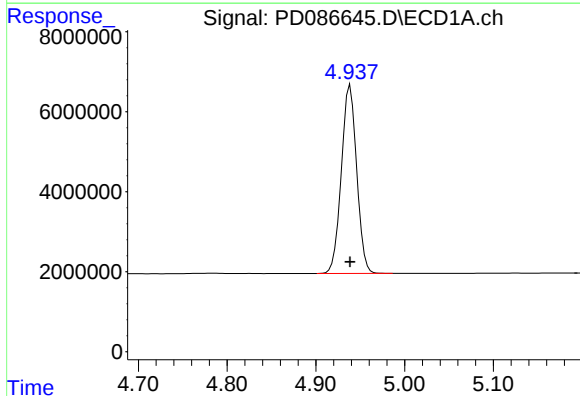


#4 Heptachlor

R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 56582070
Conc: 20.00 ng/ml

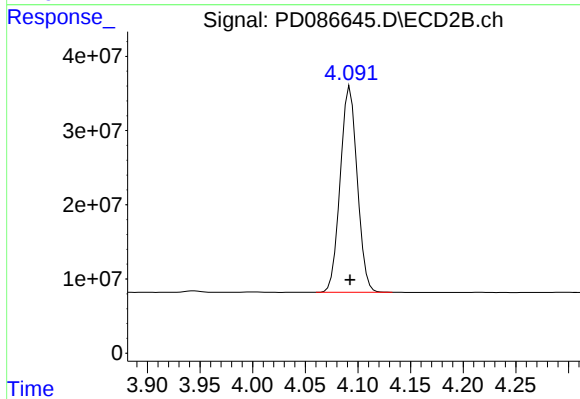


#4 Heptachlor

R.T.: 4.093 min
Delta R.T.: 0.000 min
Response: 313202183
Conc: 20.00 ng/ml

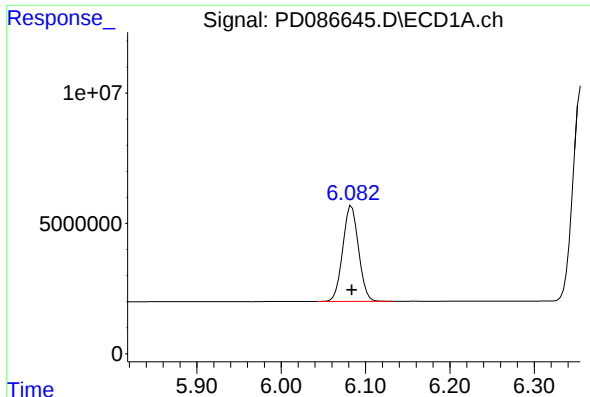


#9 Endosulfan I

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 47779391
Conc: 20.00 ng/ml

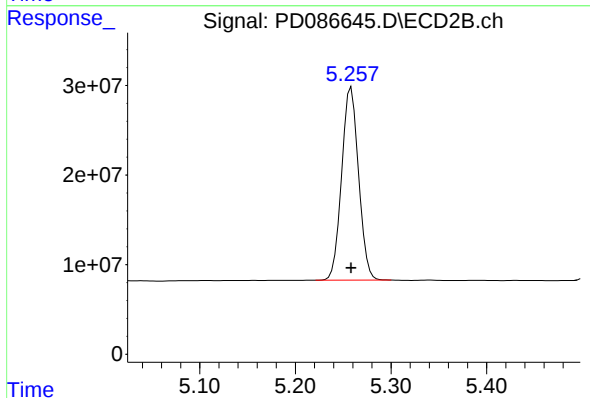


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 265156491
Conc: 20.00 ng/ml

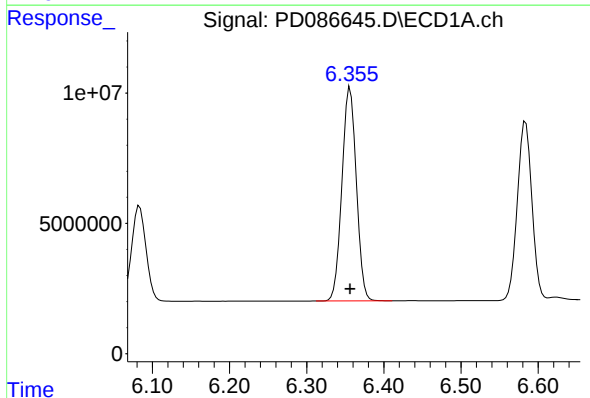


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 105947568
Conc: 40.00 ng/ml

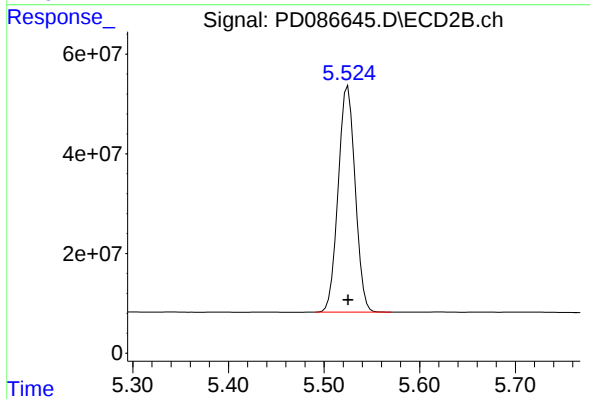


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 560674806
Conc: 40.00 ng/ml

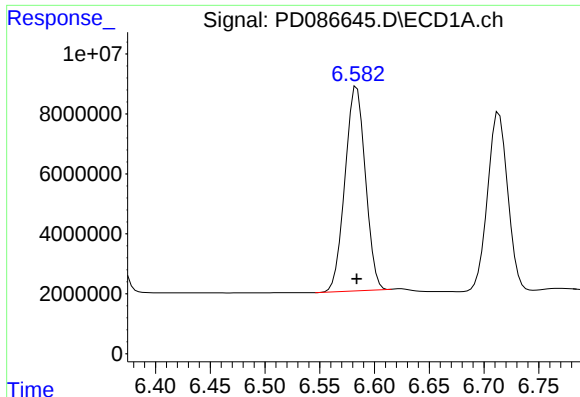


#14 Endrin

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 88260123
Conc: 40.00 ng/ml

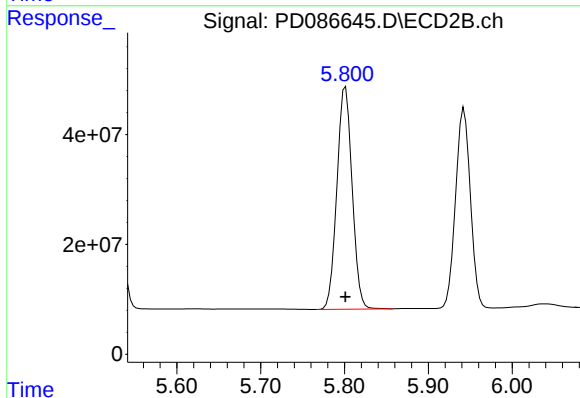


#14 Endrin

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 510704767
Conc: 40.00 ng/ml

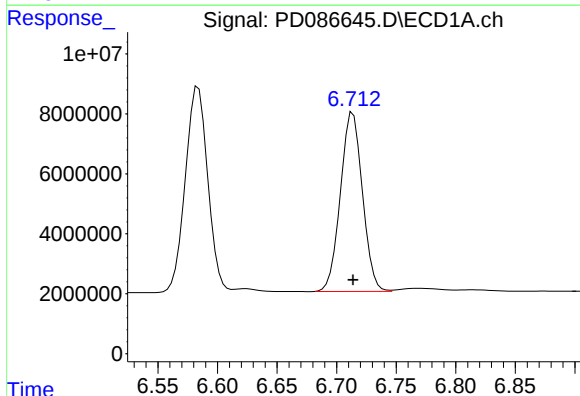


#16 4,4'-DDD

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 76856619
Conc: 40.00 ng/ml

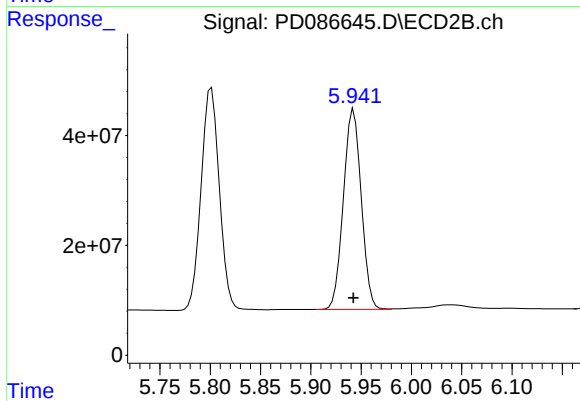


#16 4,4'-DDD

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 449385360
Conc: 40.00 ng/ml

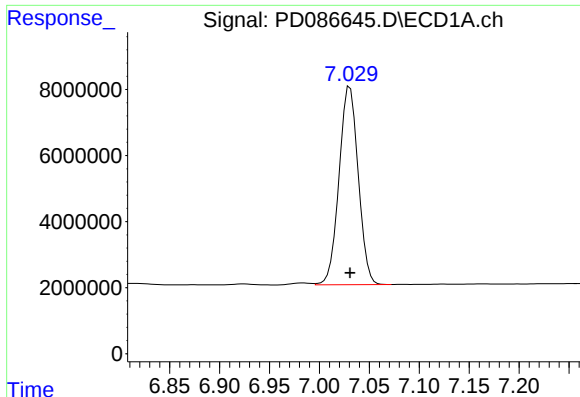


#17 4,4'-DDT

R.T.: 7.031 min
Delta R.T.: 0.000 min
Response: 80242994
Conc: 40.00 ng/ml

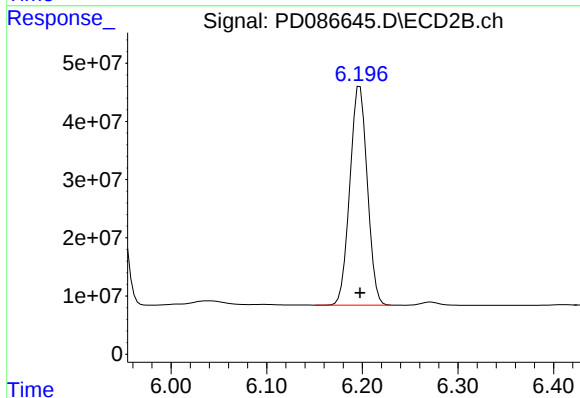


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 478041748
Conc: 40.00 ng/ml

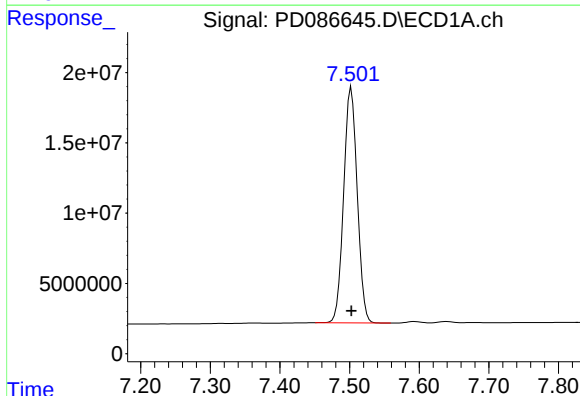


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 227148986
Conc: 200.00 ng/ml

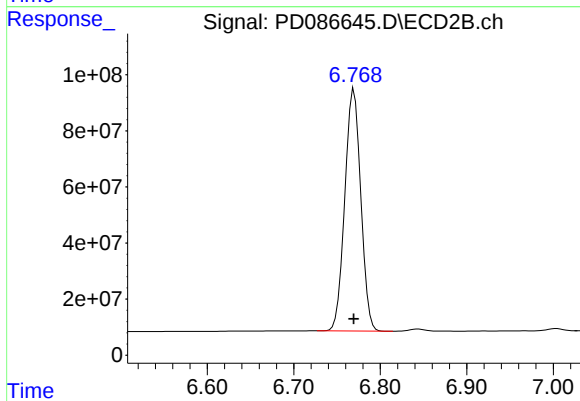


#20 Methoxychlor

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 1102740758
Conc: 200.00 ng/ml

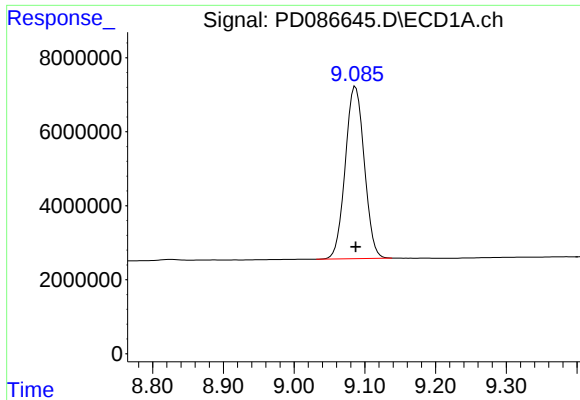

#27 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.000 min
Response: 86947674
Conc: 40.00 ng/ml

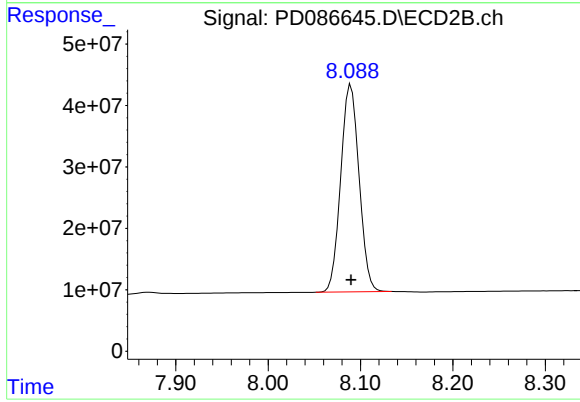

#27 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 466841080
Conc: 40.00 ng/ml