

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 15:28
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 02:06:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 02:04:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	57988823	387.5E6	38.944	37.398
27)	SA Decachlor...	9.087	8.089	166.2E6	863.7E6	76.440	74.006
Target Compounds							
2)	A alpha-BHC	4.007	3.399	118.2E6	620.8E6	41.951	38.344
3)	MA gamma-BHC...	4.338	3.737	115.0E6	575.6E6	41.291	38.020
4)	MA Heptachlor	4.938	4.093	115.3E6	587.7E6	40.751	37.530
9)	A Endosulfan I	6.084	5.258	95287377	494.3E6	39.886	37.287
13)	MA Dieldrin	6.357	5.525	218.7E6	1057.0E6	82.557	75.411
14)	MA Endrin	6.584	5.801	182.6E6	960.7E6	82.764	75.247
16)	A 4,4'-DDD	6.714	5.942	158.7E6	845.0E6	82.593	75.210
17)	MA 4,4'-DDT	7.030	6.197	165.3E6	907.3E6	82.383	75.916
20)	A Methoxychlor	7.502	6.769	446.6E6	1968.7E6	393.253	357.056


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 15:28
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 02:06:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 02:04:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

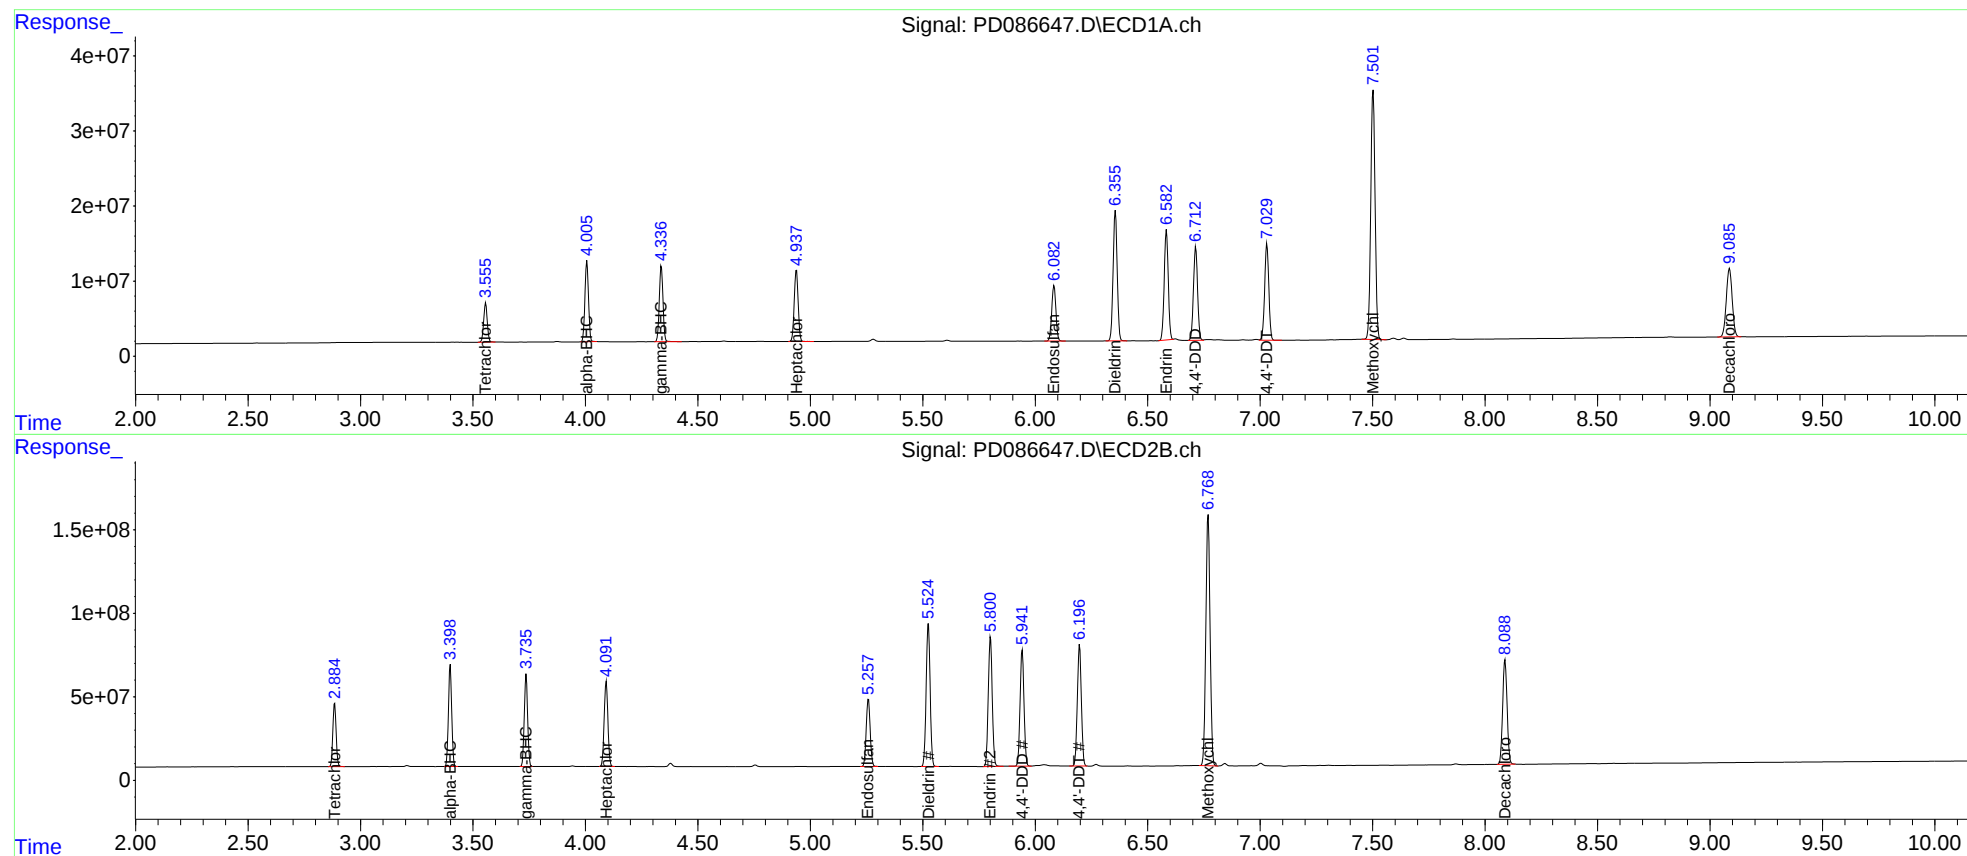

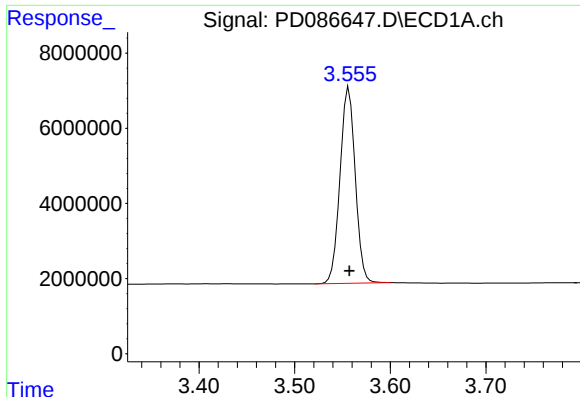


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 57988823
Conc: 38.94 ng/ml

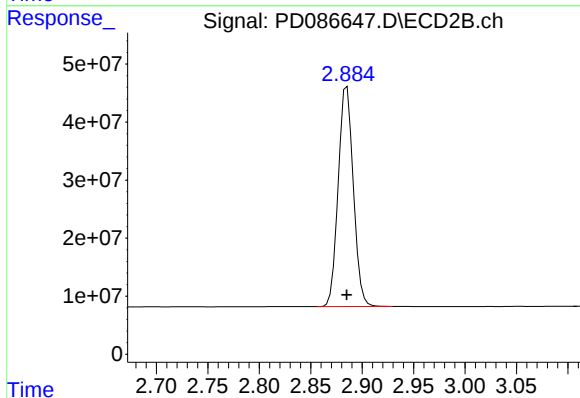


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 387527661
Conc: 37.40 ng/ml

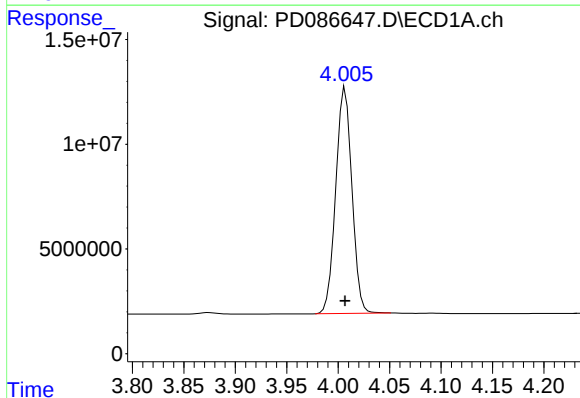


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 118200620
Conc: 41.95 ng/ml

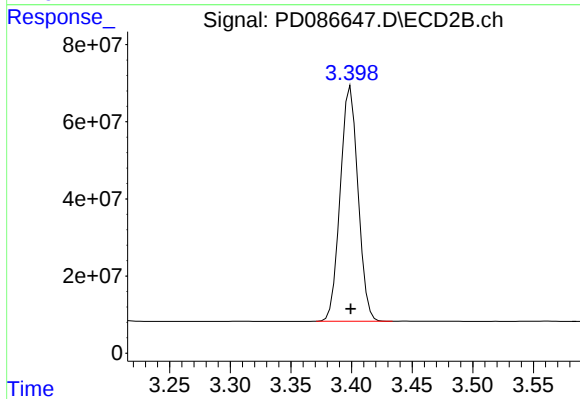


#2 alpha-BHC

R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 620752950
Conc: 38.34 ng/ml

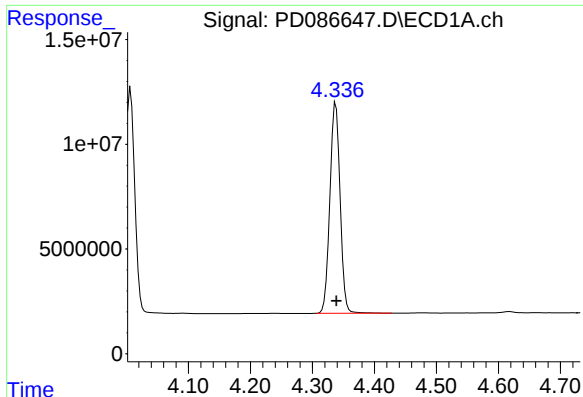


#3 gamma-BHC (Lindane)

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 115033607
Conc: 41.29 ng/ml

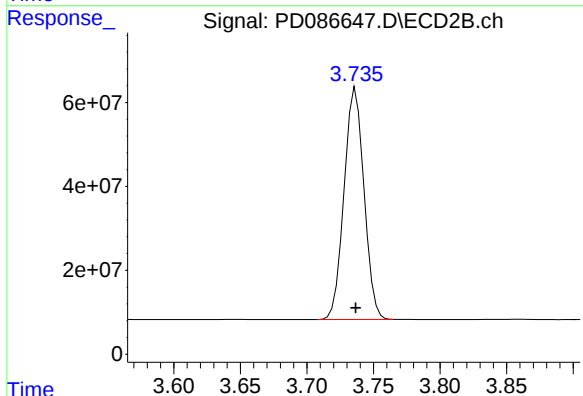


#3 gamma-BHC (Lindane)

R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 575610012
Conc: 38.02 ng/ml

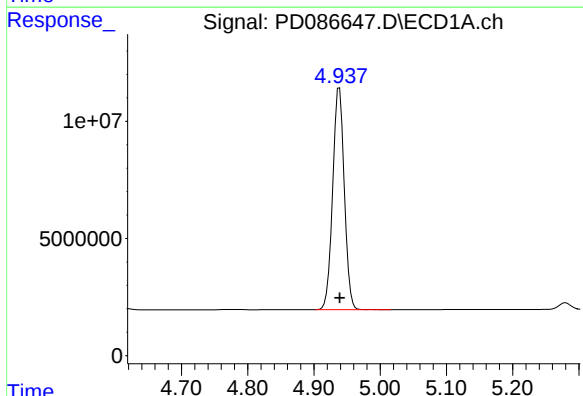


#4 Heptachlor

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 115288860
Conc: 40.75 ng/ml

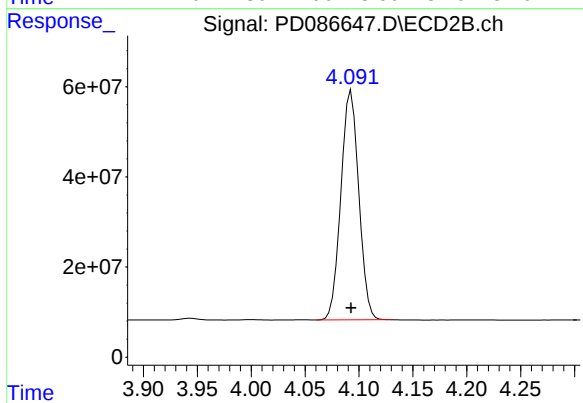


#4 Heptachlor

R.T.: 4.093 min
Delta R.T.: 0.000 min
Response: 587728231
Conc: 37.53 ng/ml

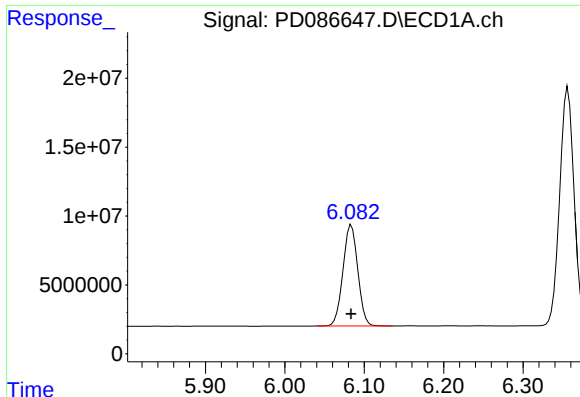


#9 Endosulfan I

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 95287377
Conc: 39.89 ng/ml

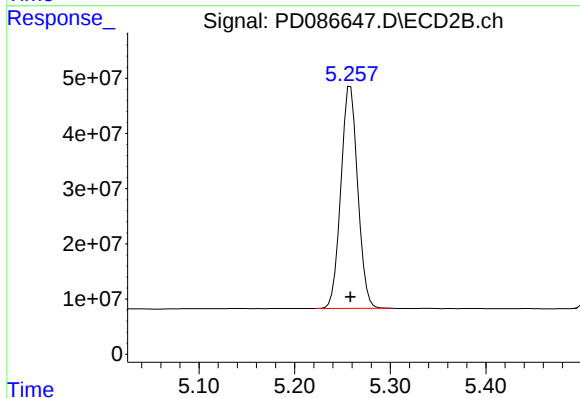


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 494342454
Conc: 37.29 ng/ml

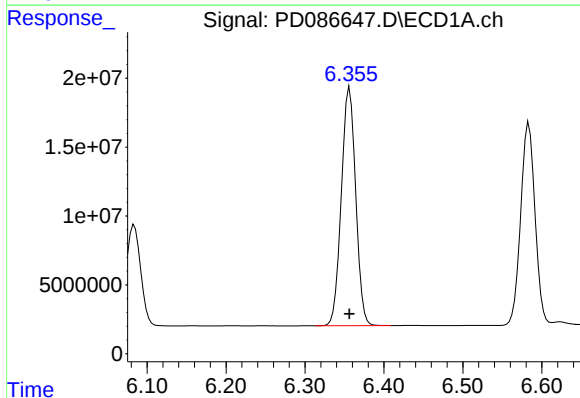


#13 Dieldrin

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 218668393
Conc: 82.56 ng/ml

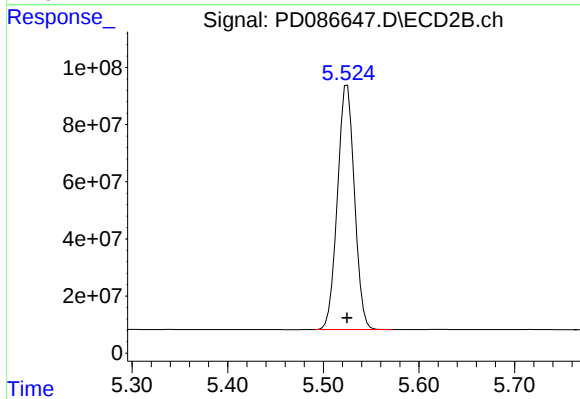


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 1057032622
Conc: 75.41 ng/ml

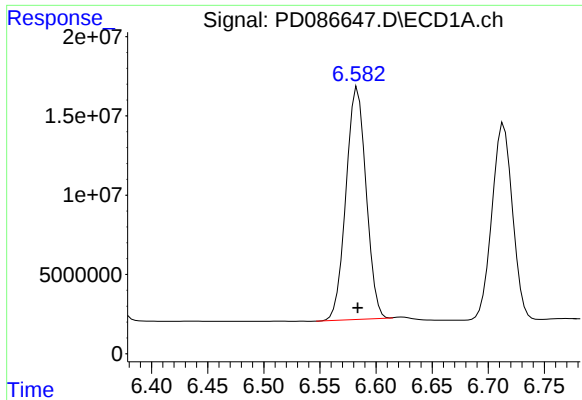


#14 Endrin

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 182617976
Conc: 82.76 ng/ml

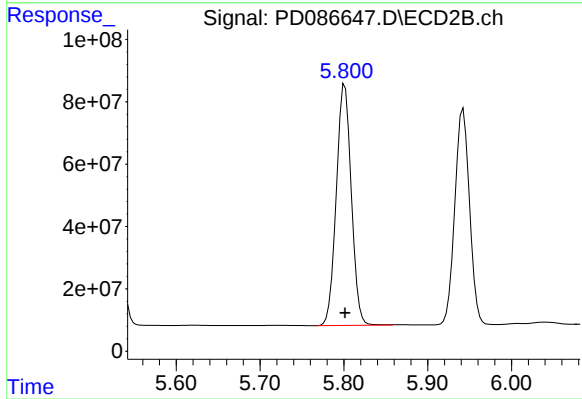


#14 Endrin

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 960731369
Conc: 75.25 ng/ml

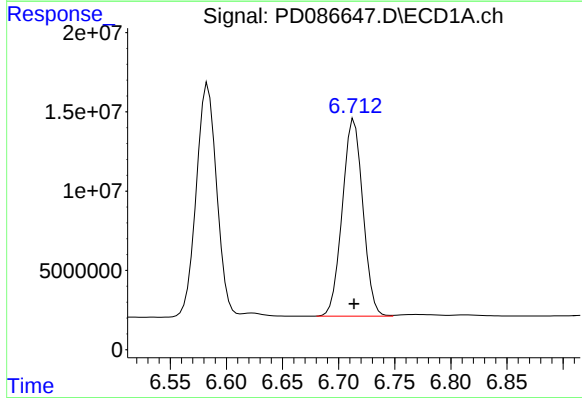


#16 4,4'-DDD

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 158694697
Conc: 82.59 ng/ml

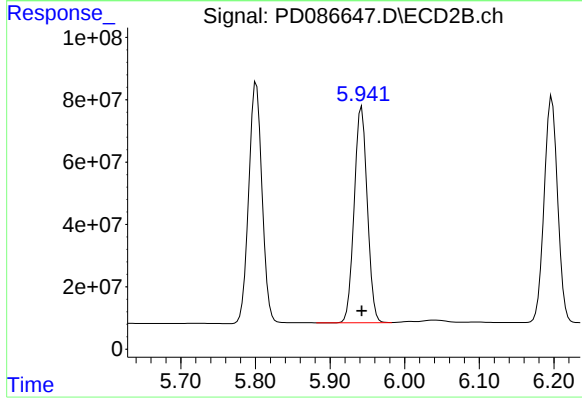


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 844959043
Conc: 75.21 ng/ml

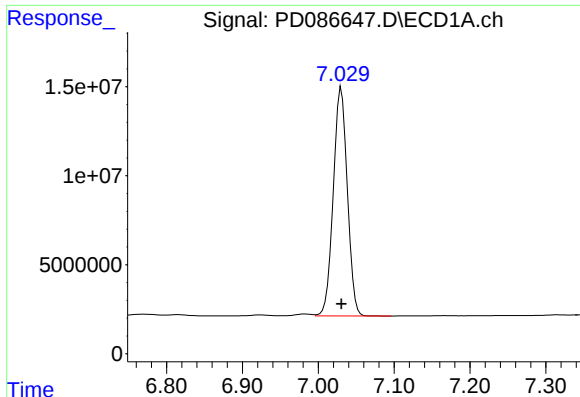


#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 165265771
Conc: 82.38 ng/ml

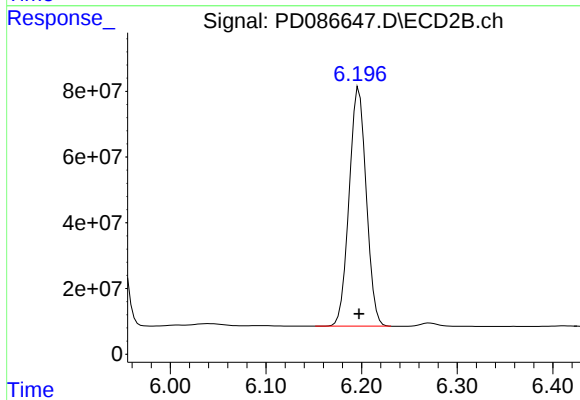


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 907269985
Conc: 75.92 ng/ml

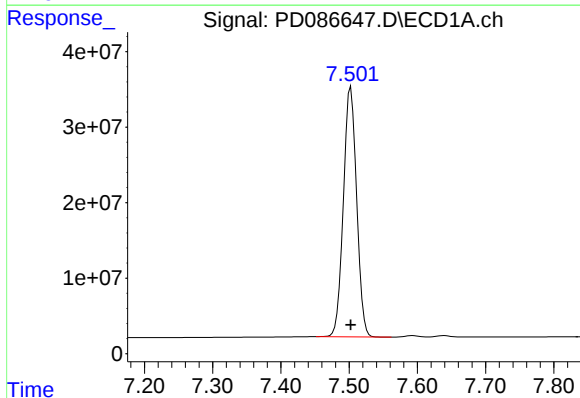


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 446634651
Conc: 393.25 ng/ml

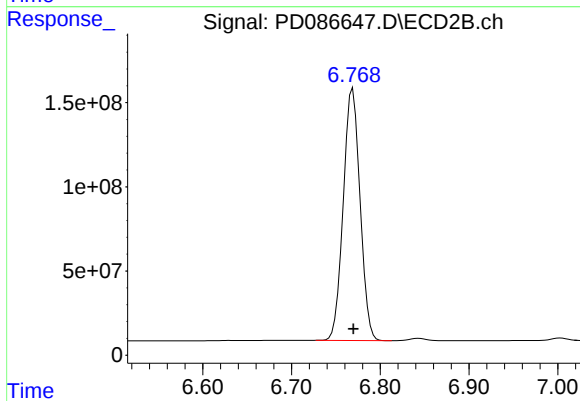

#20 Methoxychlor

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 1968701697
Conc: 357.06 ng/ml

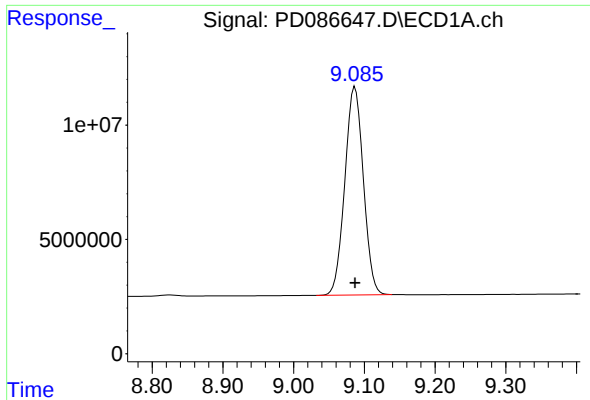


#27 Decachlorobiphenyl

R.T.: 9.087 min

Delta R.T.: 0.000 min

Response: 166156325

Conc: 76.44 ng/ml

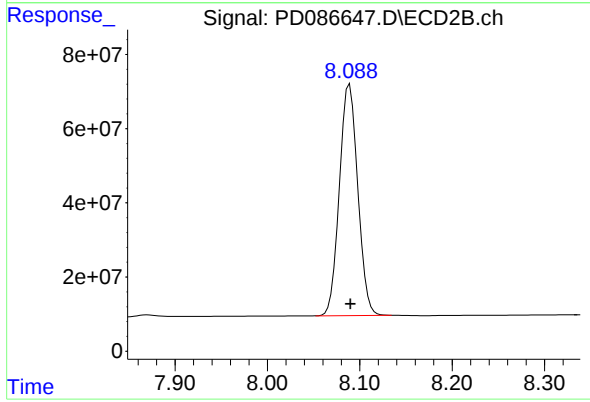

#27 Decachlorobiphenyl

R.T.: 8.089 min

Delta R.T.: 0.000 min

Response: 863723360

Conc: 74.01 ng/ml