

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 15:56
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 02:06:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 02:04:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	118.6E6	751.3E6	79.622	72.505
27)	SA Decachlor...	9.087	8.090	334.0E6	1660.1E6	153.651	142.240
Target Compounds							
2)	A alpha-BHC	4.007	3.400	261.3E6	1231.8E6	92.745	76.091
3)	MA gamma-BHC...	4.338	3.737	250.7E6	1135.9E6	89.970	75.031
4)	MA Heptachlor	4.939	4.093	246.8E6	1136.5E6	87.243	72.570
9)	A Endosulfan I	6.084	5.259	198.9E6	945.6E6	83.267	71.321
13)	MA Dieldrin	6.356	5.525	466.3E6	2041.7E6	176.052	145.661
14)	MA Endrin	6.584	5.801	389.8E6	1843.5E6	176.676	144.391
16)	A 4,4'-DDD	6.714	5.942	339.2E6	1630.5E6	176.538	145.129
17)	MA 4,4'-DDT	7.030	6.197	353.2E6	1752.9E6	176.060	146.673
20)	A Methoxychlor	7.503	6.770	897.5E6	3496.6E6	790.248	634.165


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 15:56
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 02:06:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 02:04:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

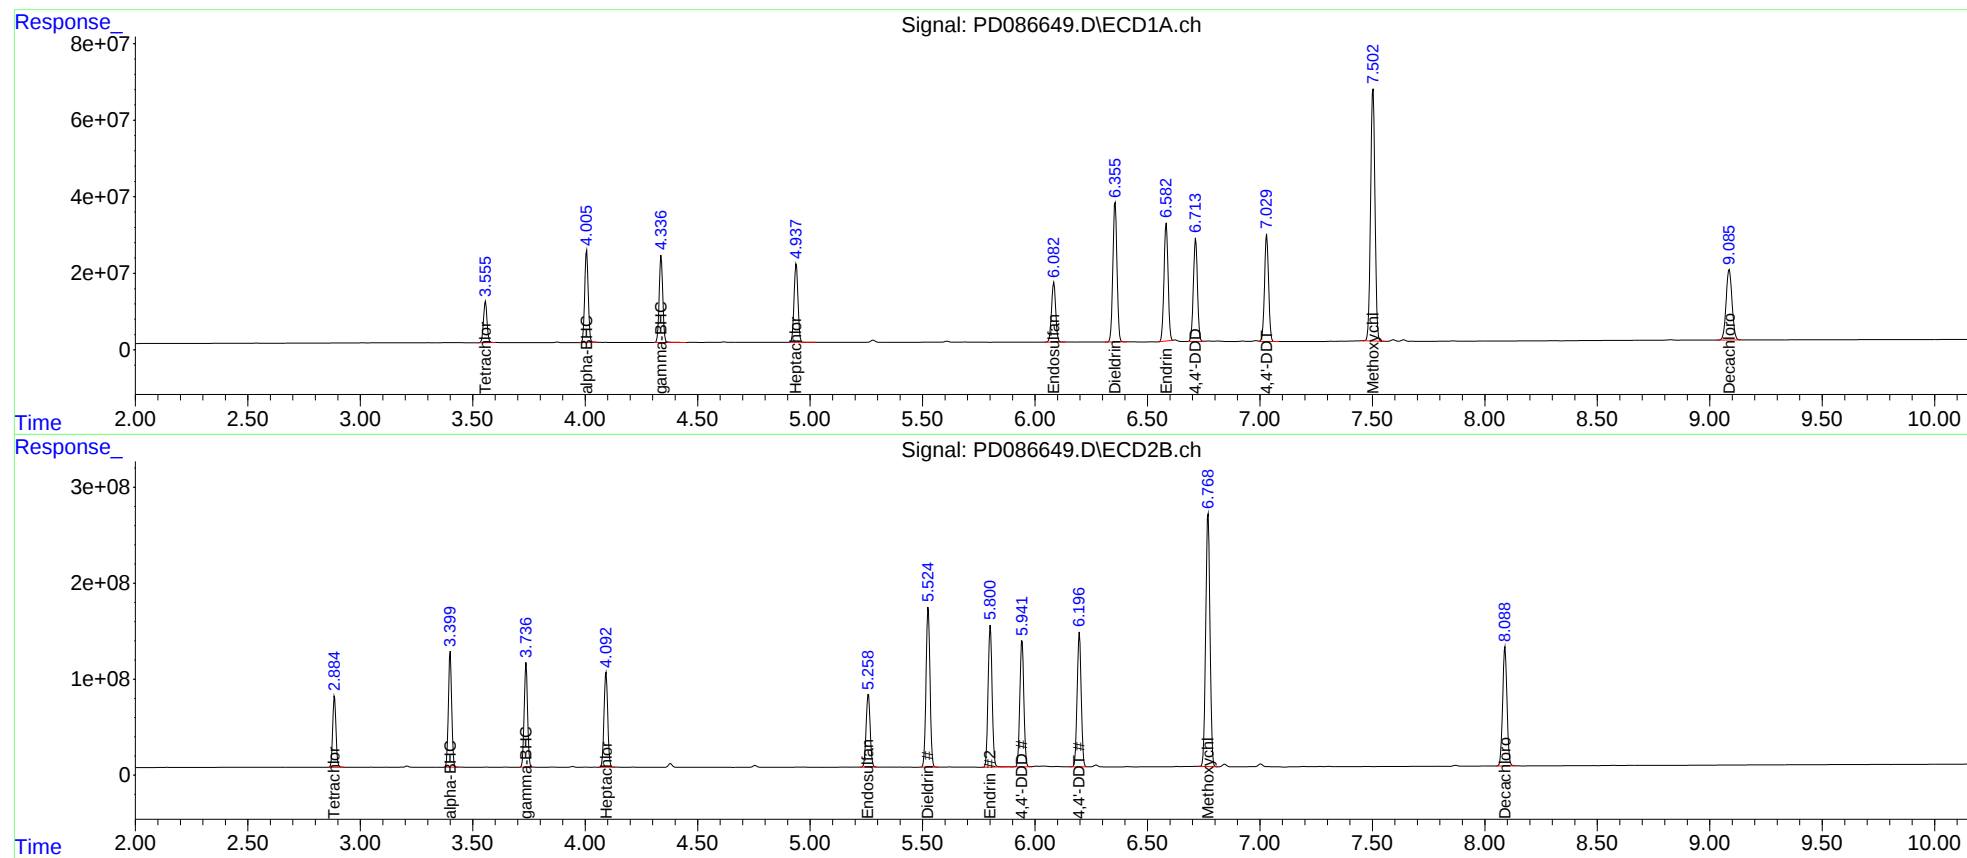

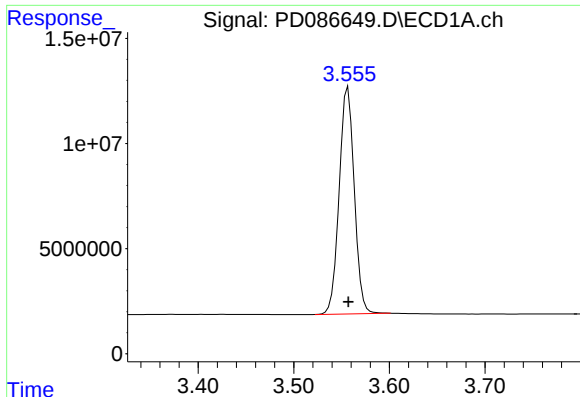


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 118560551
Conc: 79.62 ng/ml

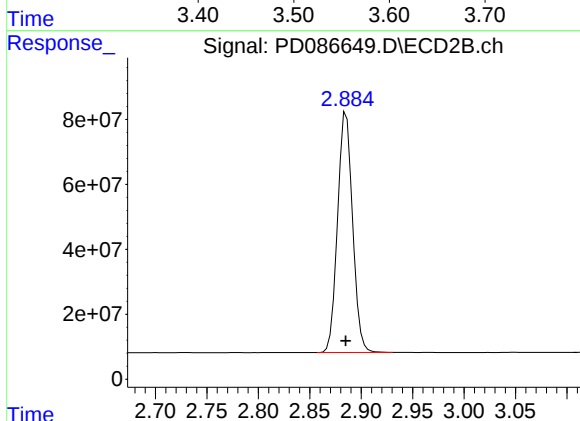


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 751304505
Conc: 72.50 ng/ml

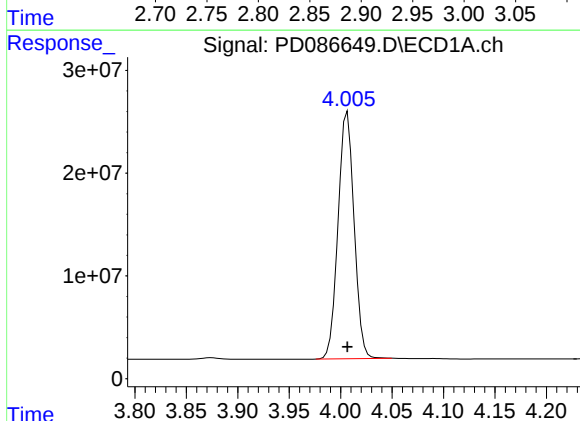


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 261318221
Conc: 92.74 ng/ml

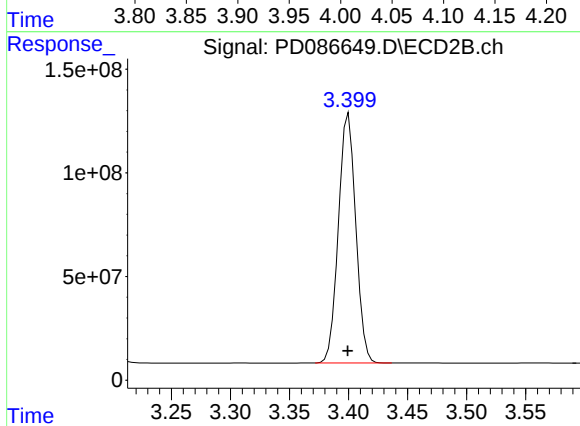


#2 alpha-BHC

R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 1231826644
Conc: 76.09 ng/ml

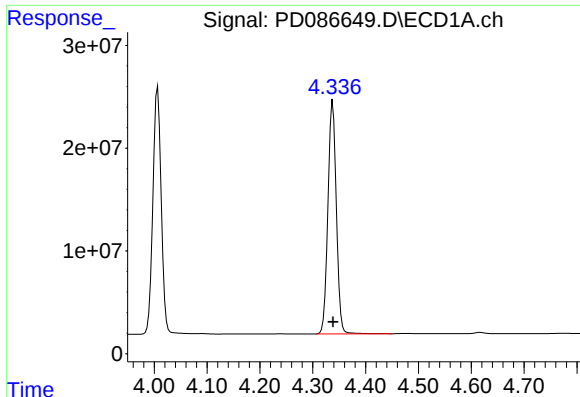


#3 gamma-BHC (Lindane)

R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 250650403
Conc: 89.97 ng/ml

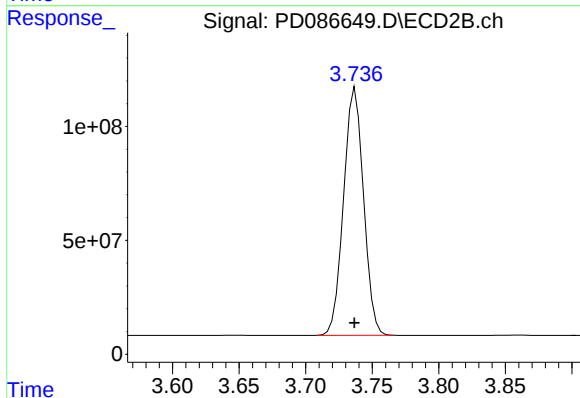


#3 gamma-BHC (Lindane)

R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 1135928387
Conc: 75.03 ng/ml

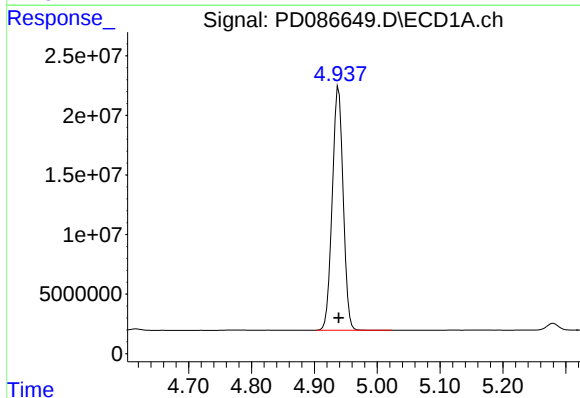


#4 Heptachlor

R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 246819420
Conc: 87.24 ng/ml

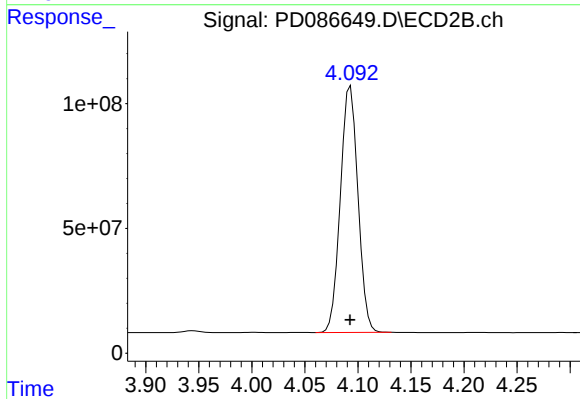


#4 Heptachlor

R.T.: 4.093 min
Delta R.T.: 0.000 min
Response: 1136450660
Conc: 72.57 ng/ml

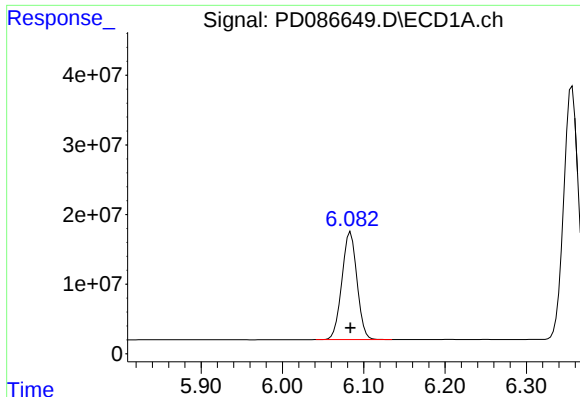


#9 Endosulfan I

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 198921798
Conc: 83.27 ng/ml

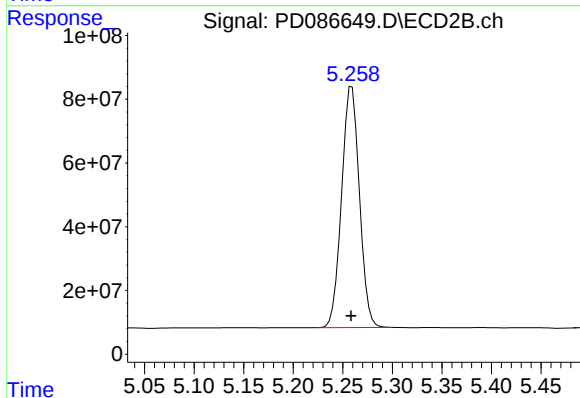


#9 Endosulfan I

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 945558030
Conc: 71.32 ng/ml

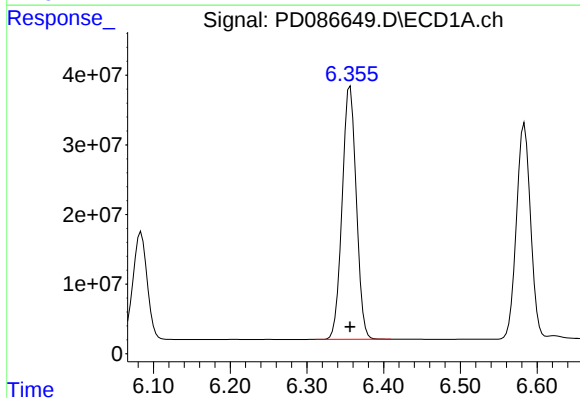


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 466306317
Conc: 176.05 ng/ml

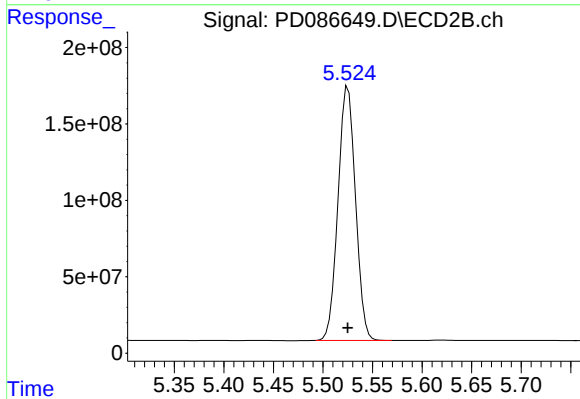


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 2041705657
Conc: 145.66 ng/ml

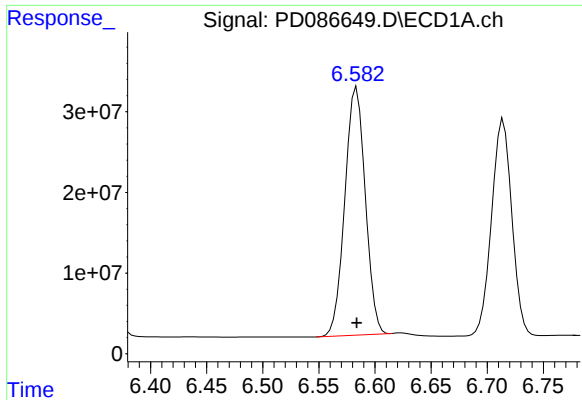


#14 Endrin

R.T.: 6.584 min
Delta R.T.: 0.000 min
Response: 389837132
Conc: 176.68 ng/ml

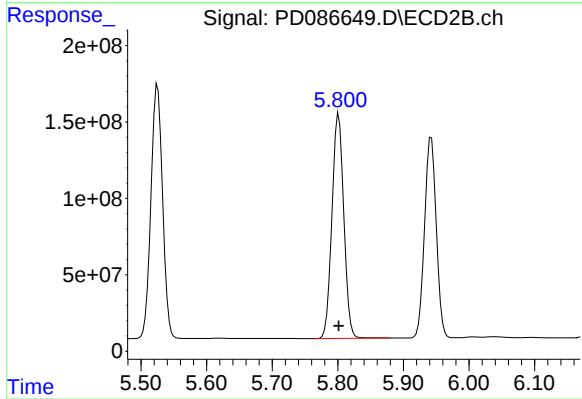


#14 Endrin

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 1843533220
Conc: 144.39 ng/ml

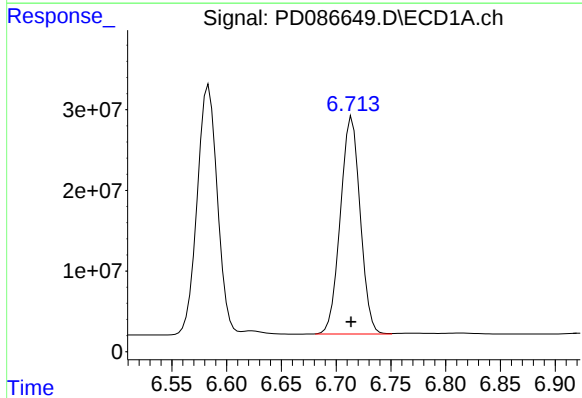


#16 4,4'-DDD

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 339202428
Conc: 176.54 ng/ml

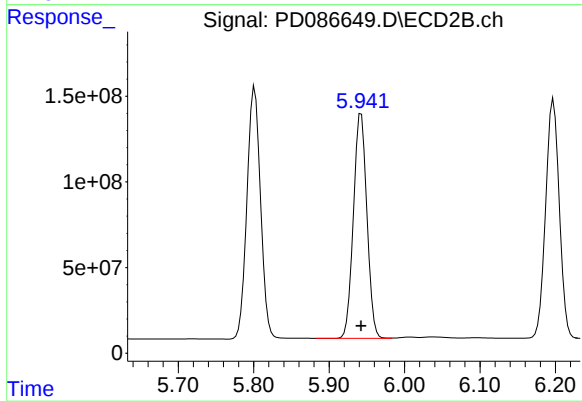


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 1630476375
Conc: 145.13 ng/ml

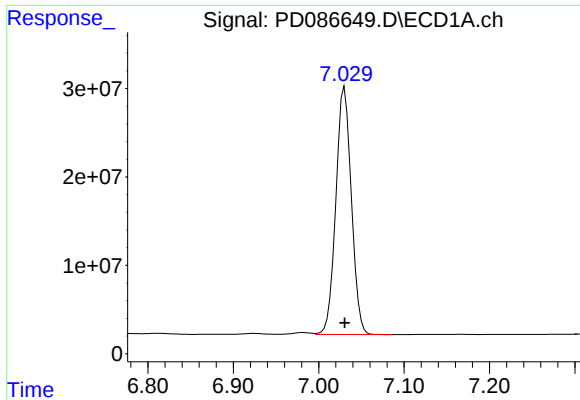


#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 353190141
Conc: 176.06 ng/ml

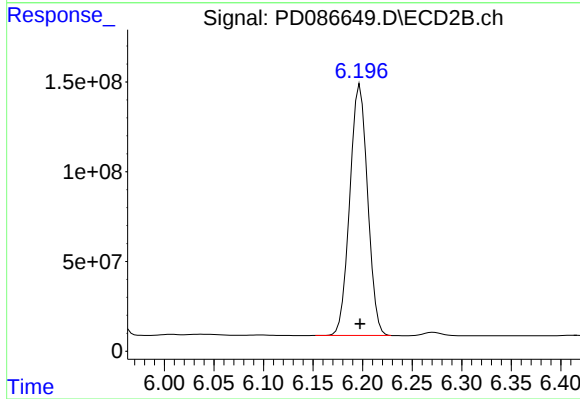


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 1752898373
Conc: 146.67 ng/ml

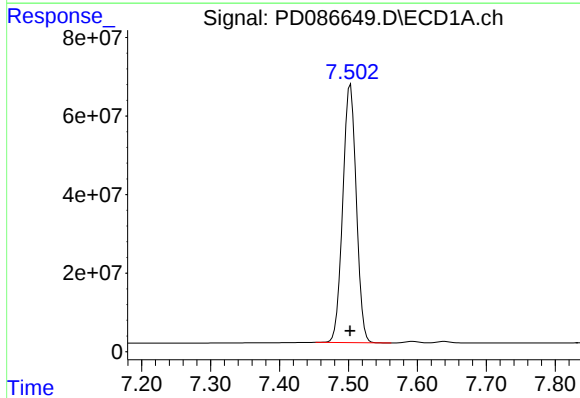


#20 Methoxychlor

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 897519855
Conc: 790.25 ng/ml

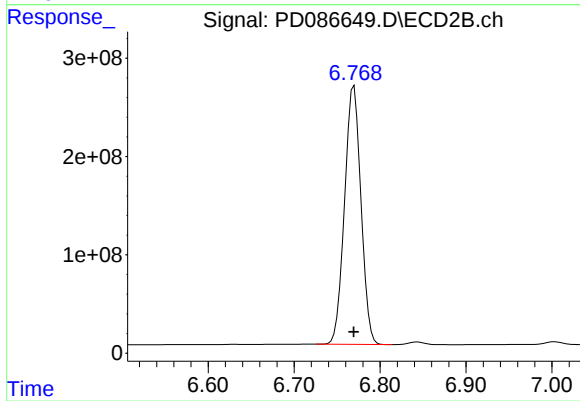


#20 Methoxychlor

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 3496595968
Conc: 634.16 ng/ml

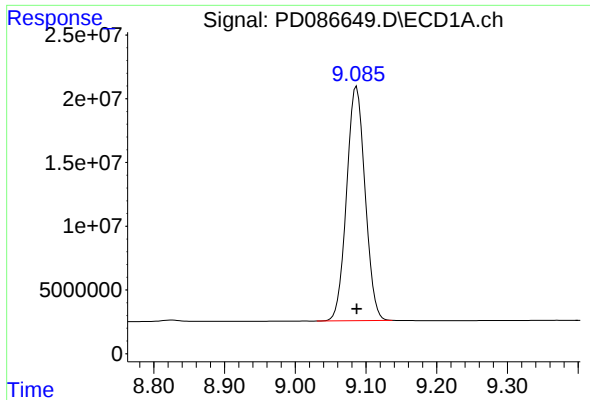

#27 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.000 min
Response: 333990284
Conc: 153.65 ng/ml

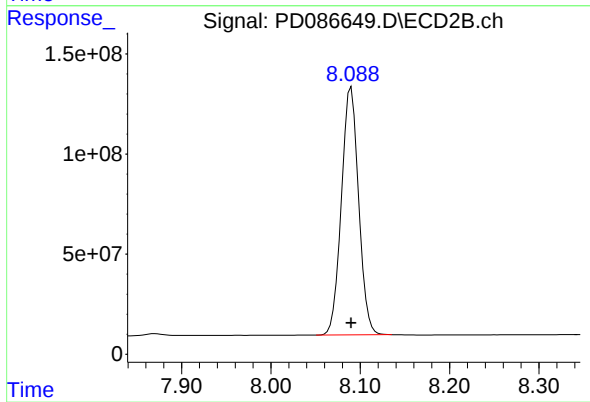

#27 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 1660084468
Conc: 142.24 ng/ml