

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 12:25
 Operator : AR\AJ
 Sample : RESC052
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:07:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	29708016	207.9E6	19.782	19.993
2)	SA Decachlor...	9.086	8.089	85362963	456.3E6	38.576	38.460
Target Compounds							
2)	A alpha-BHC	4.006	3.400	29754778	184.4E6	10.351	11.370
3)	MA gamma-BHC...	4.337	3.737	29726531	172.8E6	10.492	11.384
4)	MA Heptachlor	4.938	4.092	30620709	179.8E6	10.648	11.456
5)	MB Aldrin	5.280	4.379	23827271	141.7E6	8.855	9.620
6)	B beta-BHC	4.521	4.032	11127318	64288930	8.970	9.398
7)	B delta-BHC	4.770	4.269	23151423	139.0E6	8.191	9.114
8)	B Heptachlo...	5.699	4.884	22006674	129.7E6	8.678	9.405
9)	A Endosulfan I	6.083	5.258	26417585	153.8E6	10.919	11.682
10)	B trans-Chl...	5.954	5.137	21281885	134.7E6	8.580	9.304
11)	B cis-Chlor...	6.036	5.202	21810868	131.6E6	8.688	9.312
12)	B 4,4'-DDE	6.204	5.388	39980863	247.2E6	16.716	18.573
13)	MA Dieldrin	6.356	5.524	56589525	321.3E6	21.108	22.945
14)	MA Endrin	6.583	5.801	47426829	295.7E6	21.160	23.039
15)	B Endosulfa...	6.794	6.092	42286786	231.6E6	17.716	18.858
16)	A 4,4'-DDD	6.713	5.942	41079390	259.4E6	21.125	23.118
17)	MA 4,4'-DDT	7.030	6.197	44427776	273.1E6	21.874	22.883
18)	B Endrin al...	6.923	6.270	30845643	181.2E6	17.693	19.087
19)	B Endosulfa...	7.157	6.494	36755306	221.3E6	17.282	18.719
20)	A Methoxychlor	7.502	6.769	125.8E6	656.8E6	110.665	119.577
21)	B Endrin ke...	7.638	7.003	42954545	252.0E6	17.632	19.180

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 12:25
Operator : AR\AJ
Sample : RESC052
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:07:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

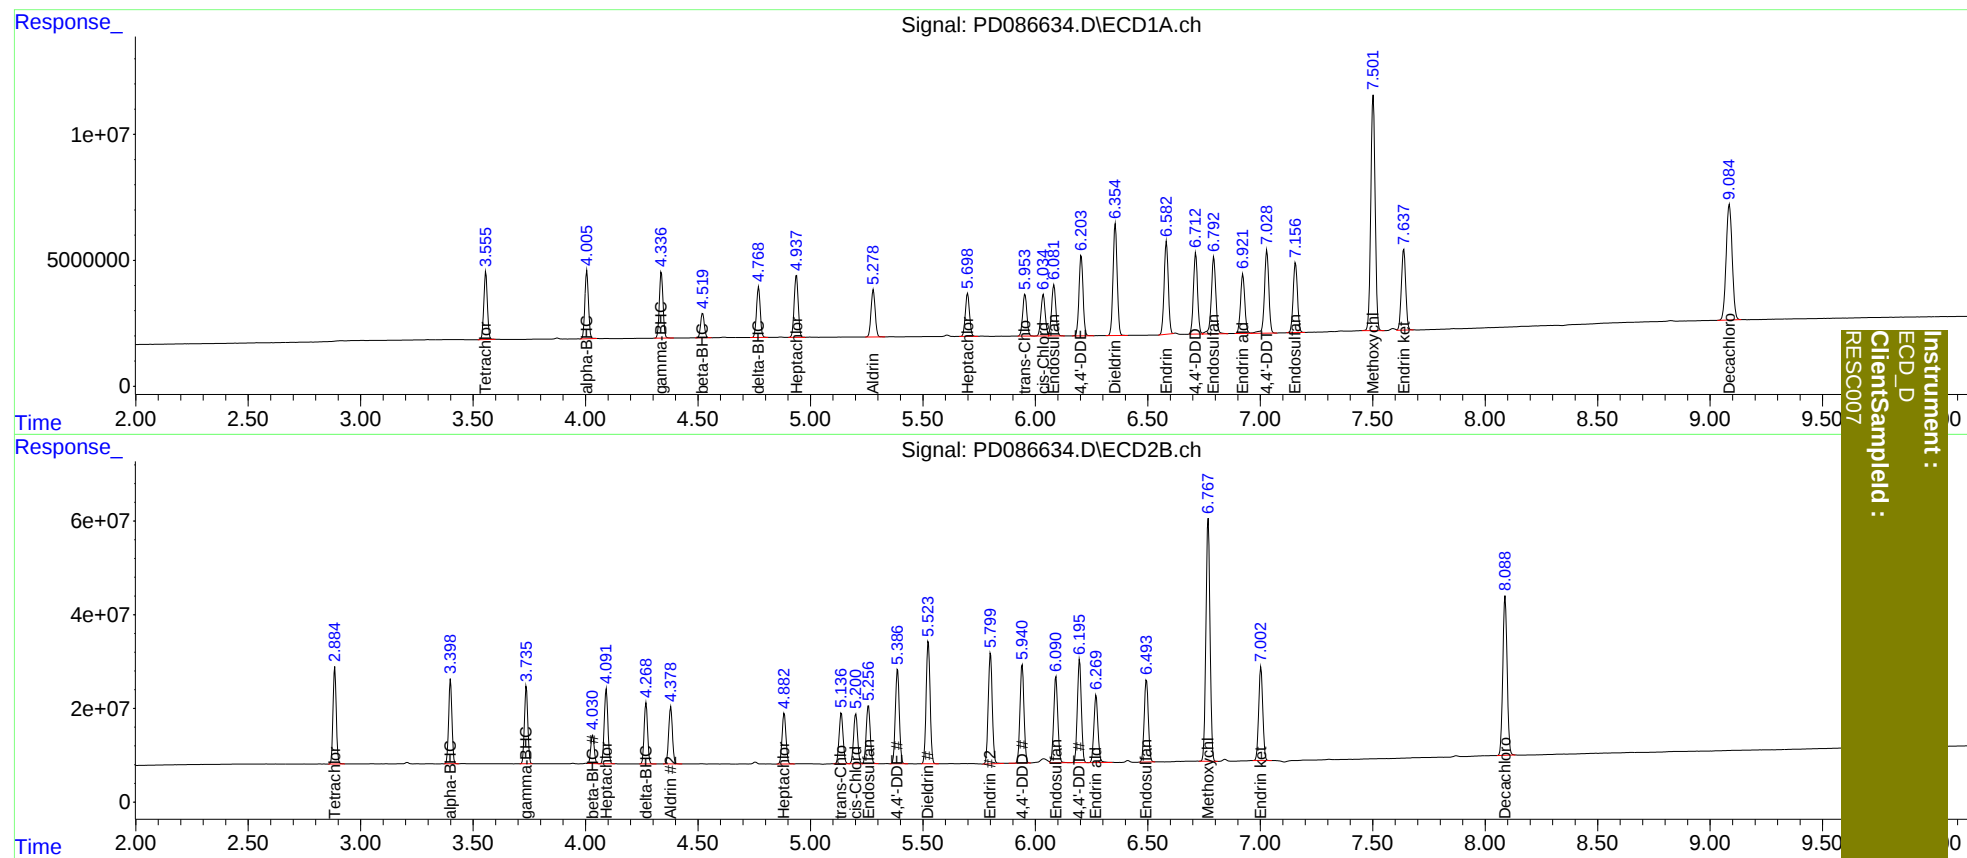

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086634.D
Acq On : 13 Nov 2024 12:25
Operator : AR\AJ
Sample : RESC052
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Title : GC Extractables
Last Update : Thu Nov 14 03:38:57 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.557	4.006	100.00%
4.006	4.337	100.00%
4.337	4.521	100.00%
4.521	4.770	100.00%
4.770	4.938	100.00%
4.938	5.280	100.00%
5.280	5.699	100.00%
5.699	5.954	100.00%
5.954	6.036	100.00%
6.036	6.083	95.18%
6.083	6.204	100.00%
6.204	6.356	100.00%
6.356	6.583	100.00%
6.583	6.713	100.00%
6.713	6.794	100.00%
6.794	6.923	100.00%
6.923	7.030	100.00%
7.030	7.157	100.00%
7.157	7.502	100.00%
7.502	7.638	100.00%
7.638	9.086	100.00%

Signal #2


2.885	3.400	100.00%
3.400	3.737	100.00%
3.737	4.032	100.00%
4.032	4.092	100.00%
4.092	4.269	100.00%
4.269	4.379	100.00%
4.379	4.884	100.00%
4.884	5.137	100.00%
5.137	5.202	100.00%
5.202	5.258	100.00%
5.258	5.388	100.00%
5.388	5.524	100.00%
5.524	5.801	100.00%
5.801	5.942	100.00%
5.942	6.092	100.00%
6.092	6.197	100.00%
6.197	6.270	100.00%
6.270	6.494	100.00%
6.494	6.769	100.00%
6.769	7.003	100.00%
7.003	8.089	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 12:25
Operator : AR\AJ
Sample : RESC052
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:07:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

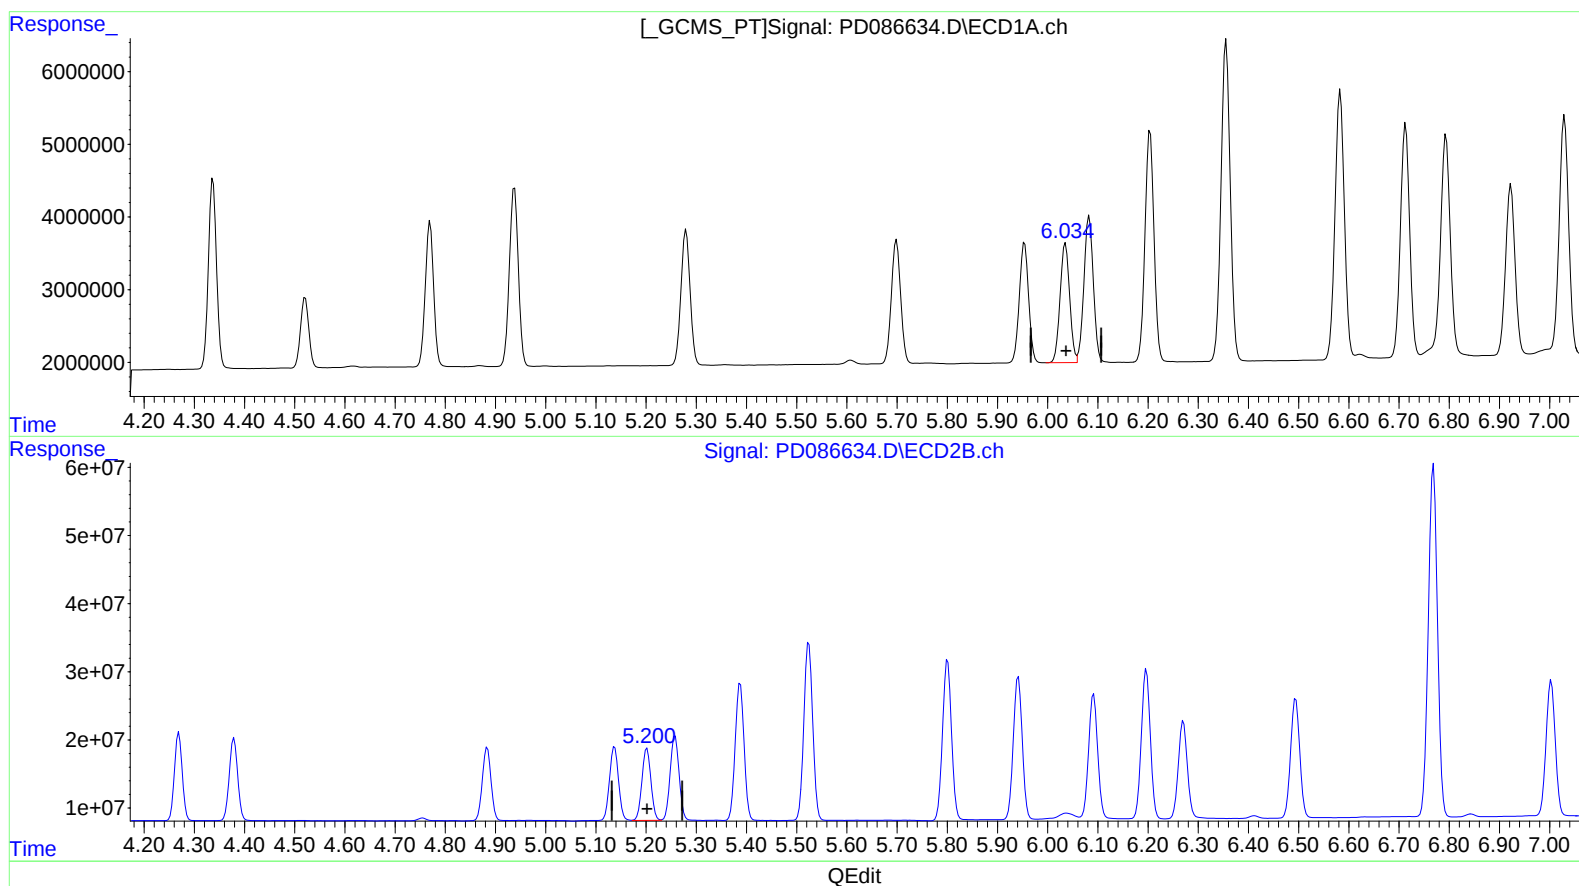

(11) cis-Chlordane (B)

6.036min 8.688 ng/ml

response 21810868

(11) cis-Chlordane #2 (B)

5.202min 9.312 ng/ml

response 131583798