

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
 Data File : PD086678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 23:53
 Operator : AR\AJ
 Sample : P4751-08MS
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9E6MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 04:28:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.886	11873828	89771662	7.907	8.634
27)	SA Decachlor...	9.093	8.088	27463846	112.5E6	12.411m	9.487m
Target Compounds							
2)	A alpha-BHC	4.007	3.400	70275728	396.6E6	24.447	24.456
3)	MA gamma-BHC...	4.337	3.737	72680287	385.8E6	25.652m	25.424
4)	MA Heptachlor	4.939	4.092	75512791	379.0E6	26.258	24.148m
5)	MB Aldrin	5.281	4.379	70429692	349.7E6	26.174	23.743
6)	B beta-BHC	4.521	4.032	25402695	140.0E6	20.479m	20.466
7)	B delta-BHC	4.773	4.270	88971551	266.5E6	31.476m	17.473 #
8)	B Heptachlo...	5.700	4.884	67656176	316.8E6	26.681	22.974
9)	A Endosulfan I	6.082	5.257	72523895	284.6E6	29.977m	21.621m#
10)	B trans-Chl...	5.953	5.136	68187750	335.0E6	27.490m	23.137m
11)	B cis-Chlor...	6.035	5.201	59508526	385.7E6	23.704m	27.296m
12)	B 4,4'-DDE	6.205	5.388	114.3E6	662.9E6	47.797	49.811
13)	MA Dieldrin	6.355	5.523	142.4E6	694.7E6	53.125m	49.617m
14)	MA Endrin	6.583	5.801	111.2E6	607.9E6	49.617	47.363
15)	B Endosulfa...	6.795	6.092	100.6E6	530.4E6	42.157	43.188
16)	A 4,4'-DDD	6.714	5.940	105.6E6	477.6E6	54.300	42.564m
17)	MA 4,4'-DDT	7.029	6.195	109.0E6	618.5E6	53.664m	51.834m
18)	B Endrin al...	6.923	6.269	81347410	368.0E6	46.662	38.771m
19)	B Endosulfa...	7.158	6.494	97810922	456.0E6	45.989	38.561
20)	A Methoxychlor	7.502	6.767	258.1E6	1153.8E6	227.059	210.052m
21)	B Endrin ke...	7.639	7.003	119.4E6	456.6E6	49.007	34.756 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111424\
Data File : PD086678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 23:53
Operator : AR\AJ
Sample : P4751-08MS
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 04:28:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

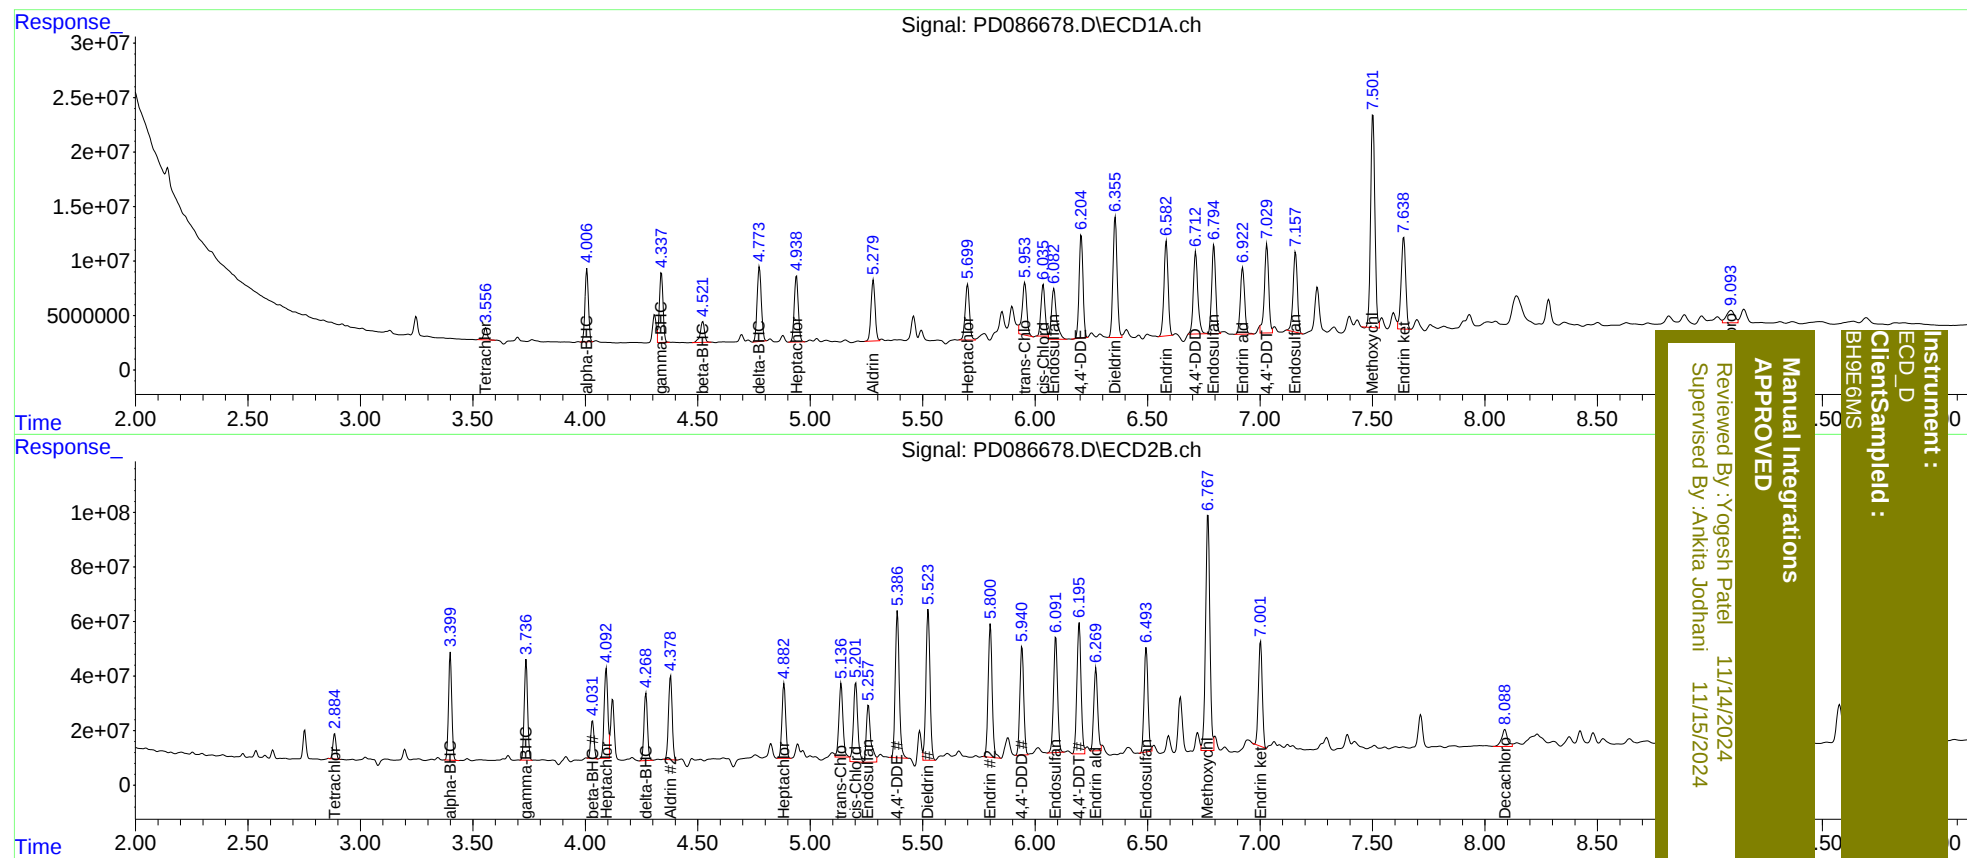

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/14/2024
Supervised By : Ankita Jodhani 11/15/2024

Instrument :
ECD_D
Client Sampled :
BH9E6MS