

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111425\
 Data File : PD091166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2025 11:02
 Operator : AR\AJ
 Sample : Q3609-07DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-713-COMP-03DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 11:27:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.689	4.862	77117523	596.2E6	13.321m 13.984
10) B	gamma-Chl...	5.947	5.115	352.2E6	2279.4E6	59.385 50.710
11) B	alpha-Chl...	6.030	5.179	491.6E6	2843.6E6	79.546 65.920



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111425\
Data File : PD091166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2025 11:02
Operator : AR\AJ
Sample : Q3609-07DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 11:27:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

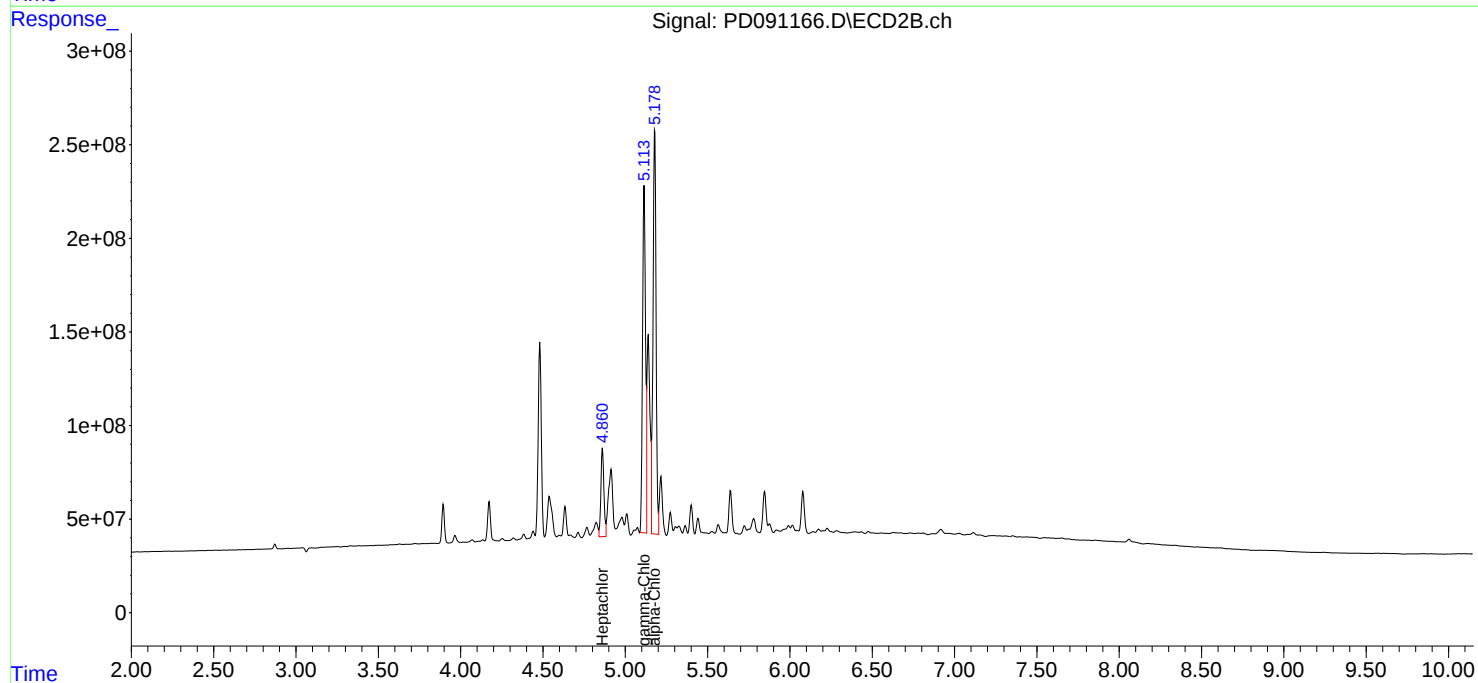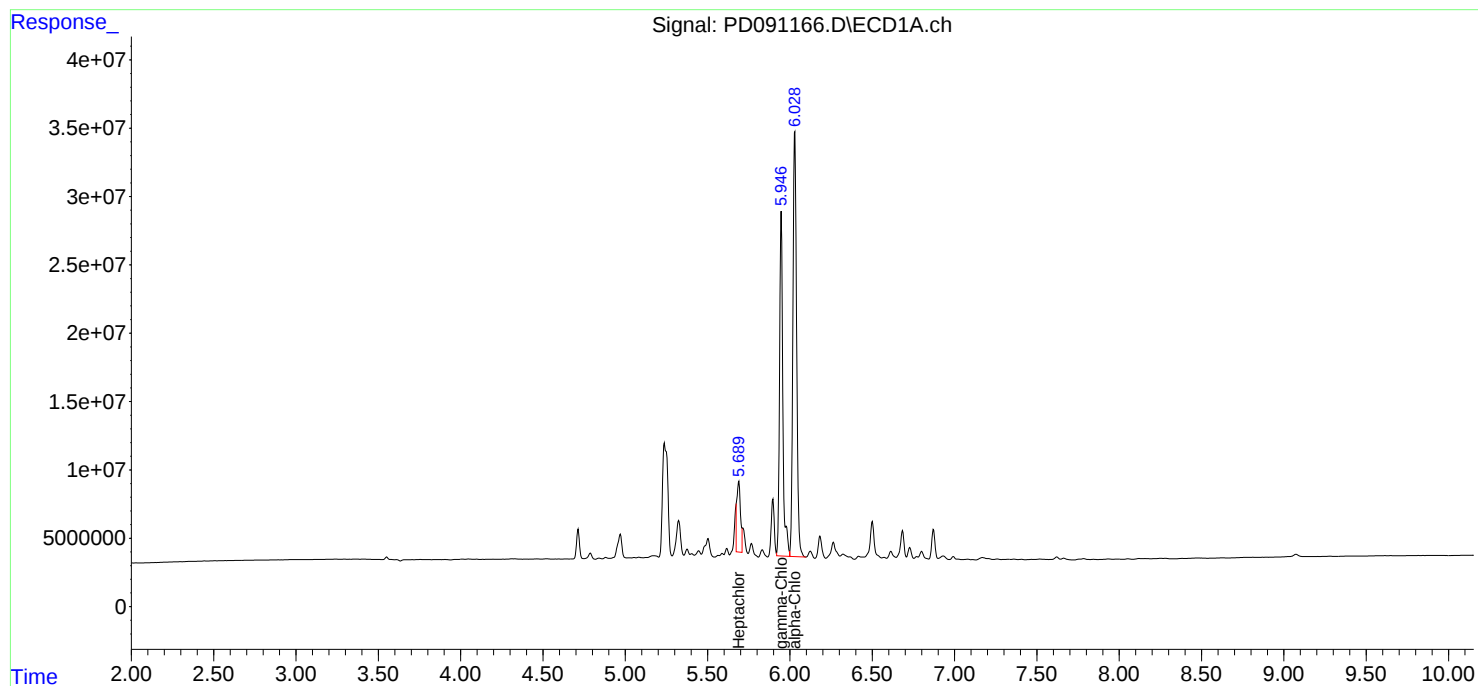


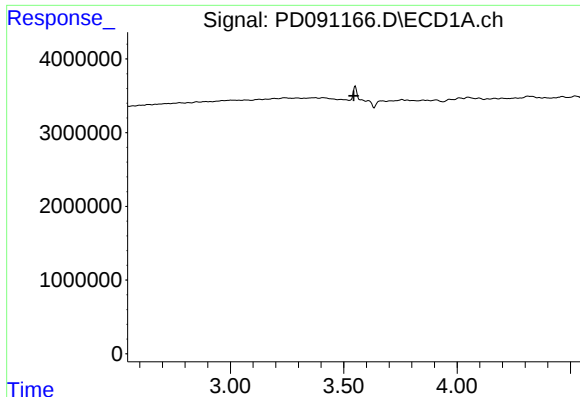

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03DL

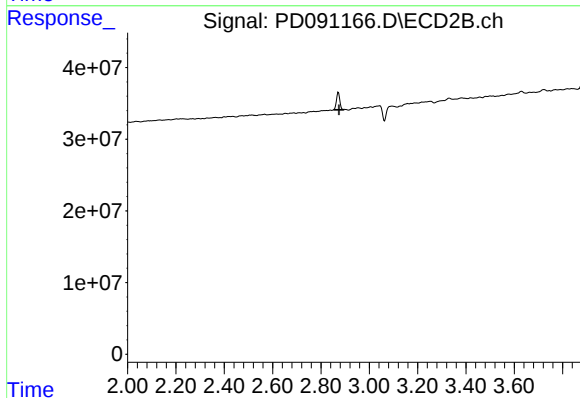


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.875 min
Response: 0
Conc: N.D.

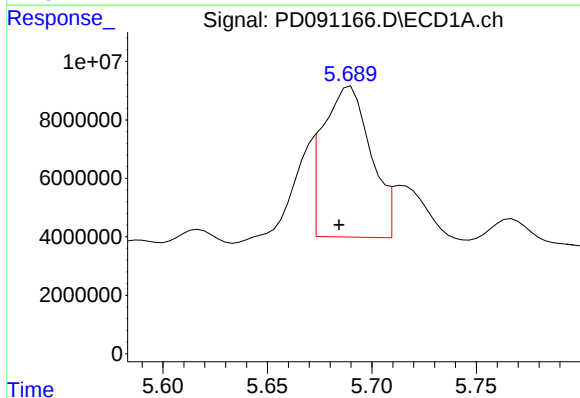


#8 Heptachlor epoxide

R.T.: 5.689 min
Delta R.T.: 0.004 min
Response: 77117523
Conc: 13.32 ng/ml m

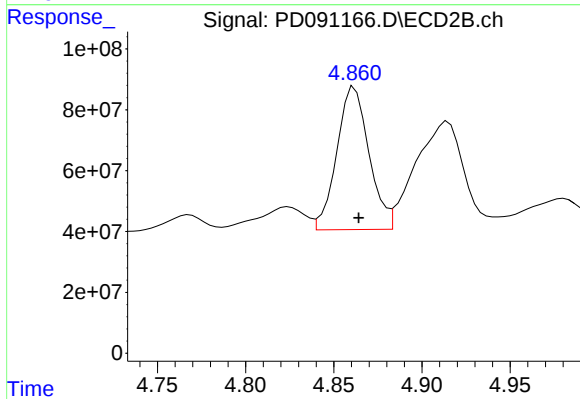

#8 Heptachlor epoxide


R.T.: 4.862 min
Delta R.T.: -0.002 min
Response: 596244470
Conc: 13.98 ng/ml

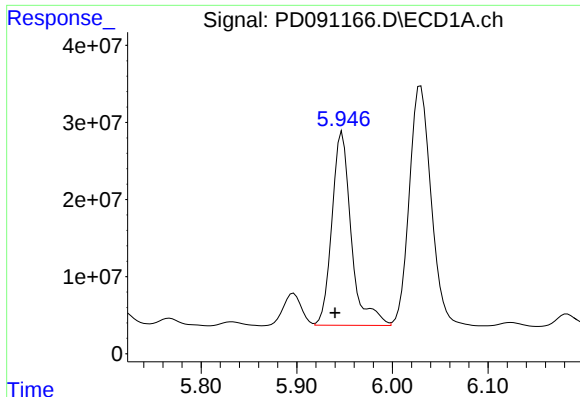

#10 gamma-Chlordane


R.T.: 5.947 min
Delta R.T.: 0.007 min
Response: 352225628
Conc: 59.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03DL

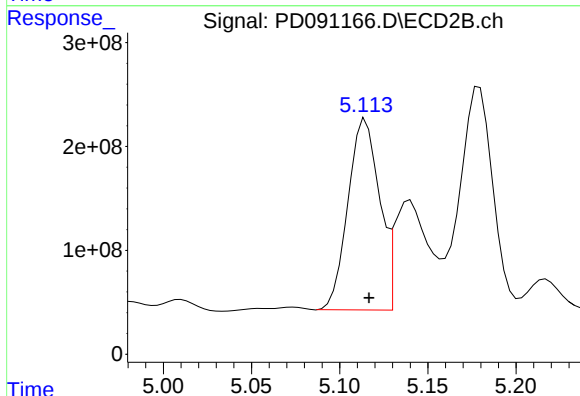


#10 gamma-Chlordane

R.T.: 5.115 min
Delta R.T.: -0.002 min
Response: 2279366666
Conc: 50.71 ng/ml

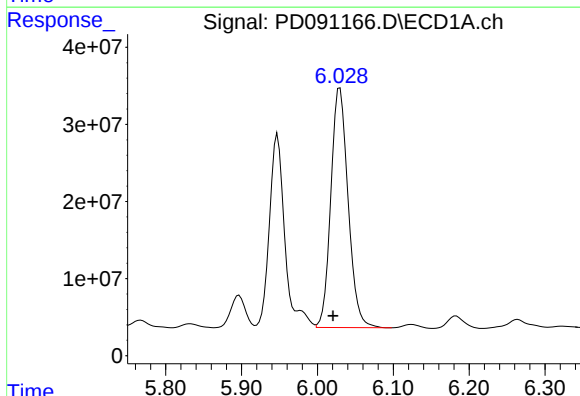


#11 alpha-Chlordane

R.T.: 6.030 min
Delta R.T.: 0.009 min
Response: 491616180
Conc: 79.55 ng/ml

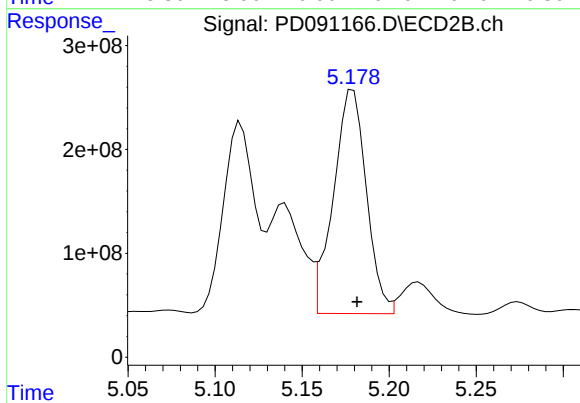

#11 alpha-Chlordane


R.T.: 5.179 min
Delta R.T.: -0.002 min
Response: 2843646086
Conc: 65.92 ng/ml

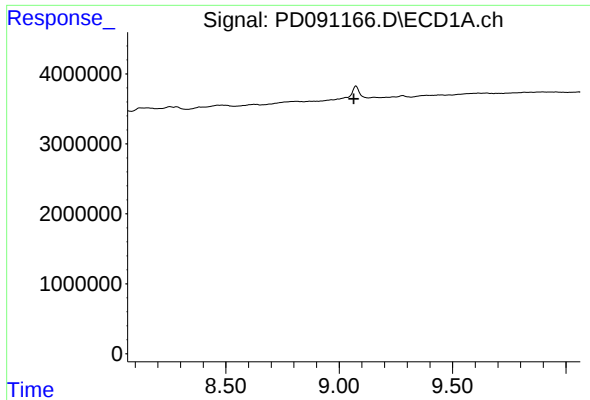

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
AU-713-COMP-03DL

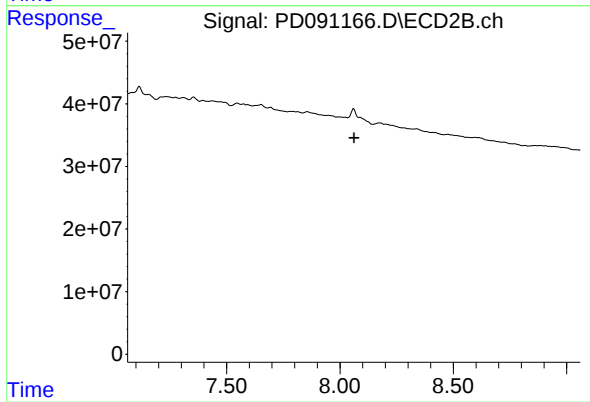

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.