

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111425\
 Data File : PD091167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2025 11:16
 Operator : AR\AJ
 Sample : Q3621-02DL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VNJ-231DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 11:36:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.872	6765148	79363648	2.172m	2.665
28)	SA Decachlor...	9.067	8.055	13997150	90600628	2.992	2.991m
Target Compounds							
4)	MA Heptachlor	4.921	4.071	8307175	75880152	1.486	1.701
8)	B Heptachlo...	5.680	4.861	49214717	391.2E6	8.501m	9.174
10)	B gamma-Chl...	5.939	5.113	264.7E6	1956.5E6	44.630	43.527
11)	B alpha-Chl...	6.020	5.178	387.9E6	2506.9E6	62.771	58.115
13)	MA Dieldrin	6.339	5.499	17207410	184.7E6	2.951	4.181m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111425\
Data File : PD091167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2025 11:16
Operator : AR\AJ
Sample : Q3621-02DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
VNJ-231DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 11:36:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

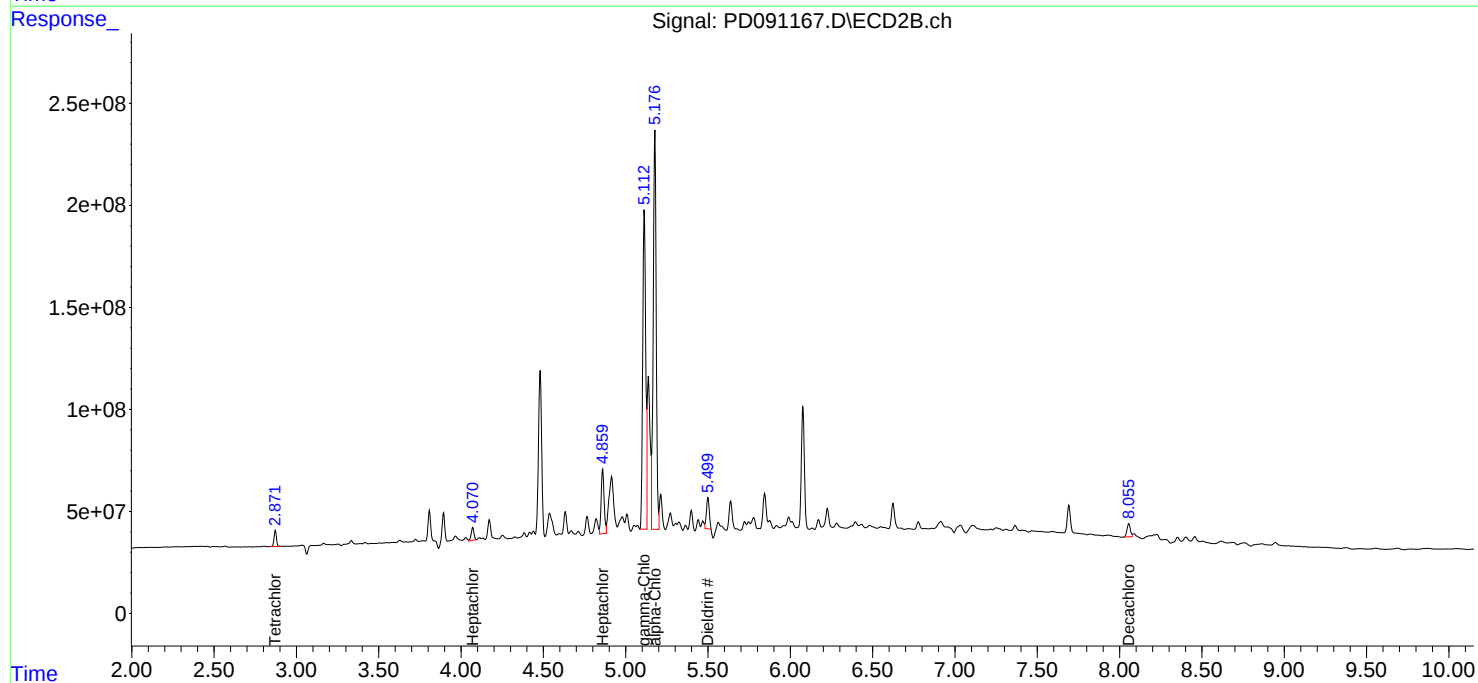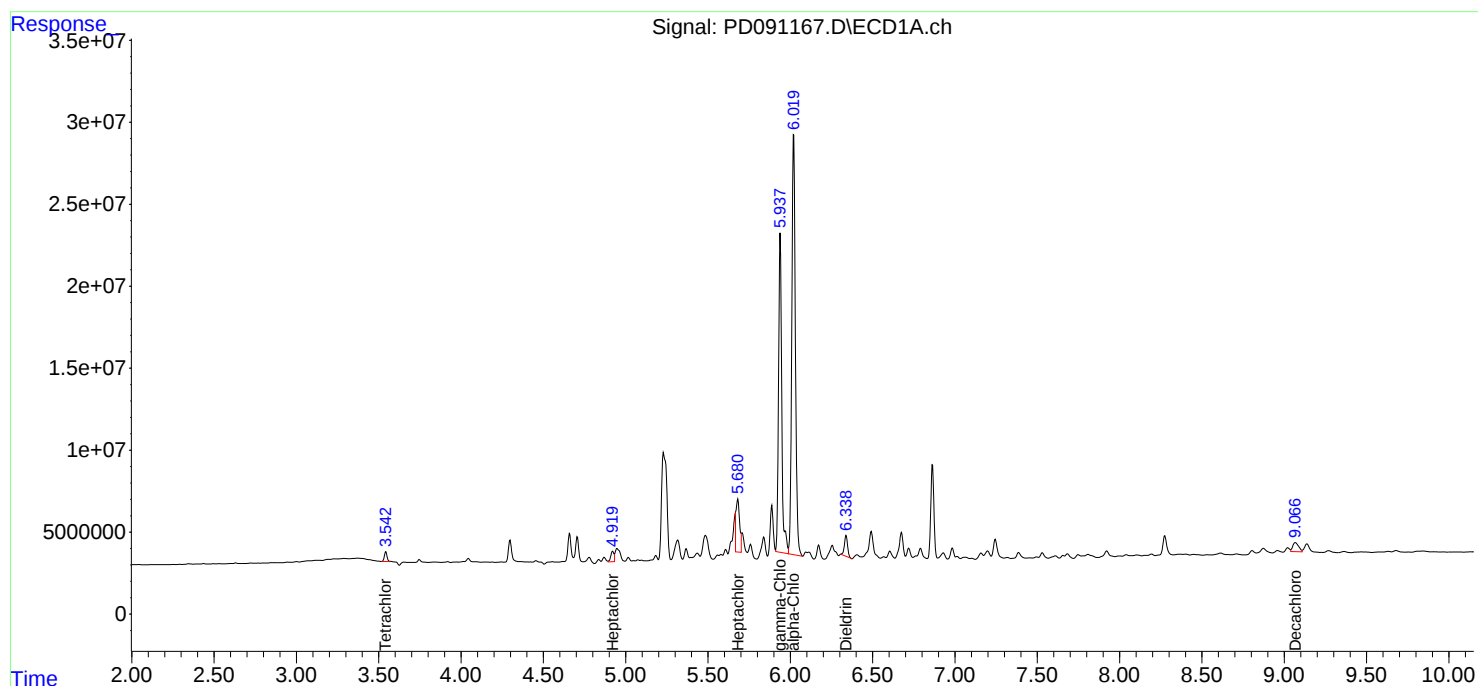


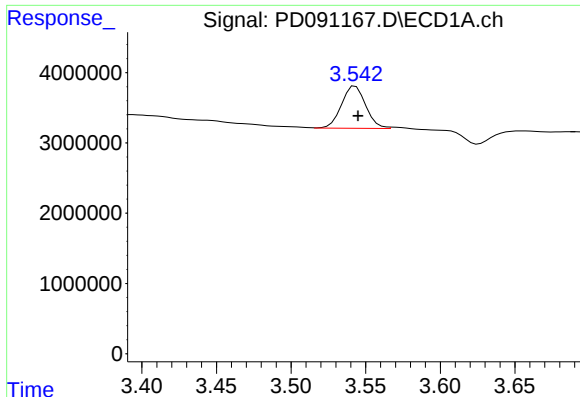

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.003 min
Response: 6765148
Conc: 2.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-231DL

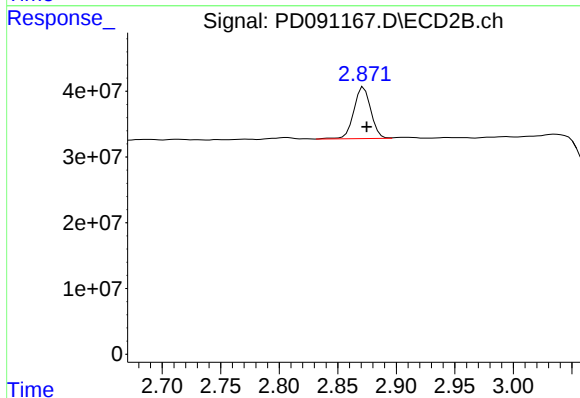


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.003 min
Response: 79363648
Conc: 2.67 ng/ml

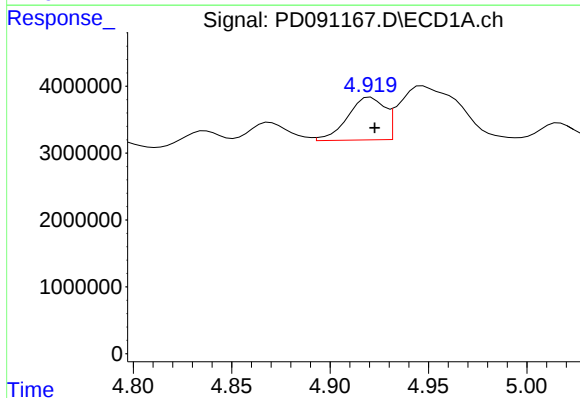


#4 Heptachlor

R.T.: 4.921 min
Delta R.T.: -0.002 min
Response: 8307175
Conc: 1.49 ng/ml

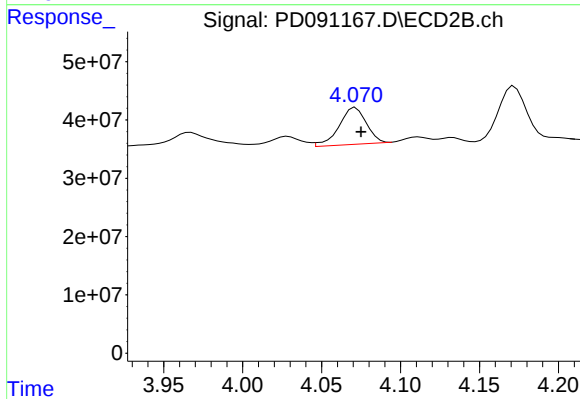

#4 Heptachlor


R.T.: 4.071 min
Delta R.T.: -0.003 min
Response: 75880152
Conc: 1.70 ng/ml

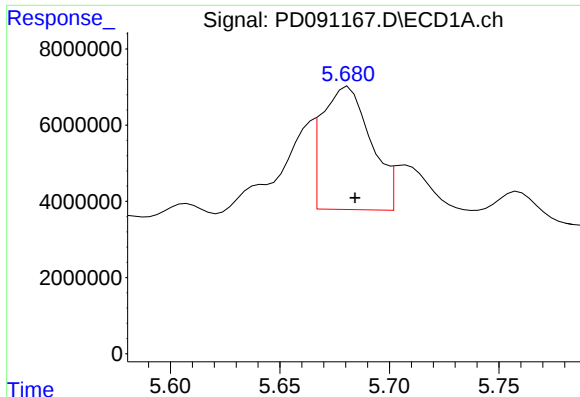

#8 Heptachlor epoxide


R.T.: 5.680 min
Delta R.T.: -0.004 min
Response: 49214717
Conc: 8.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-231DL

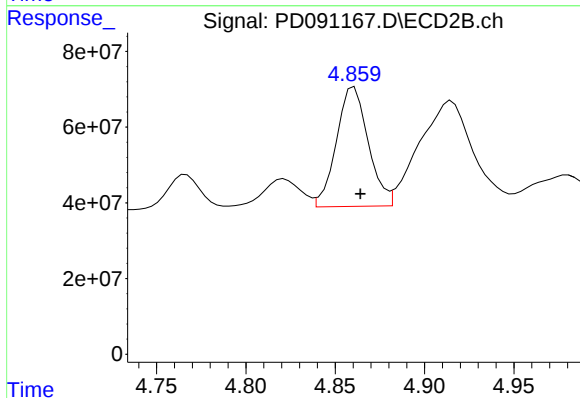


#8 Heptachlor epoxide

R.T.: 4.861 min
Delta R.T.: -0.003 min
Response: 391188687
Conc: 9.17 ng/ml

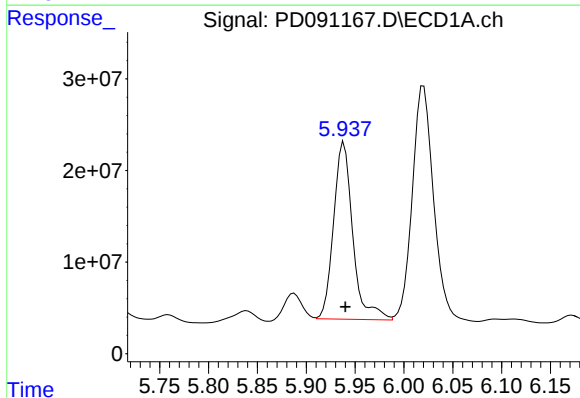


#10 gamma-Chlordane

R.T.: 5.939 min
Delta R.T.: -0.002 min
Response: 264706750
Conc: 44.63 ng/ml

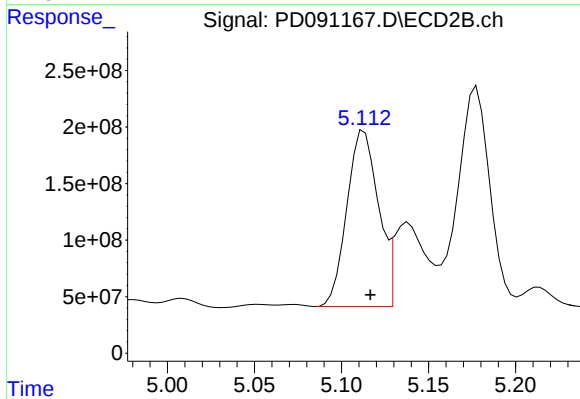

#10 gamma-Chlordane


R.T.: 5.113 min
Delta R.T.: -0.004 min
Response: 1956507802
Conc: 43.53 ng/ml

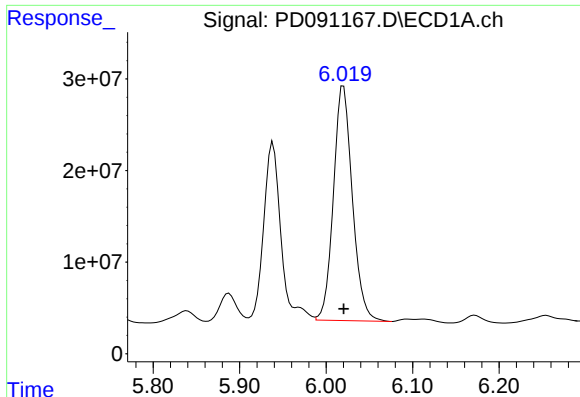

#11 alpha-Chlordane


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 387938746
Conc: 62.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-231DL

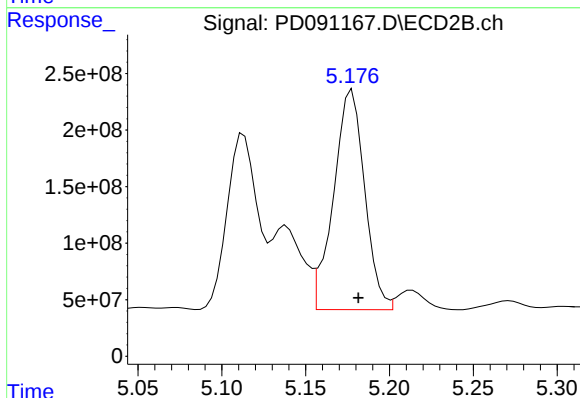


#11 alpha-Chlordane

R.T.: 5.178 min
Delta R.T.: -0.004 min
Response: 2506948179
Conc: 58.11 ng/ml

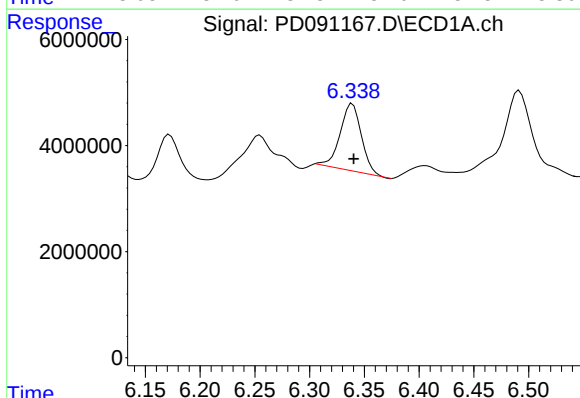


#13 Dieldrin

R.T.: 6.339 min
Delta R.T.: -0.001 min
Response: 17207410
Conc: 2.95 ng/ml

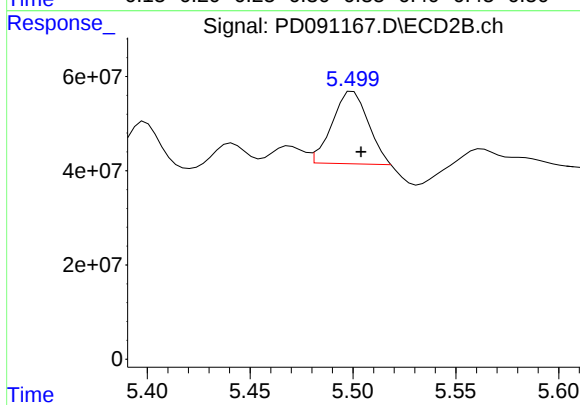

#13 Dieldrin


R.T.: 5.499 min
Delta R.T.: -0.005 min
Response: 184718351
Conc: 4.18 ng/ml m

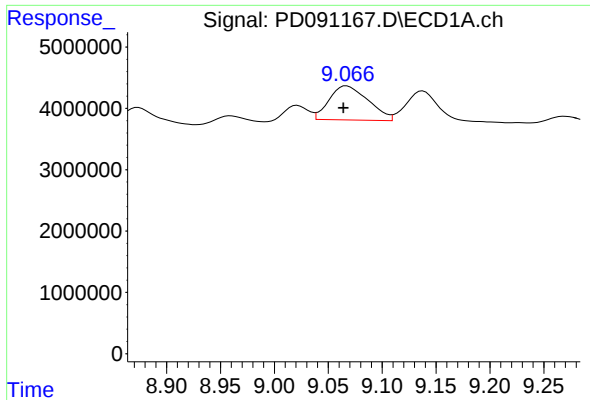

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.003 min
Response: 13997150
Conc: 2.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-231DL

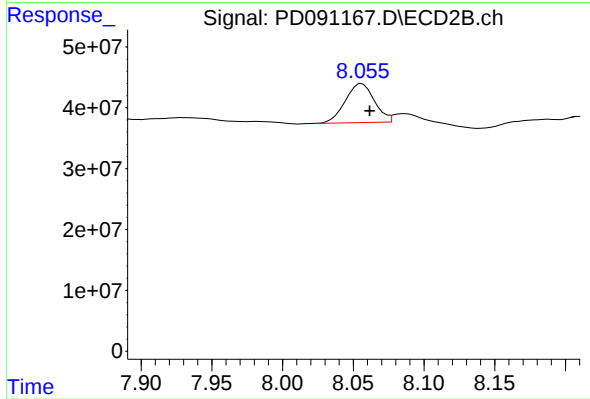

#28 Decachlorobiphenyl

R.T.: 8.055 min
Delta R.T.: -0.007 min
Response: 90600628
Conc: 2.99 ng/ml m