

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
 Data File : PD056015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 08:55
 Operator : SG\AJ
 Sample : PIBLK22
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK22

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:13:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.290	3.962	19498558	25815315	25.902	24.634
27) SA Decachlor...	7.965	8.996	37713722	45045073	46.268	39.668
Target Compounds						
8) B Heptachlo...	0.000	5.817	0	12496109	N.D.	9.260


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
Data File : PD056015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 08:55
Operator : SG\AJ
Sample : PIBLK22
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:13:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

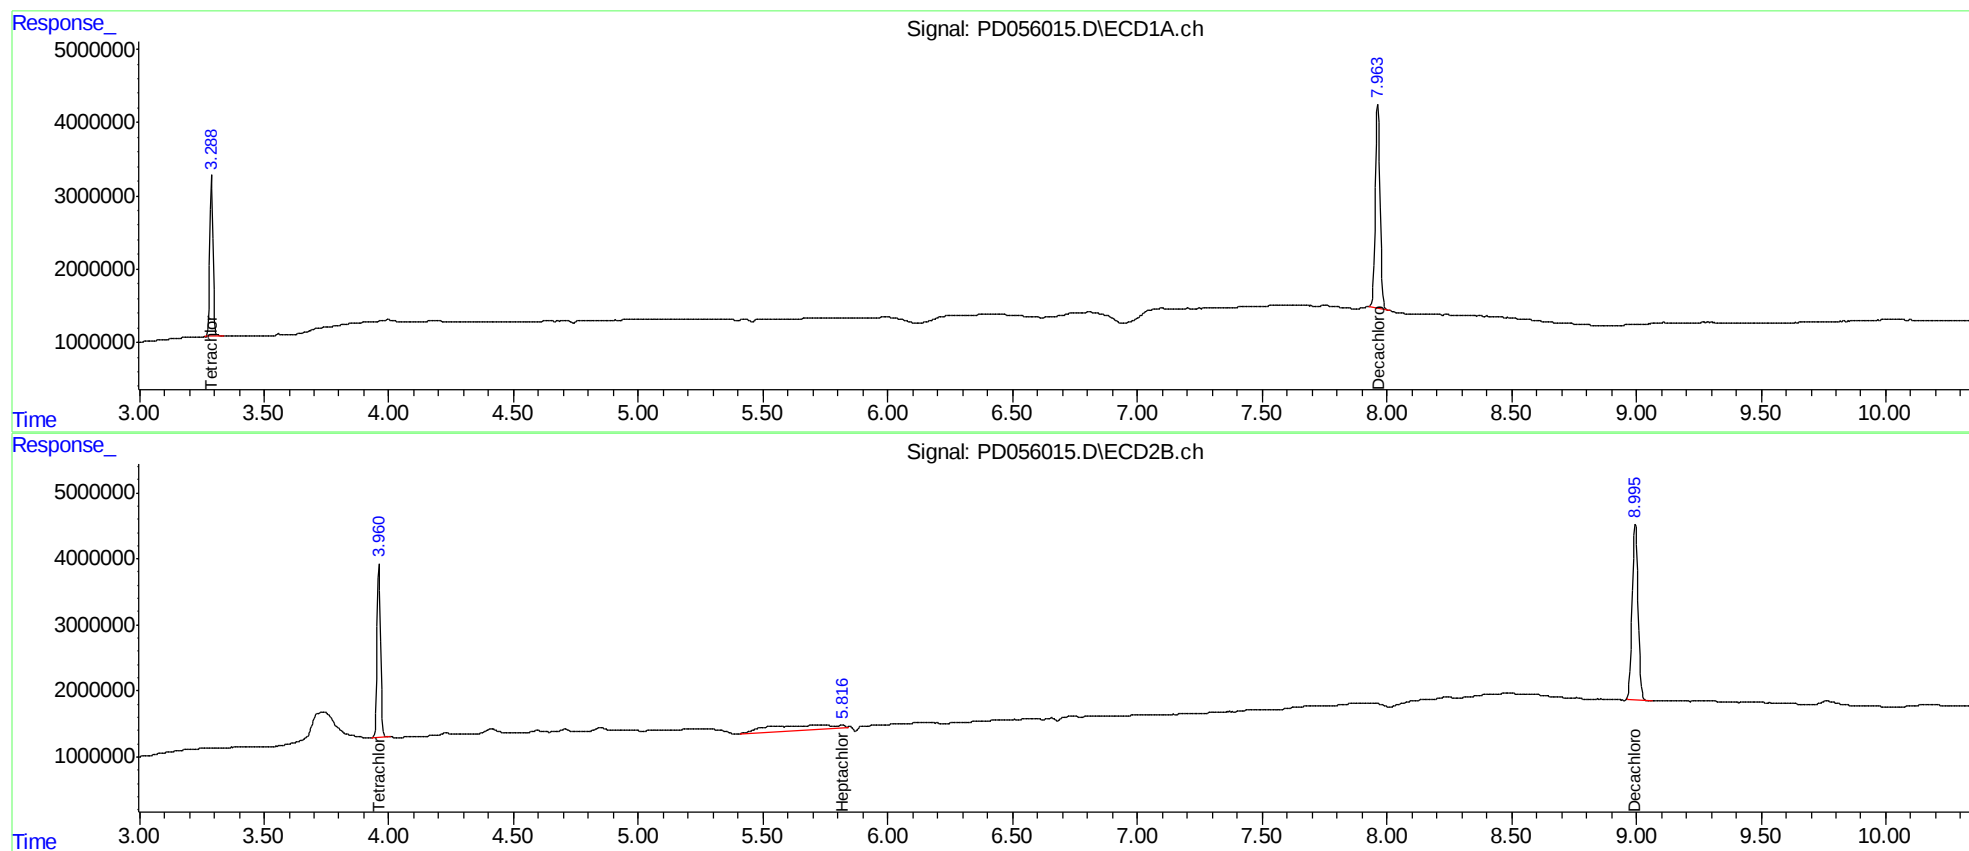


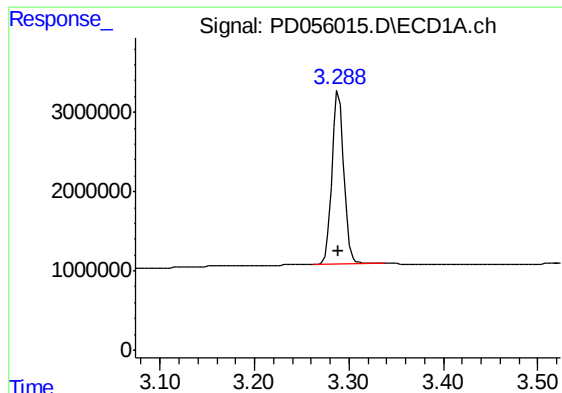

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 19498558
Conc: 25.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK22

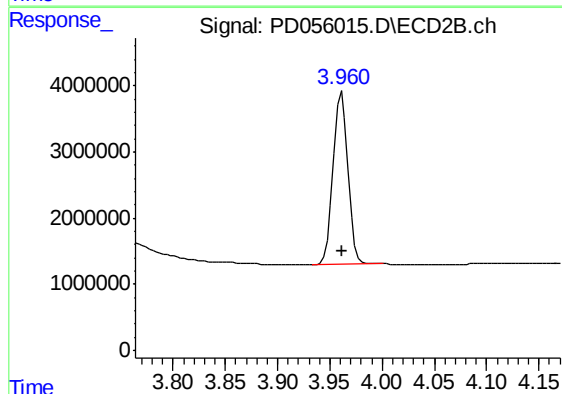


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 25815315
Conc: 24.63 ng/ml

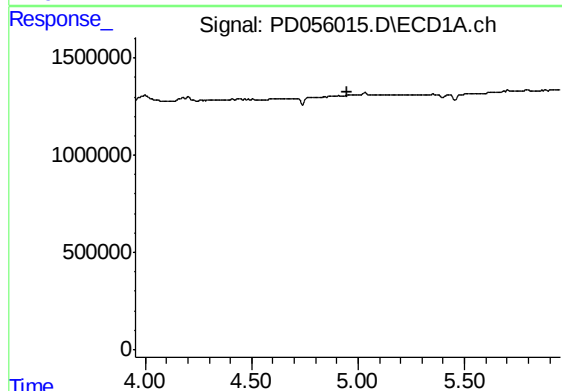


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

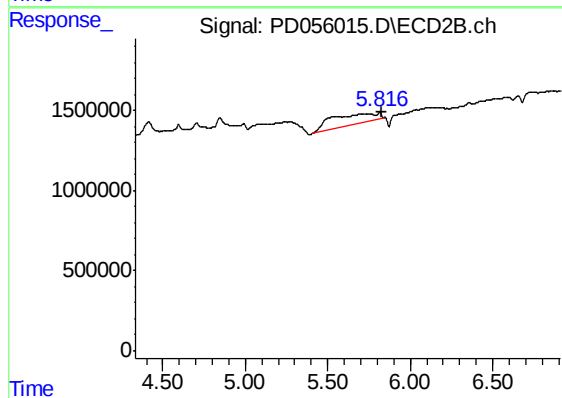

#8 Heptachlor epoxide


R.T.: 5.817 min
Delta R.T.: -0.007 min
Response: 12496109
Conc: 9.26 ng/ml

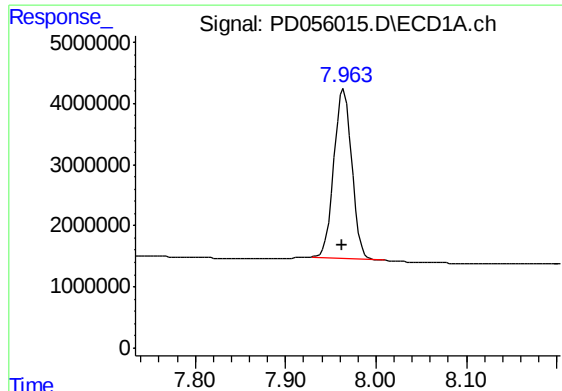

#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.002 min
Response: 37713722
Conc: 46.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK22

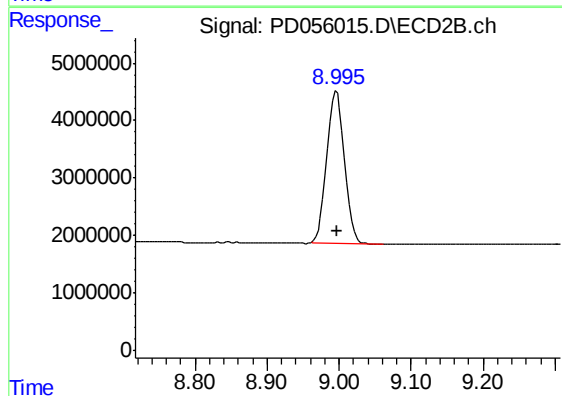

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 45045073
Conc: 39.67 ng/ml