

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
 Data File : PD056028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 12:38
 Operator : SG\AJ
 Sample : K5783-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AY1

Manual Integrations
 APPROVED

Ankita
 11/18/2019 2:56:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:16:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.287	3.960	20801004	20015238	27.632m	19.099m#
27) SA Decachlor...	7.963	8.996	30755125	38149110	37.731	33.595m
Target Compounds						
3) MA gamma-BHC...	3.997	4.610	9321380	8339380	9.113	5.919m#
14) MA Endrin	5.776	6.648	1082379	2854374	1.349m	2.479m#
16) A 4,4'-DDD	5.914	6.769	9210357	10736191	13.041m	9.615m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
Data File : PD056028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 12:38
Operator : SG\AJ
Sample : K5783-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:16:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

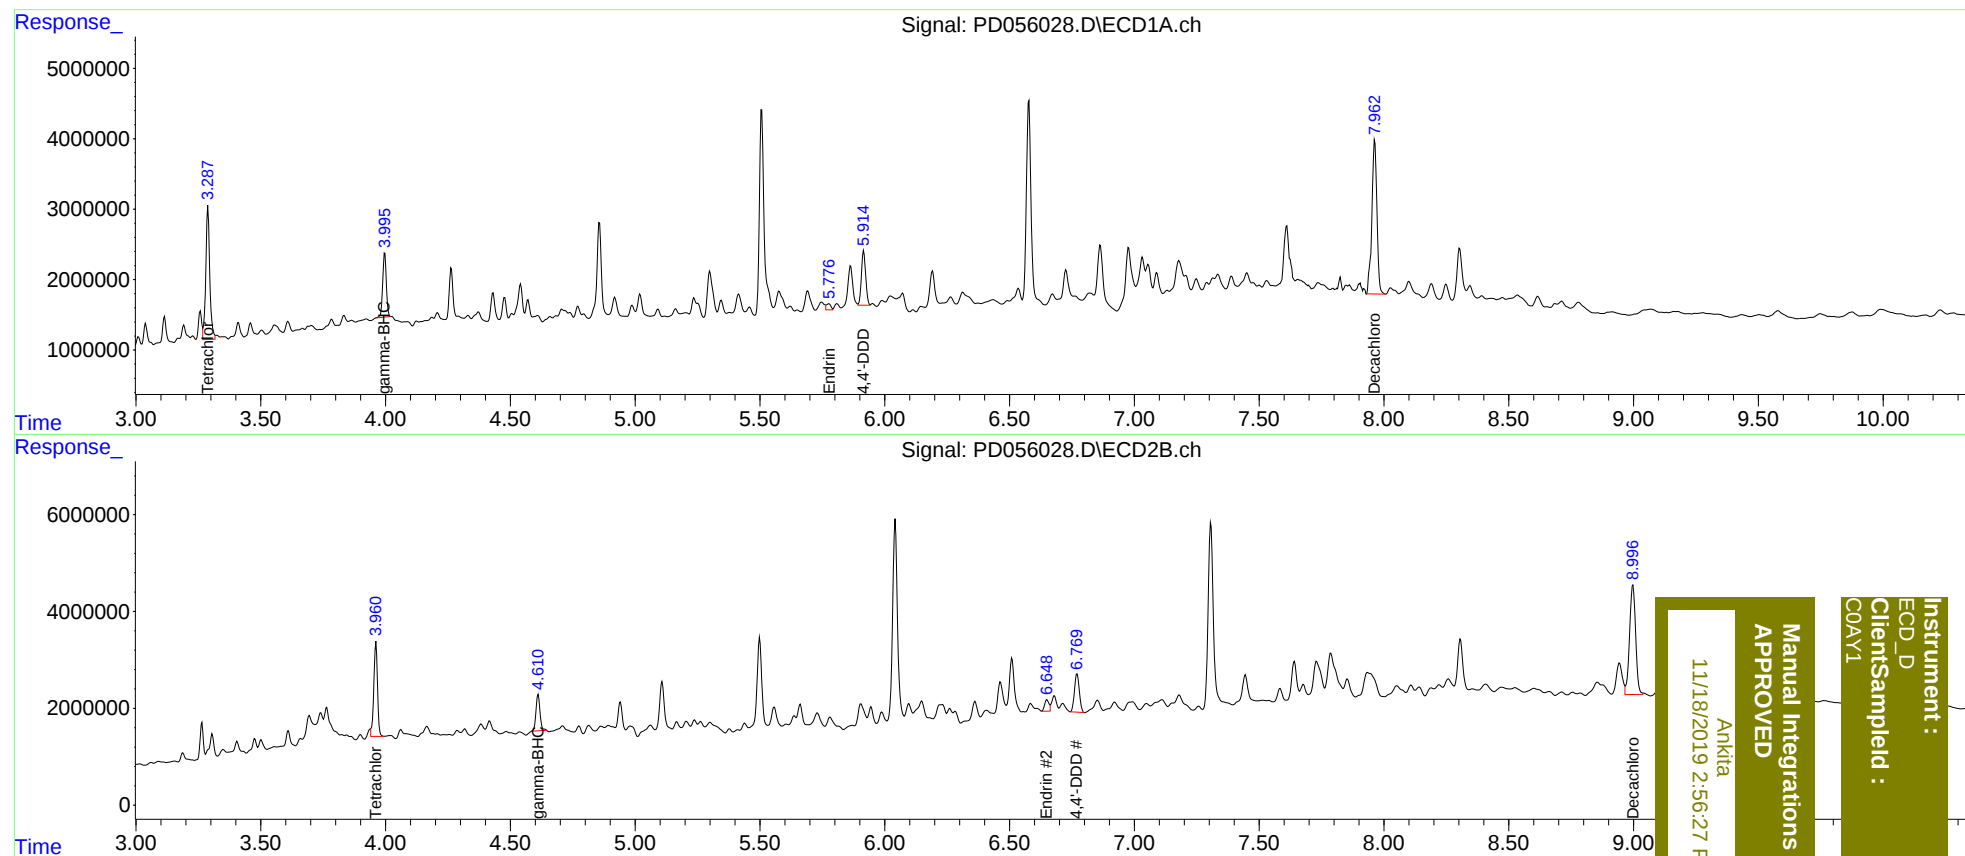

11/18/2019 2:56:27 PM

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0A71