

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
 Data File : PD056040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 16:42
 Operator : SG\AJ
 Sample : K5783-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AY3

Manual Integrations
 APPROVED

Ankita
 11/18/2019 2:56:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:20:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	19883044	19654963	26.413m	18.756m#
27)	SA Decachlor...	7.964	8.996	26714217	34271846	32.774	30.181m
Target Compounds							
3)	MA gamma-BHC...	3.997	4.611	11205061	8730813	10.955	6.197m#
14)	MA Endrin	5.775	6.651	2258989	4276762	2.816m	3.715m#
15)	B Endosulfa...	6.056	6.853	5809927	5702139	6.895m	4.403 #
16)	A 4,4'-DDD	5.914	6.770	11841318	16641456	16.766m	14.903m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
Data File : PD056040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 16:42
Operator : SG\AJ
Sample : K5783-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:20:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

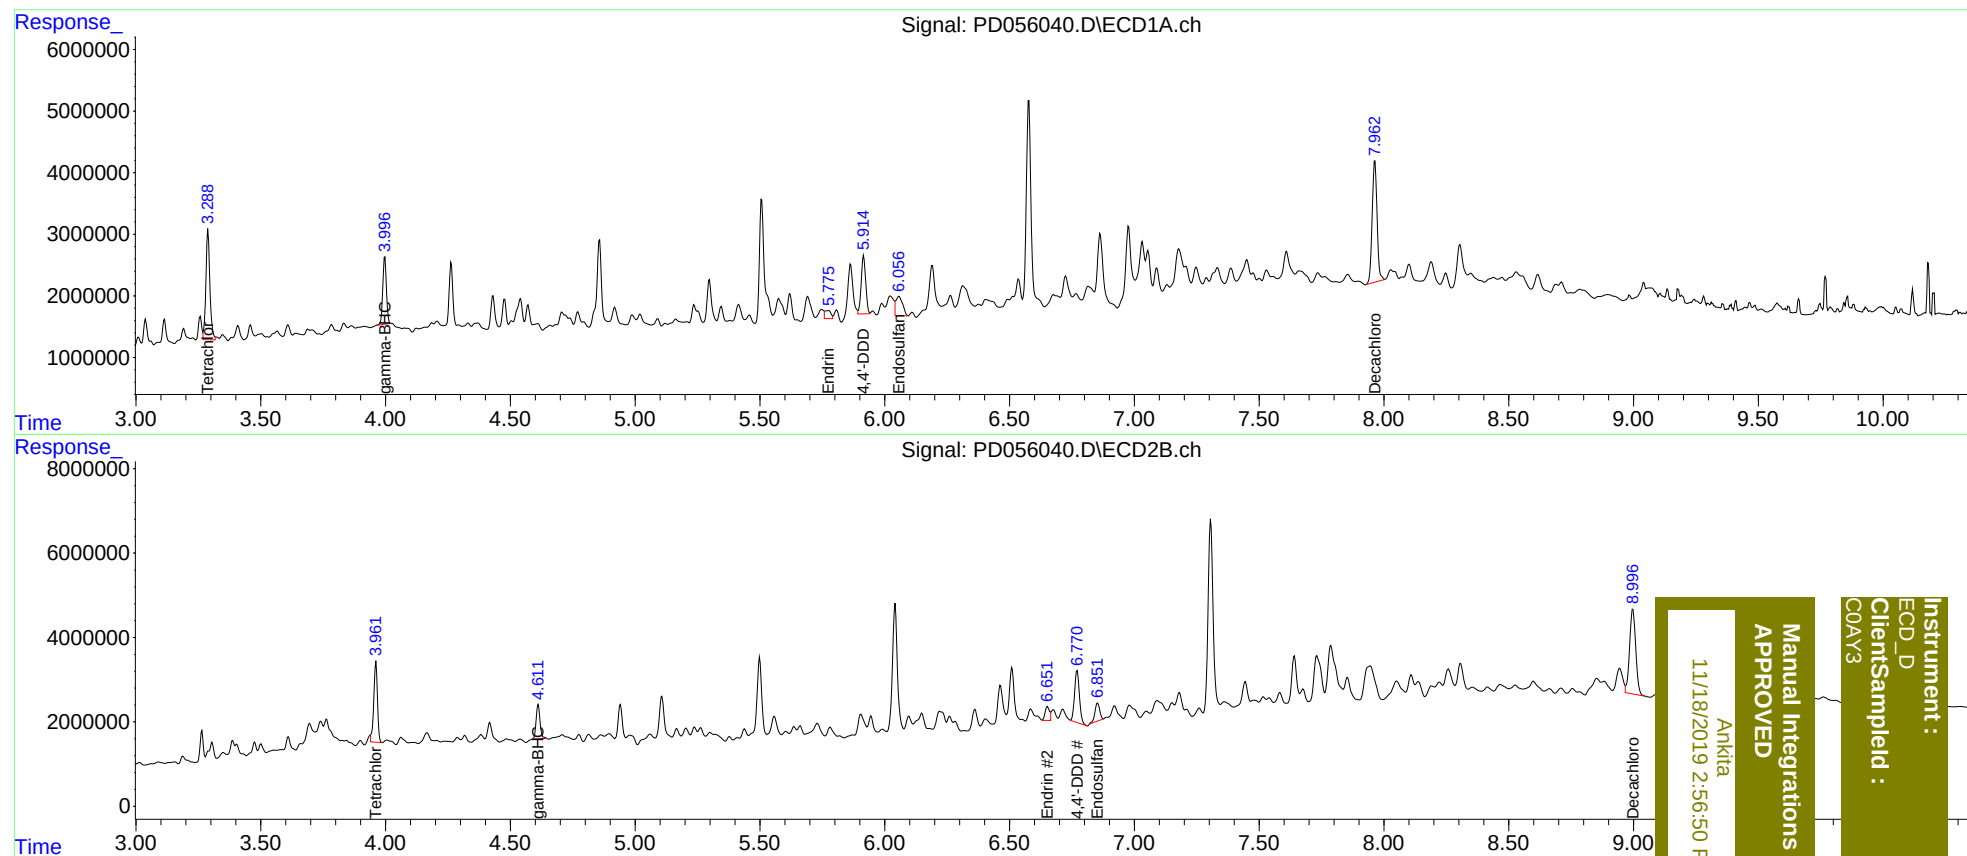

11/18/2019 2:56:50 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSample :
C0AY3