

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
 Data File : PD056042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2019 17:38
 Operator : SG\AJ
 Sample : K5783-21
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ6

Manual Integrations
 APPROVED

Ankita
 11/18/2019 2:56:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:21:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.287	3.962	16643796	18468289	22.110m	17.623
27) SA Decachlor...	7.963	8.996	25917073	31399770	31.796	27.651m
Target Compounds						
3) MA gamma-BHC...	3.997	4.611	7815020	6647664	7.640	4.718m#
14) MA Endrin	5.777	6.649	1014156	1758940	1.264m	1.528m
16) A 4,4'-DDD	5.915	6.769	4509392	5826626	6.385m	5.218m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111519\
Data File : PD056042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2019 17:38
Operator : SG\AJ
Sample : K5783-21
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:21:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

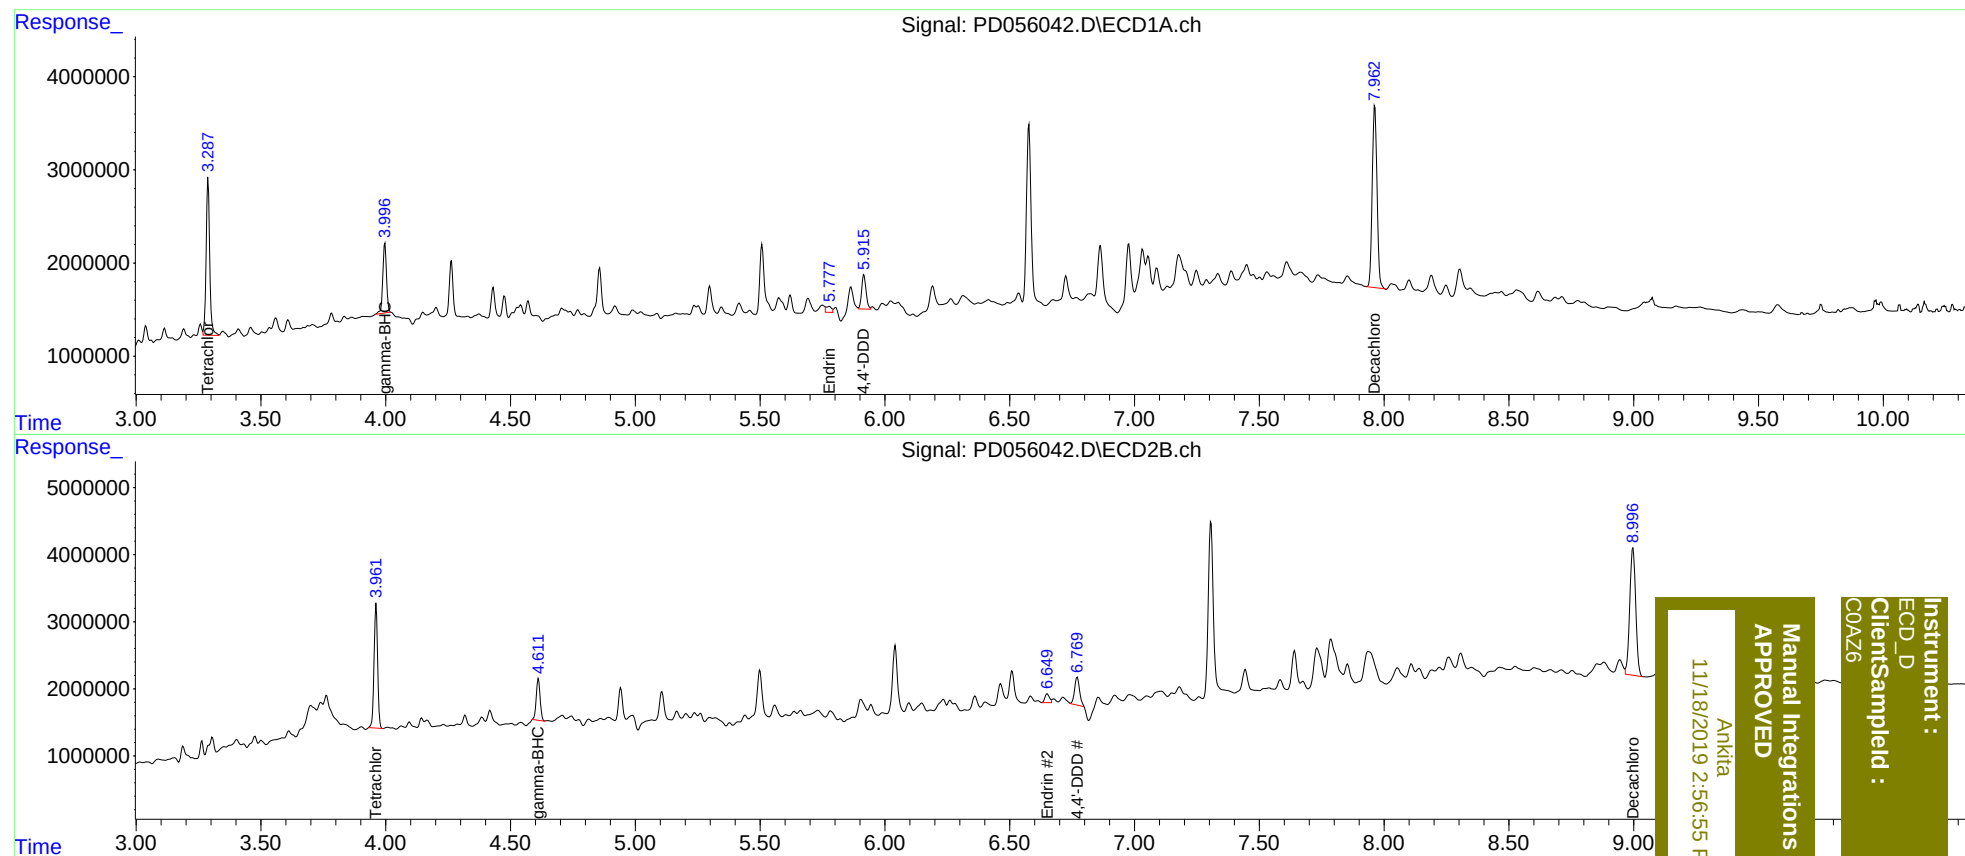

Manual Integrations
APPROVED

Ankita
11/18/2019 2:56:55 PM

Instrument :
ECD_D
Client Sampled :
C0A26