

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
 Data File : PD066927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 13:33
 Operator : AR\AJ
 Sample : PB140759BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 06:15:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	36007226	173.1E6	19.298	21.393
28)	SA Decachlor...	8.165	9.029	20957581	101.5E6	18.139	18.850
Target Compounds							
6)	B beta-BHC	0.000	4.841f	0	1240190	N.D.	0.266 #
9)	A Endosulfan I	0.000	6.190	0	348951	N.D.	0.044 #
11)	B alpha-Chl...	0.000	6.157	0	1142793	N.D.	0.138 #
12)	B 4,4'-DDE	0.000	6.327f	0	5355814	N.D.	0.680 #
14)	MA Endrin	0.000	6.683	0	114419	N.D.	0.017 #
15)	B Endosulfa...	0.000	6.888	0	3788659	N.D.	0.537 #
21)	B Endrin ke...	0.000	7.703	0	2342034	N.D.	0.278 #
22)	Mirex	0.000	8.184f	0	1067071	N.D.	0.180 #
26)	Chlordane-4	0.000	6.157	0	1142793	N.D.	0.907 #
27)	Chlordane-5	0.000	6.932f	0	430509	N.D.	1.580 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
Data File : PD066927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 13:33
Operator : AR\AJ
Sample : PB140759BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 06:15:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

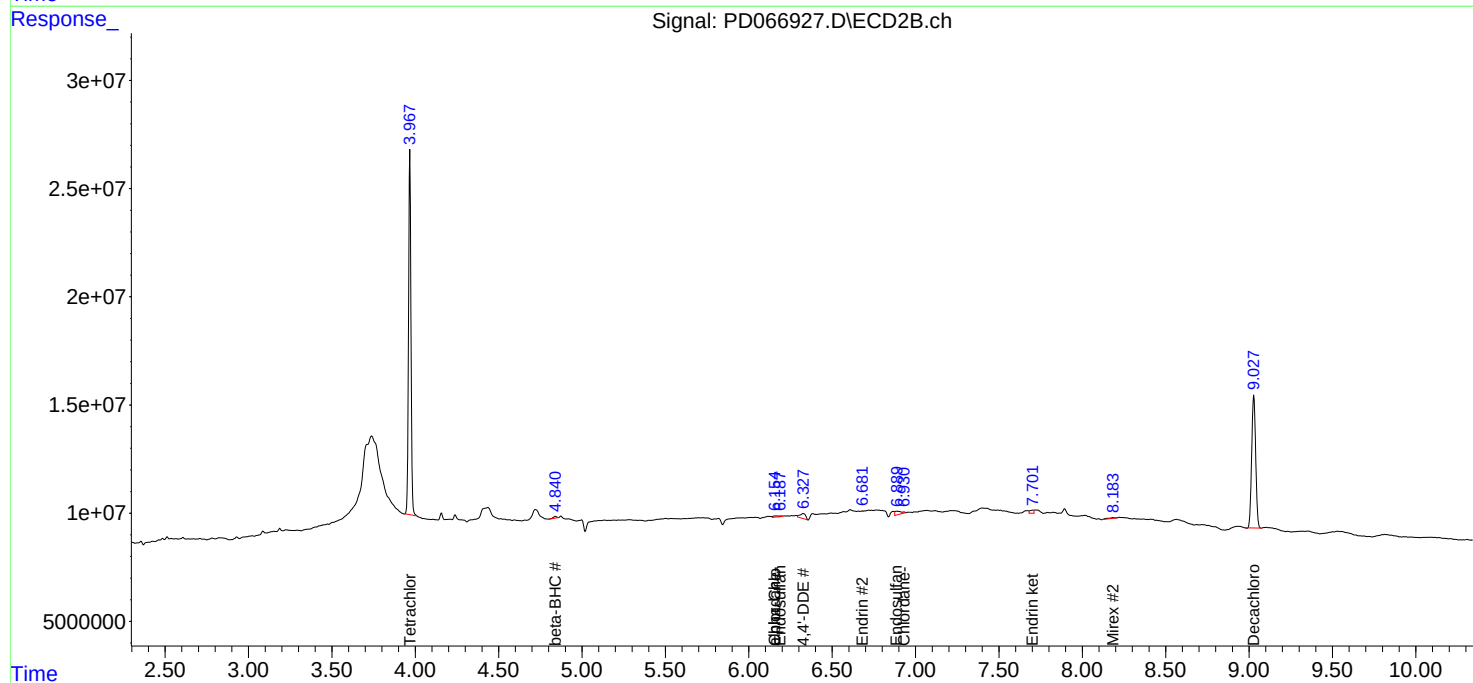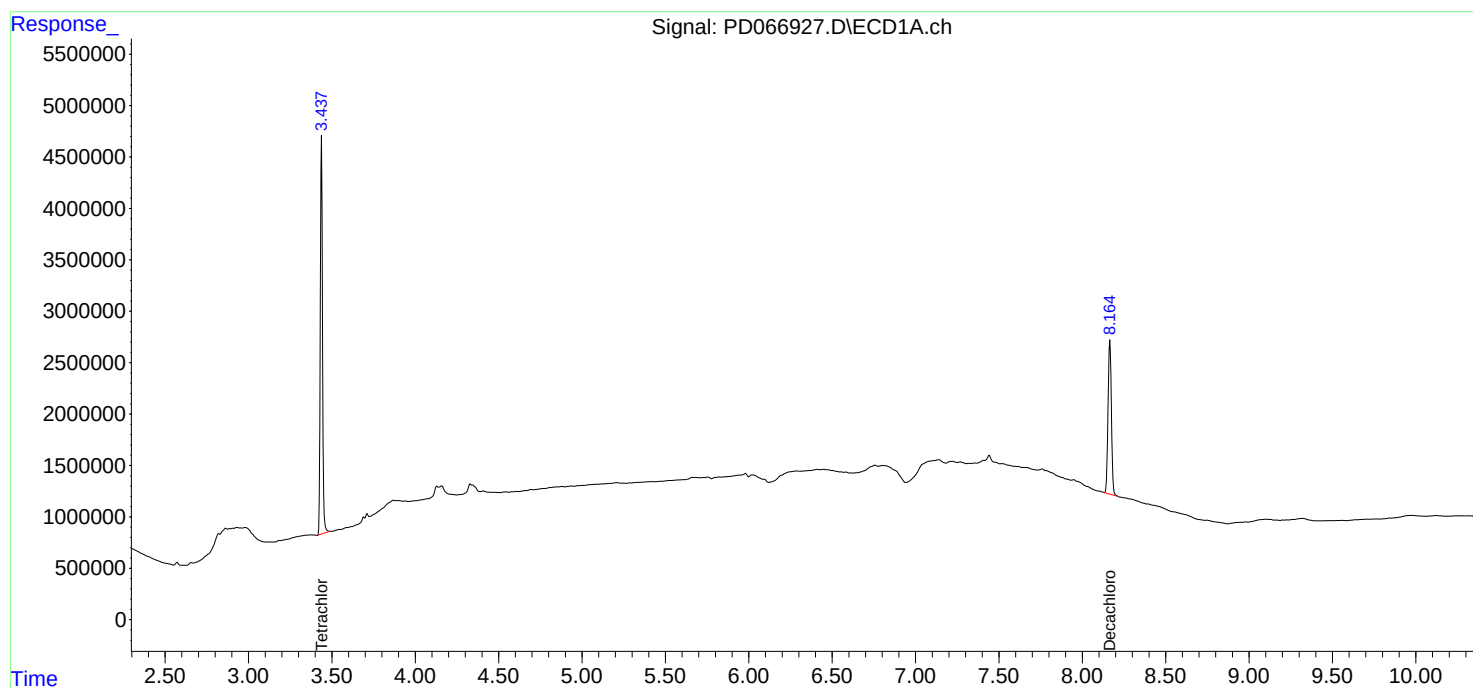


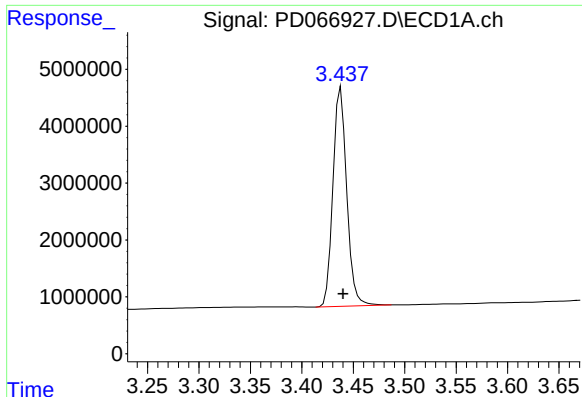

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 36007226
Conc: 19.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

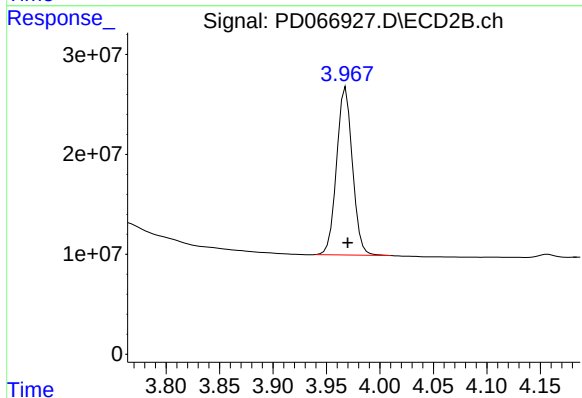


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 173113231
Conc: 21.39 ng/ml

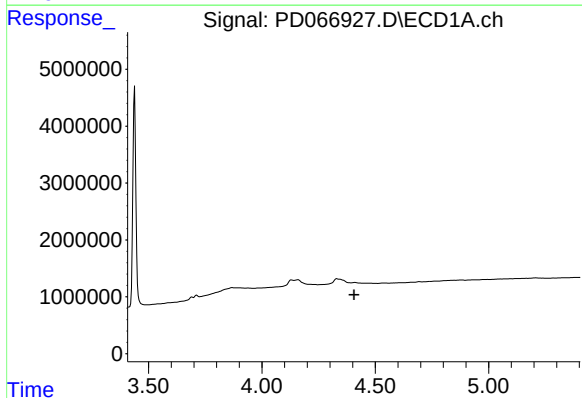


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.406 min
Response: 0
Conc: N.D.

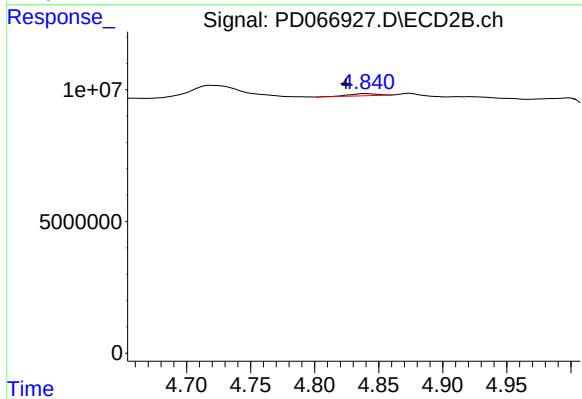

#6 beta-BHC


R.T.: 4.841 min
Delta R.T.: 0.016 min
Response: 1240190
Conc: 0.27 ng/ml

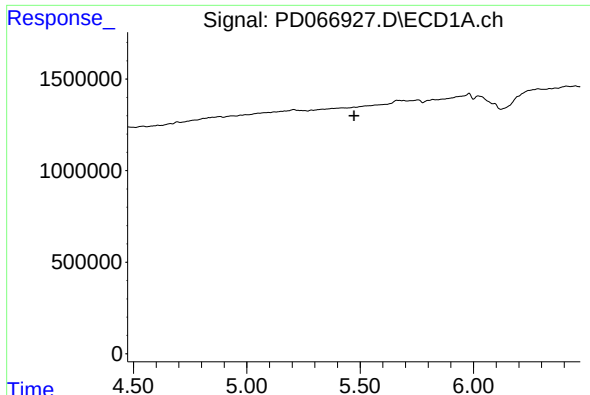

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

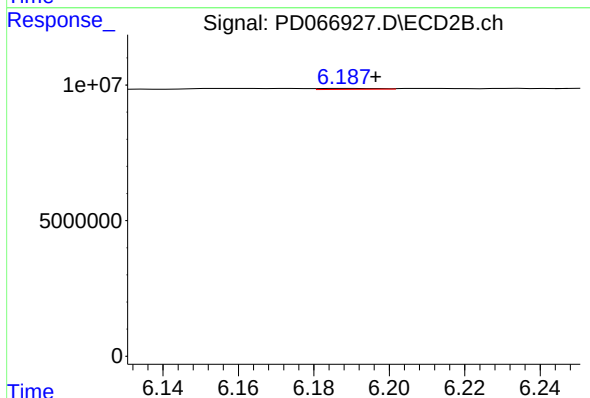


#9 Endosulfan I

R.T.: 6.190 min
Delta R.T.: -0.007 min
Response: 348951
Conc: 0.04 ng/ml

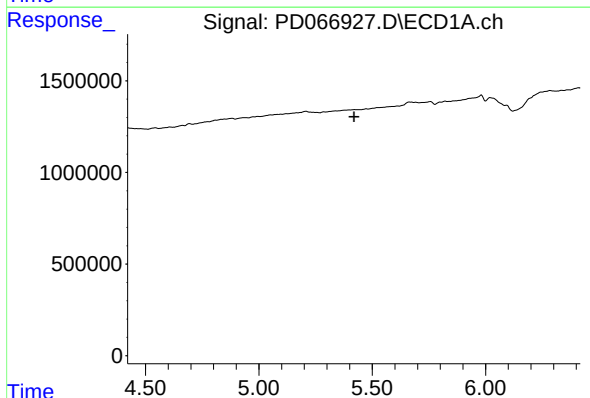


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

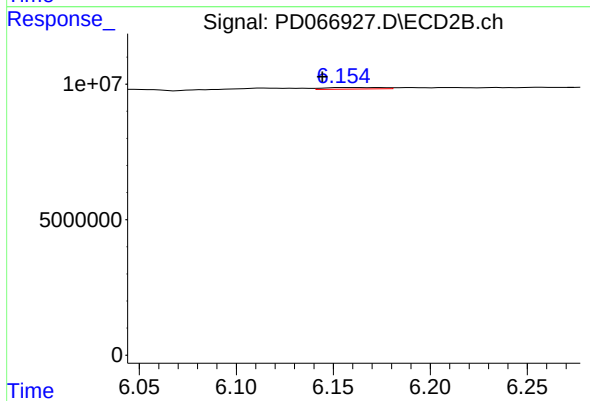

#11 alpha-Chlordane


R.T.: 6.157 min
Delta R.T.: 0.012 min
Response: 1142793
Conc: 0.14 ng/ml

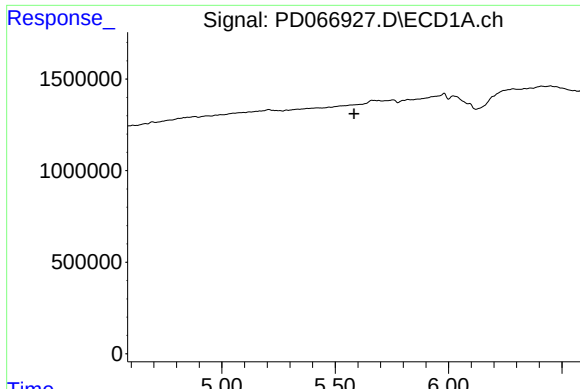

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.584 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

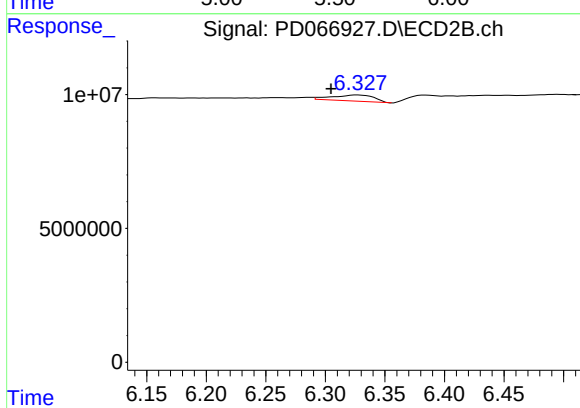


#12 4,4'-DDE

R.T.: 6.327 min
Delta R.T.: 0.022 min
Response: 5355814
Conc: 0.68 ng/ml

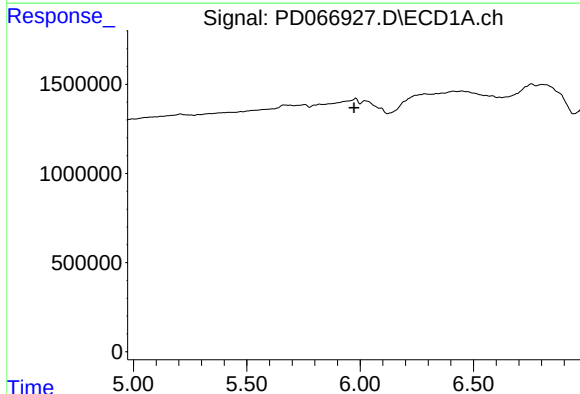


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.973 min
Response: 0
Conc: N.D.

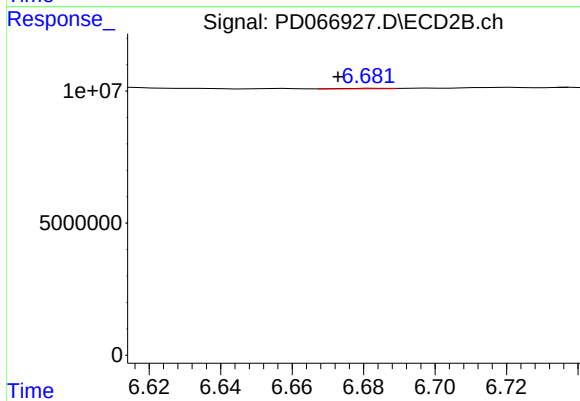

#14 Endrin


R.T.: 6.683 min
Delta R.T.: 0.010 min
Response: 114419
Conc: 0.02 ng/ml

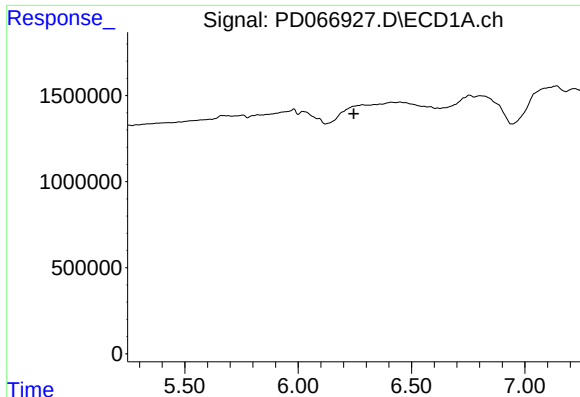

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

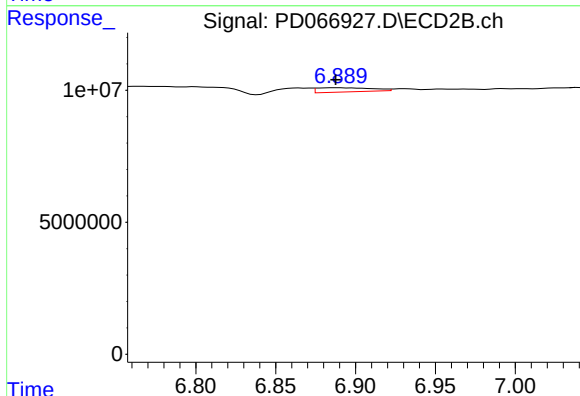


#15 Endosulfan II

R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 3788659
Conc: 0.54 ng/ml

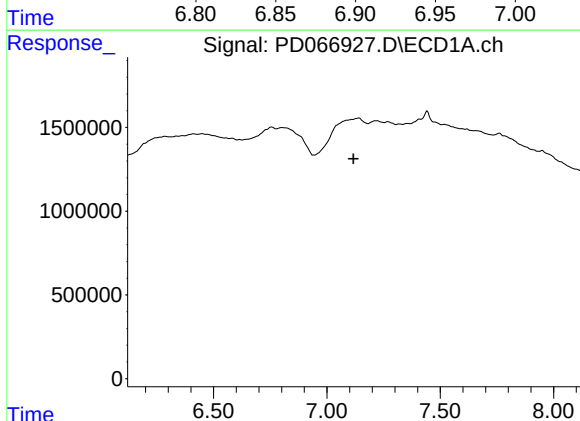


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

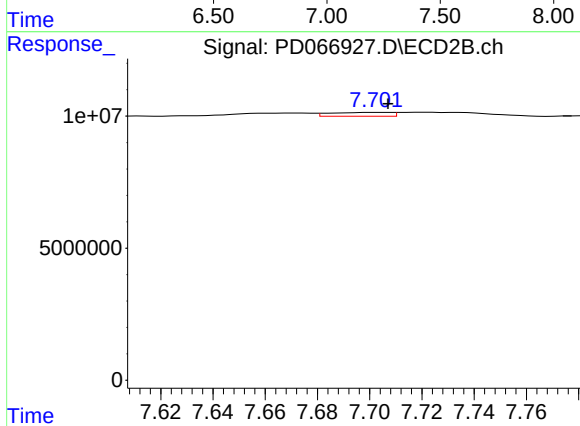

#21 Endrin ketone


R.T.: 7.703 min
Delta R.T.: -0.004 min
Response: 2342034
Conc: 0.28 ng/ml

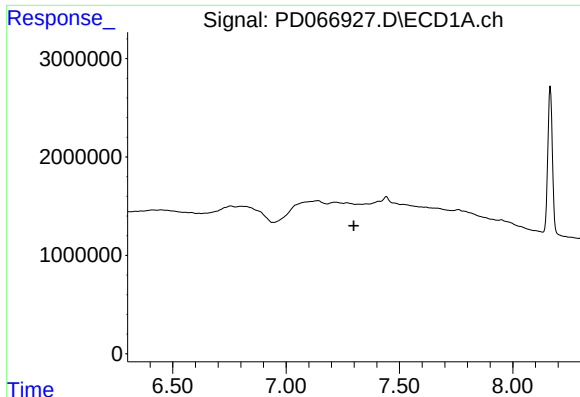

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

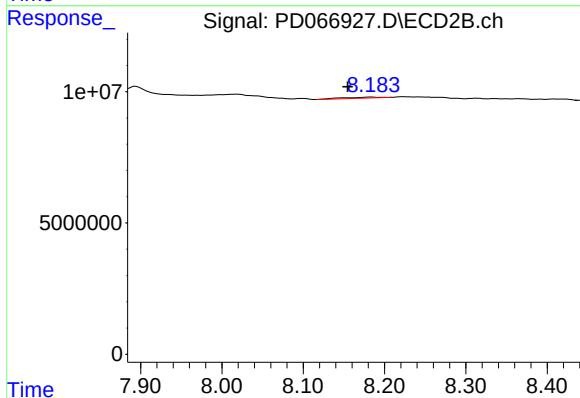


#22 Mirex

R.T.: 8.184 min
Delta R.T.: 0.029 min
Response: 1067071
Conc: 0.18 ng/ml

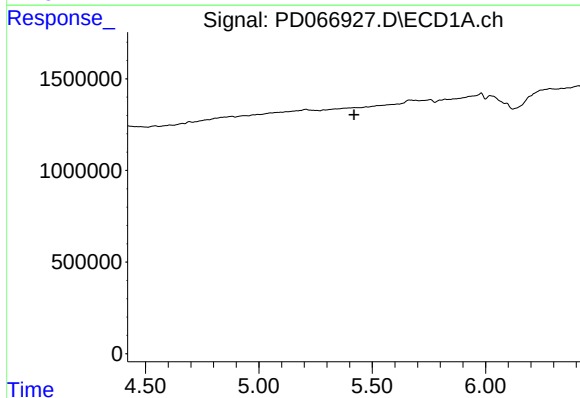


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

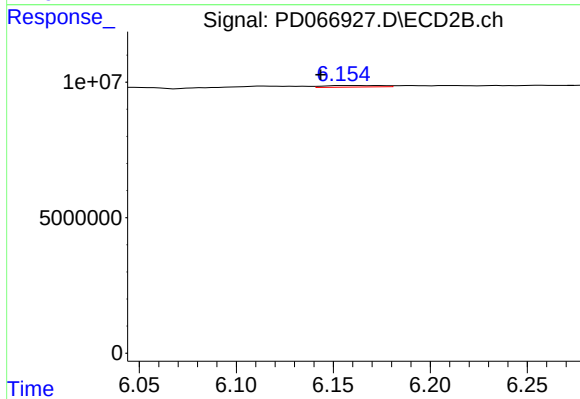

#26 Chlordane-4


R.T.: 6.157 min
Delta R.T.: 0.013 min
Response: 1142793
Conc: 0.91 ng/ml

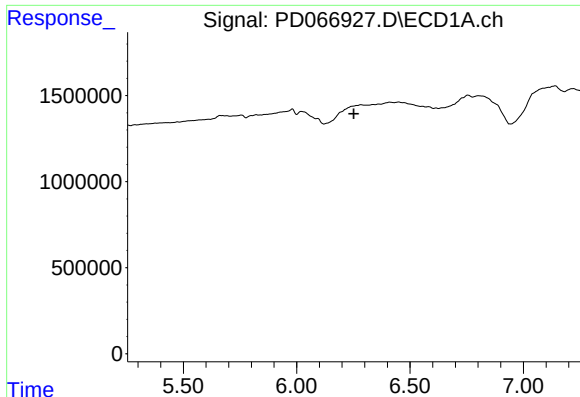

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

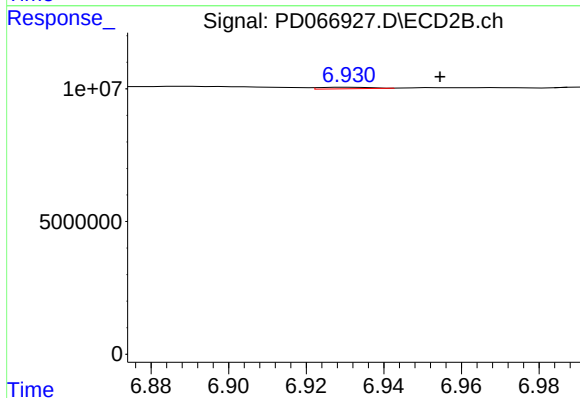


#27 Chlordane-5

R.T.: 6.932 min
Delta R.T.: -0.023 min
Response: 430509
Conc: 1.58 ng/ml

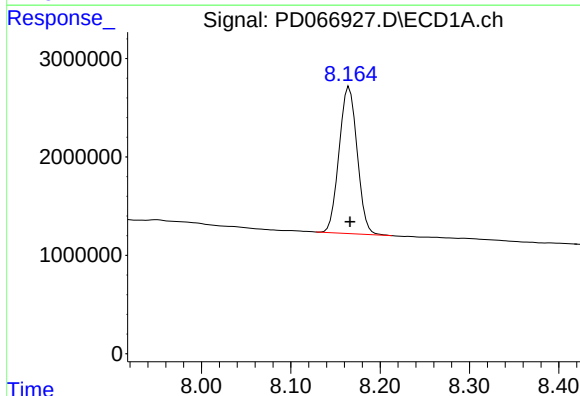

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.001 min
Response: 20957581
Conc: 18.14 ng/ml

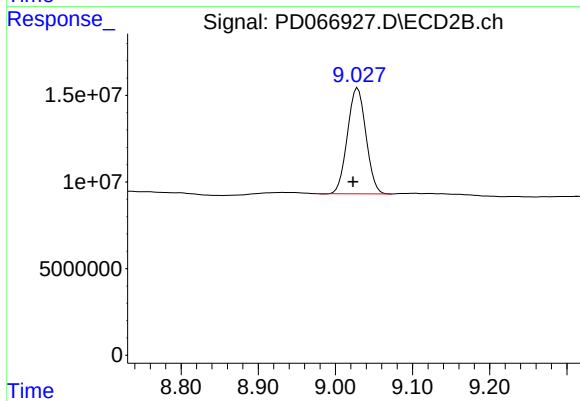

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.006 min
Response: 101532161
Conc: 18.85 ng/ml