

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
 Data File : PD066948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 18:32
 Operator : AR\AJ
 Sample : PB140768BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 06:18:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	37628559	185.6E6	20.167	22.934
28)	SA Decachlor...	8.164	9.027	22655913	115.9E6	19.608	21.526
Target Compounds							
6)	B beta-BHC	0.000	4.845f	0	1091995	N.D.	0.235 #
7)	B delta-BHC	0.000	5.050	0	2422156	N.D.	0.265 #
8)	B Heptachlo...	0.000	5.862f	0	1145919	N.D.	0.158 #
15)	B Endosulfa...	0.000	6.894	0	2144655	N.D.	0.304 #
27)	Chlordane-5	0.000	6.929f	0	489529	N.D.	1.796 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
Data File : PD066948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 18:32
Operator : AR\AJ
Sample : PB140768BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 06:18:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

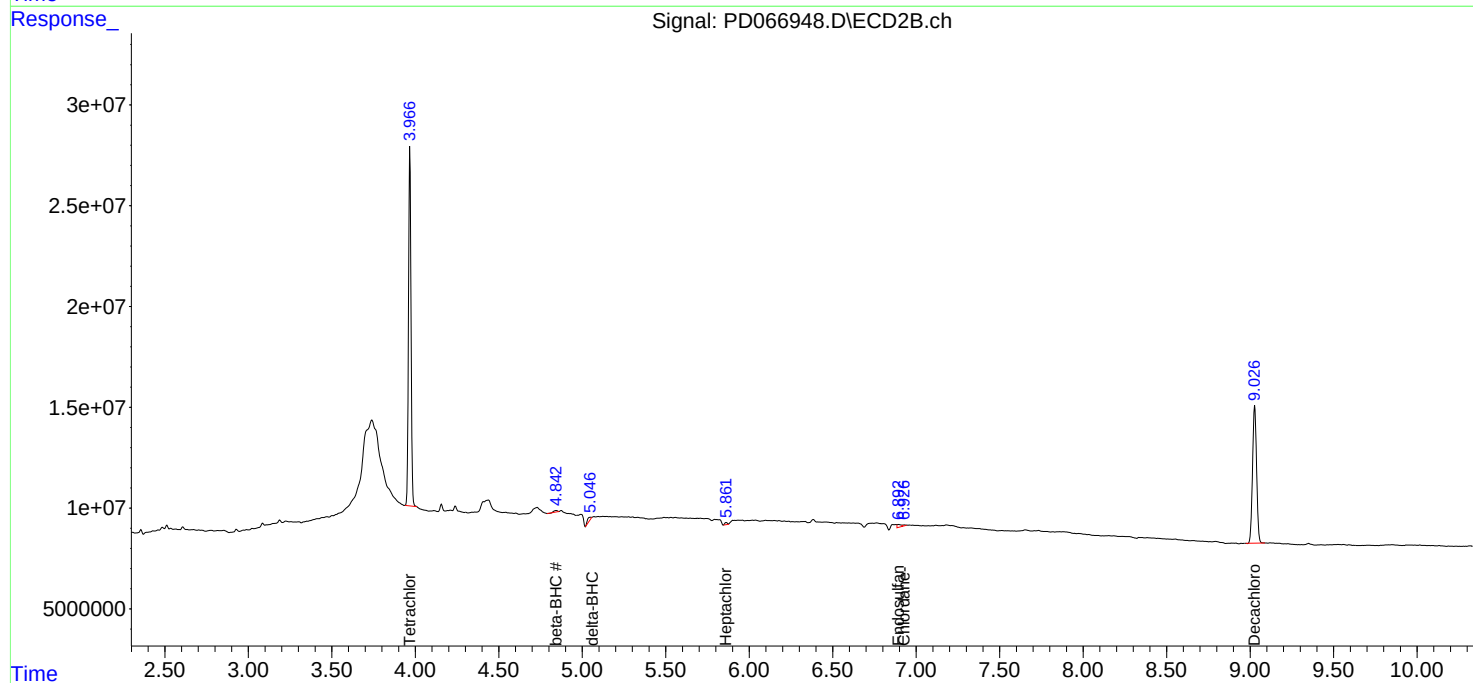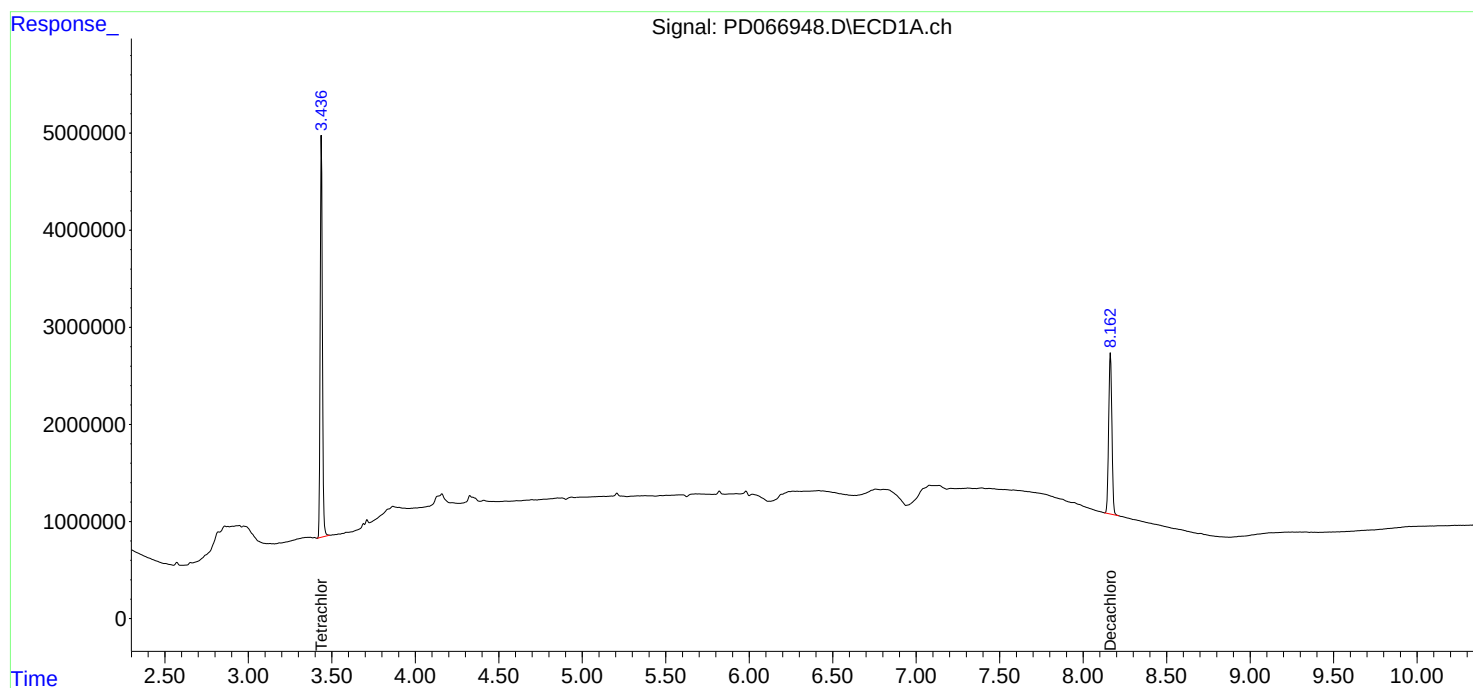


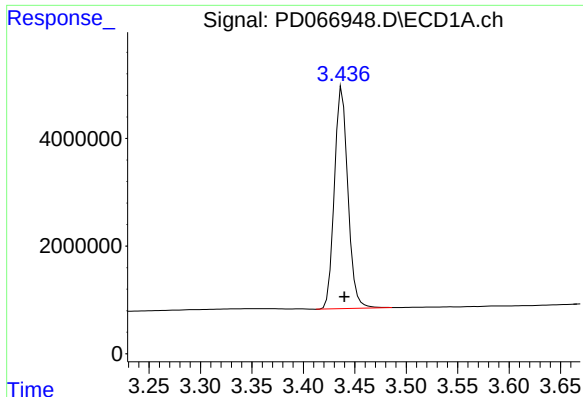

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 37628559
Conc: 20.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

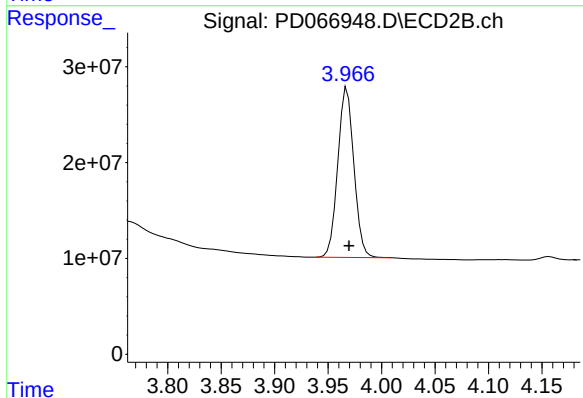


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 185583576
Conc: 22.93 ng/ml

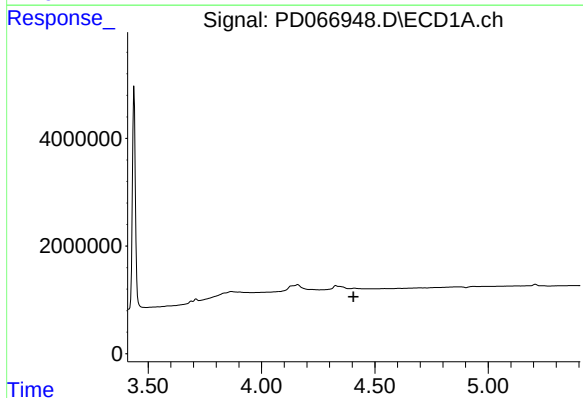


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.406 min
Response: 0
Conc: N.D.

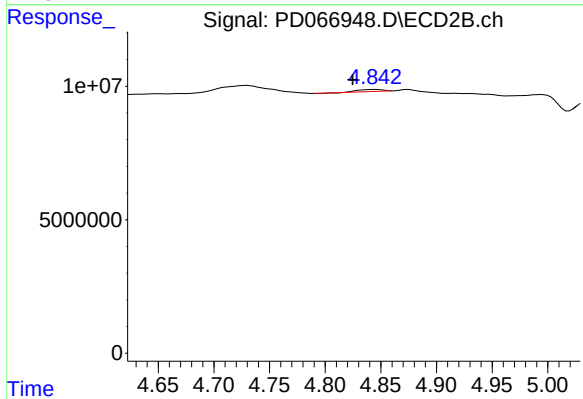

#6 beta-BHC


R.T.: 4.845 min
Delta R.T.: 0.020 min
Response: 1091995
Conc: 0.23 ng/ml

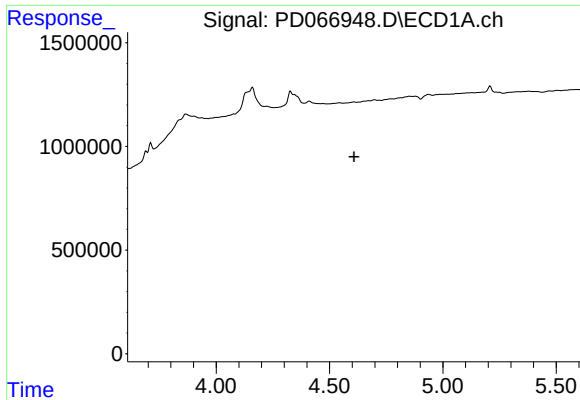

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

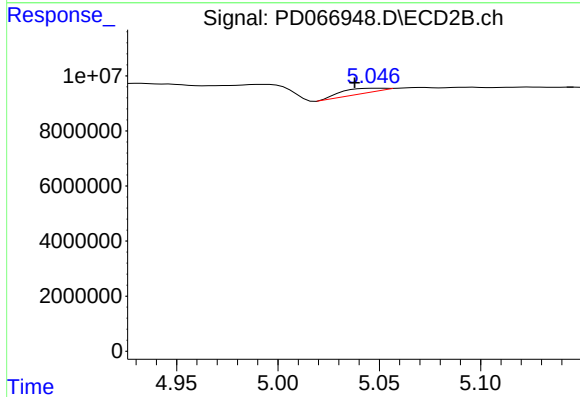


#7 delta-BHC

R.T.: 5.050 min
Delta R.T.: 0.012 min
Response: 2422156
Conc: 0.26 ng/ml

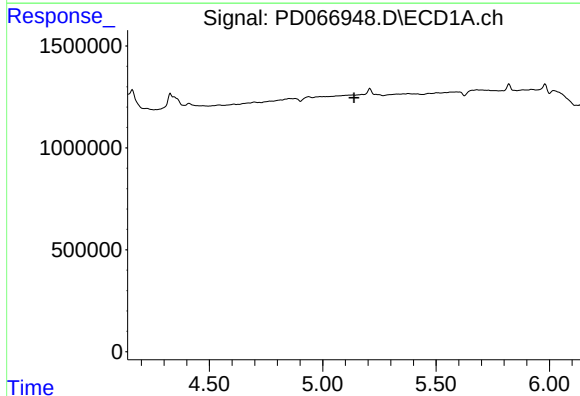


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

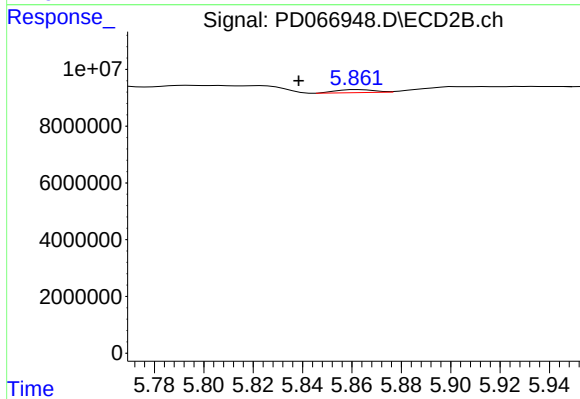

#8 Heptachlor epoxide


R.T.: 5.862 min
Delta R.T.: 0.024 min
Response: 1145919
Conc: 0.16 ng/ml

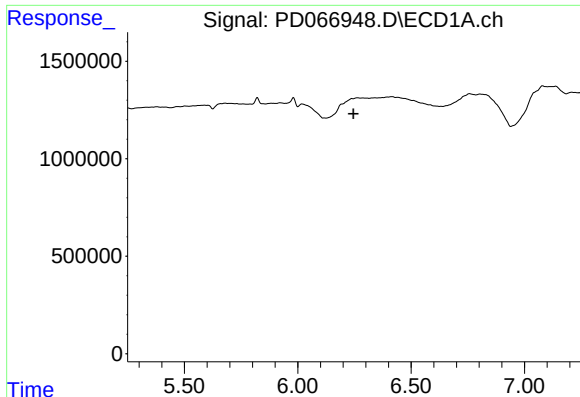

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

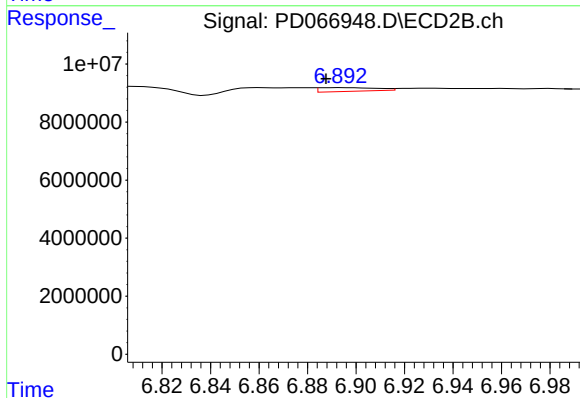


#15 Endosulfan II

R.T.: 6.894 min
Delta R.T.: 0.006 min
Response: 2144655
Conc: 0.30 ng/ml

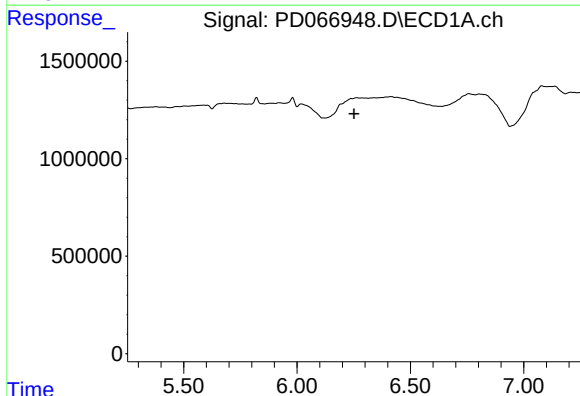


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

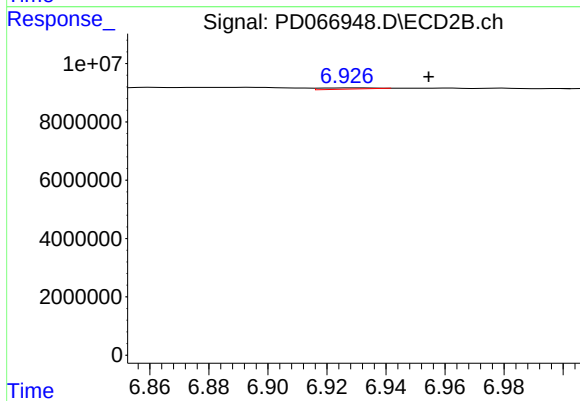

#27 Chlordane-5


R.T.: 6.929 min
Delta R.T.: -0.026 min
Response: 489529
Conc: 1.80 ng/ml

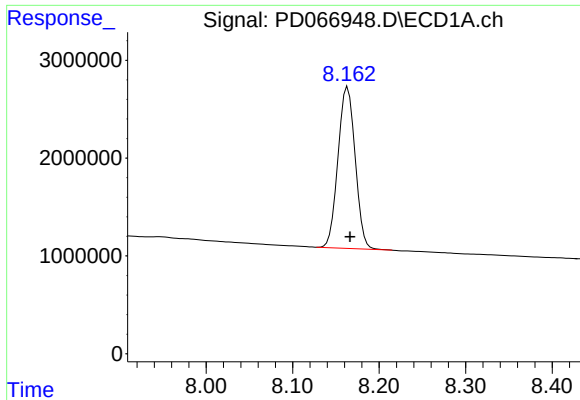

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.003 min
Response: 22655913
Conc: 19.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

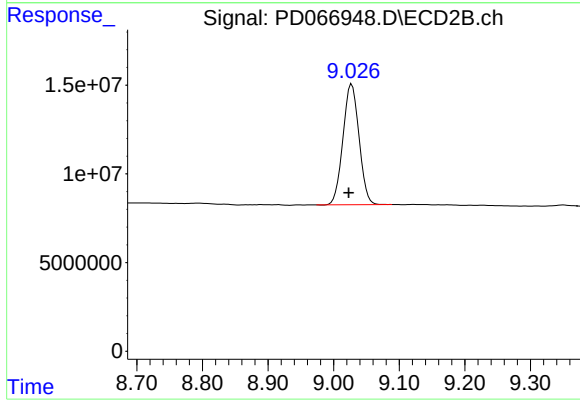

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.005 min
Response: 115947104
Conc: 21.53 ng/ml