

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
 Data File : PD066958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 23:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 06:19:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	36025662	175.2E6	19.308	21.654
28)	SA Decachlor...	8.163	9.026	21961513	112.8E6	19.007	20.939
Target Compounds							
4)	MA Heptachlor	0.000	5.129f	0	1604690	N.D.	0.164 #
6)	B beta-BHC	0.000	4.842f	0	2007182	N.D.	0.431 #
7)	B delta-BHC	0.000	5.058f	0	3382779	N.D.	0.370 #
8)	B Heptachlo...	0.000	5.831	0	13393243	N.D.	1.848 #
15)	B Endosulfa...	0.000	6.894	0	911157	N.D.	0.129 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
Data File : PD066958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 23:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 06:19:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

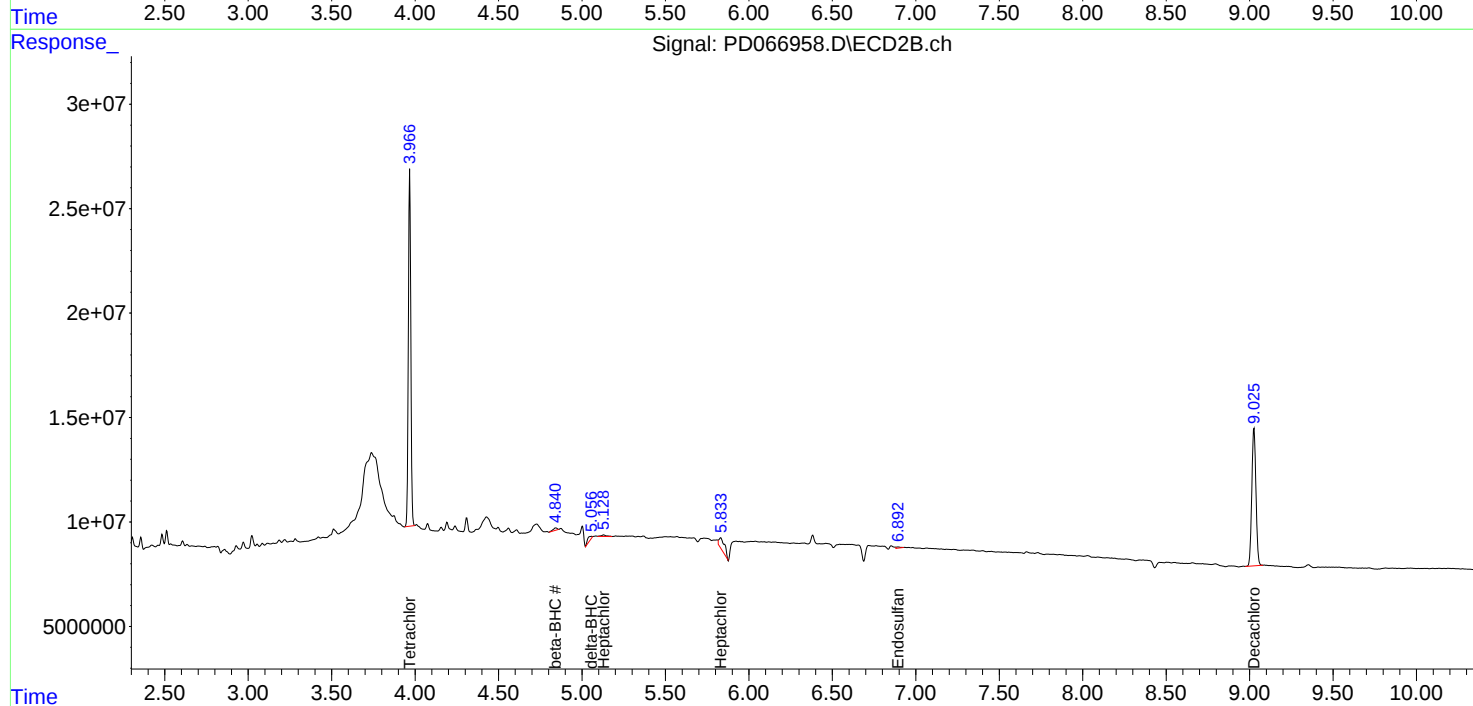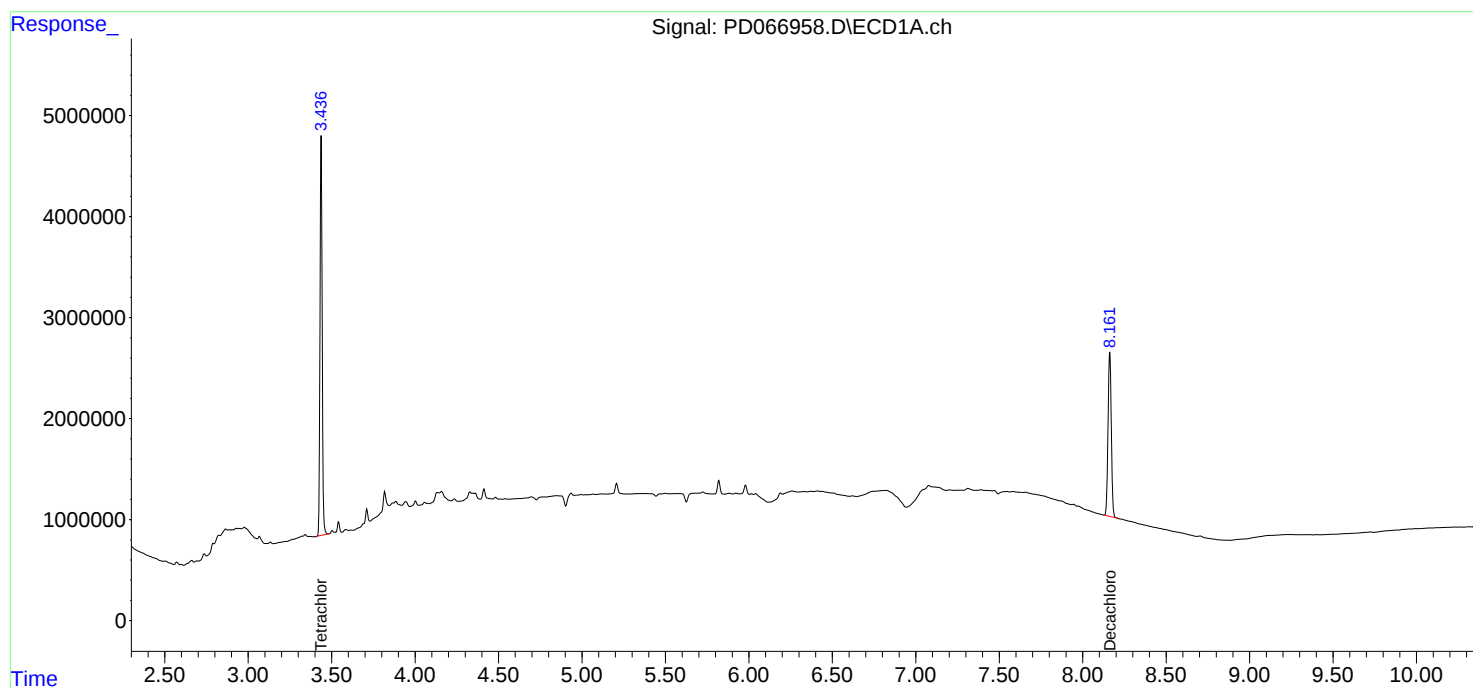


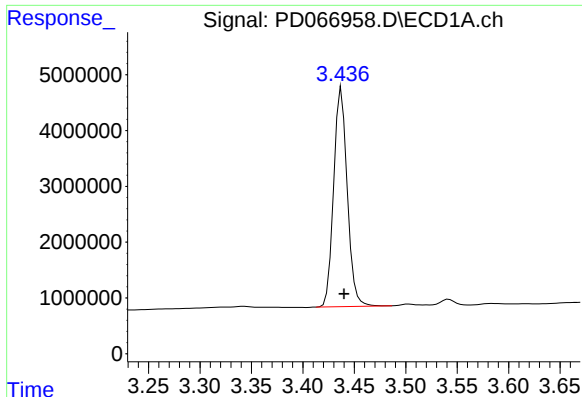

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 36025662
Conc: 19.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

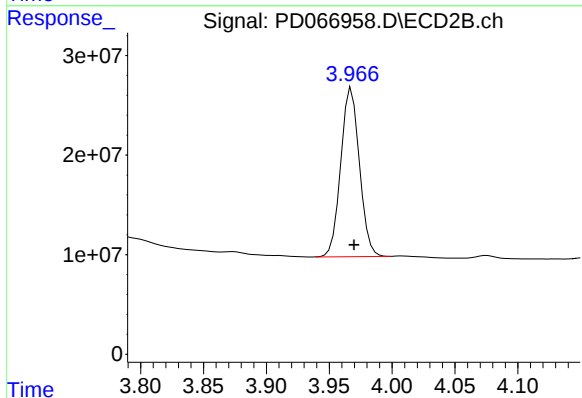


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 175226573
Conc: 21.65 ng/ml

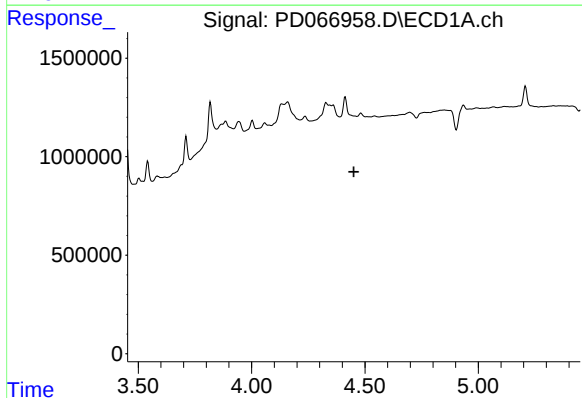


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.452 min
Response: 0
Conc: N.D.

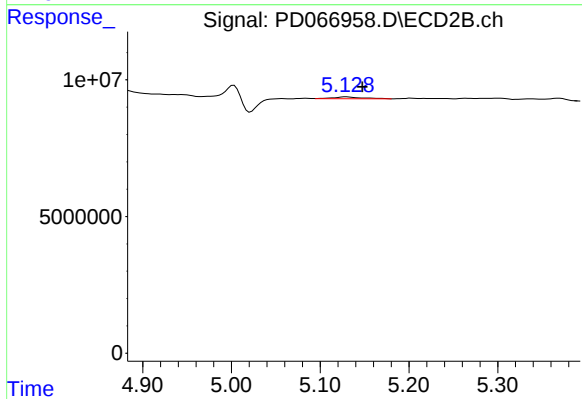

#4 Heptachlor


R.T.: 5.129 min
Delta R.T.: -0.018 min
Response: 1604690
Conc: 0.16 ng/ml

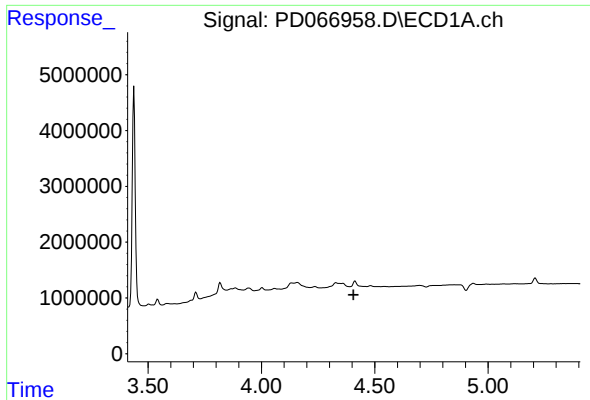

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

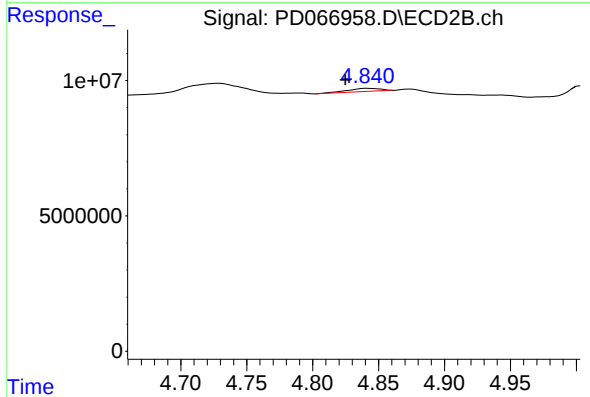


#6 beta-BHC

R.T.: 4.842 min
Delta R.T.: 0.017 min
Response: 2007182
Conc: 0.43 ng/ml

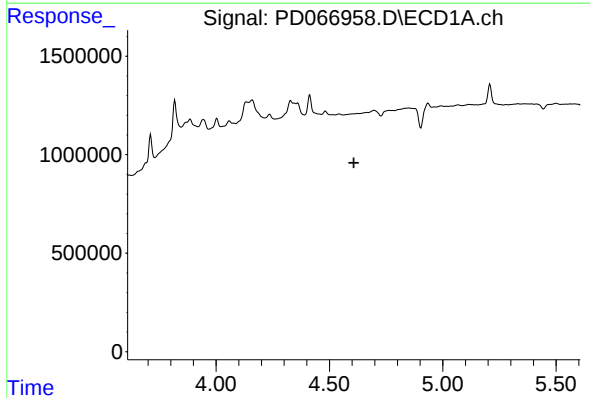


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.608 min
Response: 0
Conc: N.D.

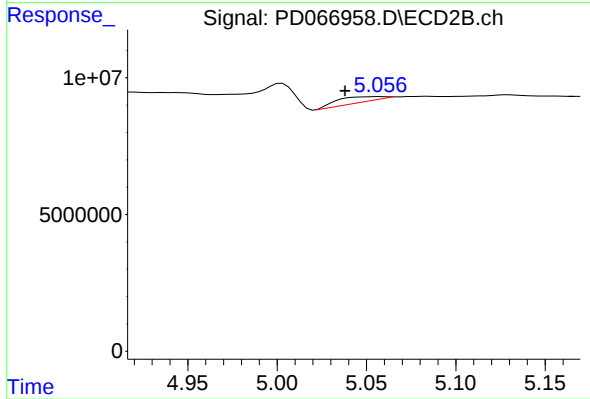

#7 delta-BHC


R.T.: 5.058 min
Delta R.T.: 0.020 min
Response: 3382779
Conc: 0.37 ng/ml

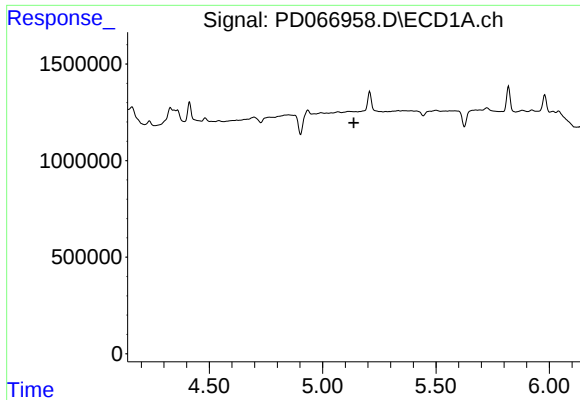

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

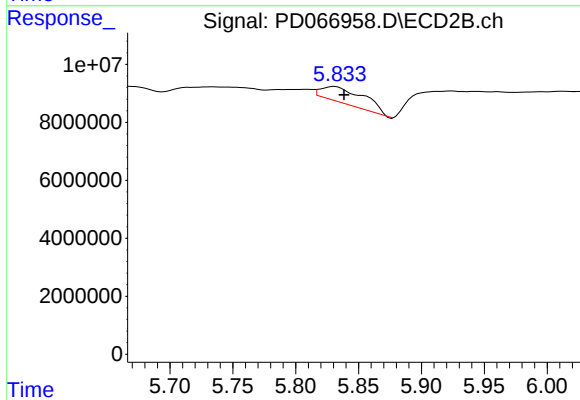


#8 Heptachlor epoxide

R.T.: 5.831 min
Delta R.T.: -0.007 min
Response: 13393243
Conc: 1.85 ng/ml

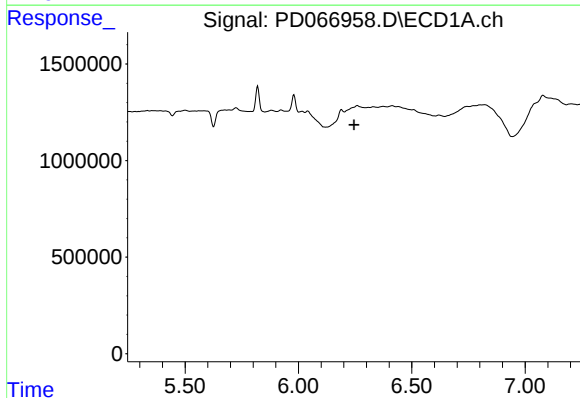


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

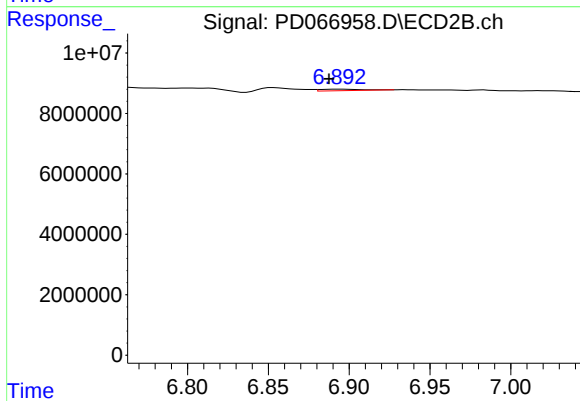

#15 Endosulfan II


R.T.: 6.894 min
Delta R.T.: 0.006 min
Response: 911157
Conc: 0.13 ng/ml

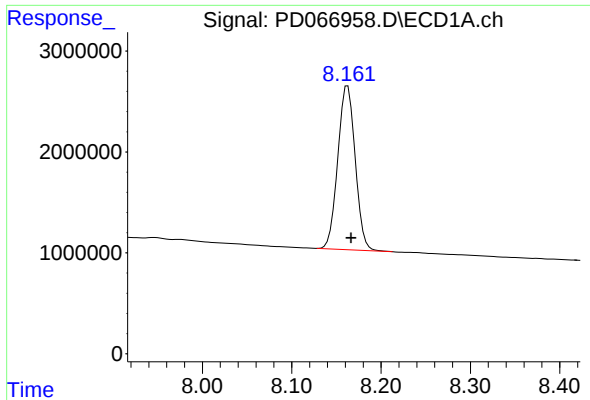

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: -0.004 min
Response: 21961513
Conc: 19.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

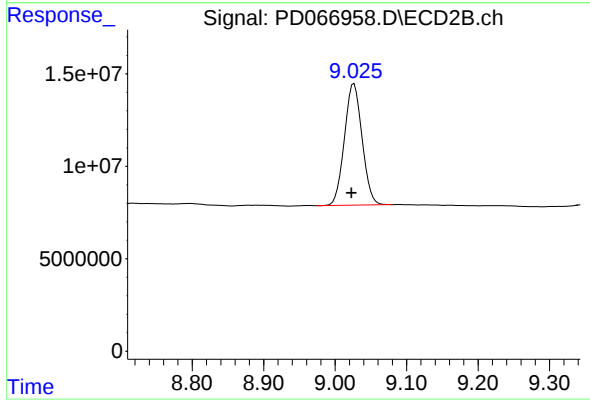

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.003 min
Response: 112786695
Conc: 20.94 ng/ml