

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
 Data File : PD066926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 13:19
 Operator : AR\AJ
 Sample : M4623-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/16/2021
 Supervised By : mohammad ahmed 11/16/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 11:16:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.968	23764056	77502719	12.736m	9.578
28)	SA Decachlor...	8.164	9.035	3524596	18926341	3.051	3.514m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
Data File : PD066926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 13:19
Operator : AR\AJ
Sample : M4623-01
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/16/2021
Supervised By : mohammad ahmed 11/16/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 11:16:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

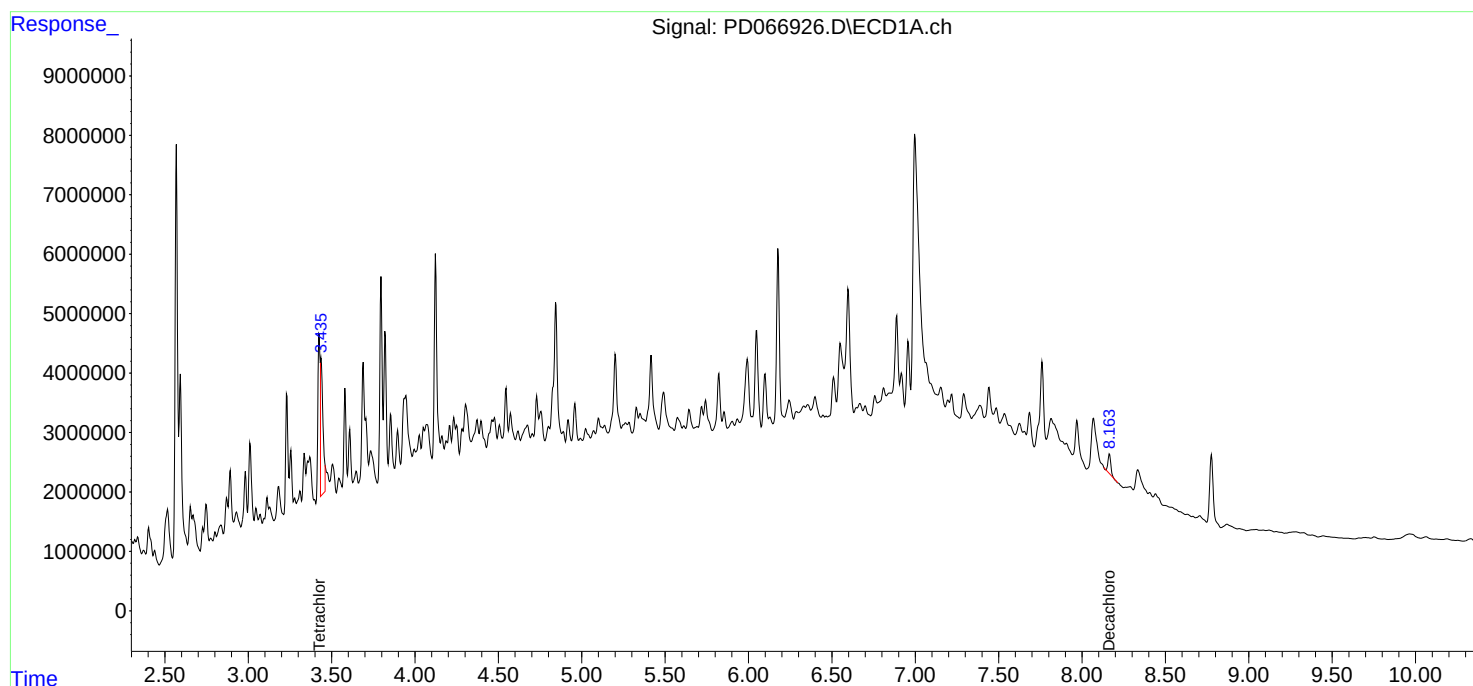

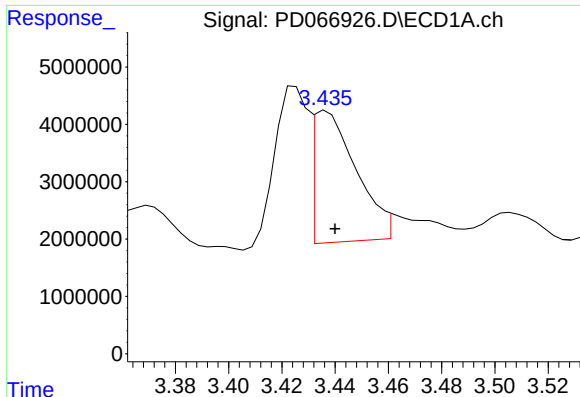


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 23764056
Conc: 12.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/16/2021
Supervised By :mohammad ahmed 11/16/2021

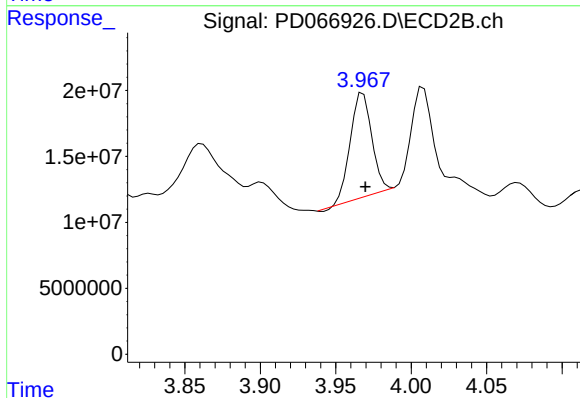


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 77502719
Conc: 9.58 ng/ml

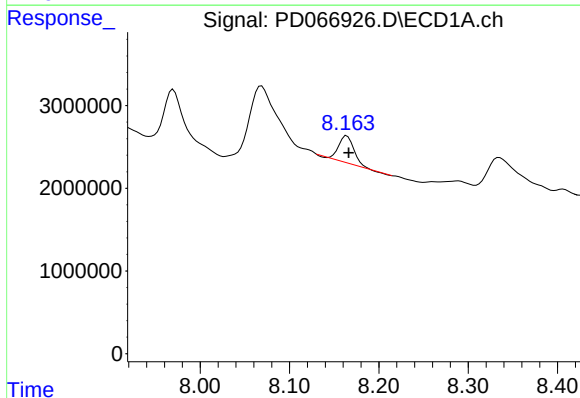

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.002 min
Response: 3524596
Conc: 3.05 ng/ml

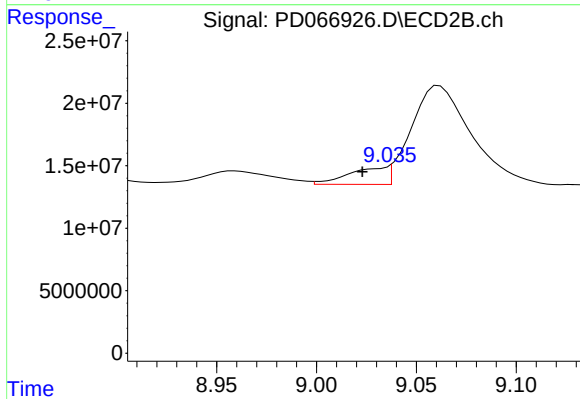

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.012 min
Response: 18926341
Conc: 3.51 ng/ml m