

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
 Data File : PD066939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 16:28
 Operator : AR\AJ
 Sample : M4674-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MF-WATER-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 06:16:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	30944405	147.3E6	16.585	18.197
28)	SA Decachlor...	8.163	9.029	5703956	27015311	4.937	5.015

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111521\
Data File : PD066939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 16:28
Operator : AR\AJ
Sample : M4674-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MF-WATER-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 06:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

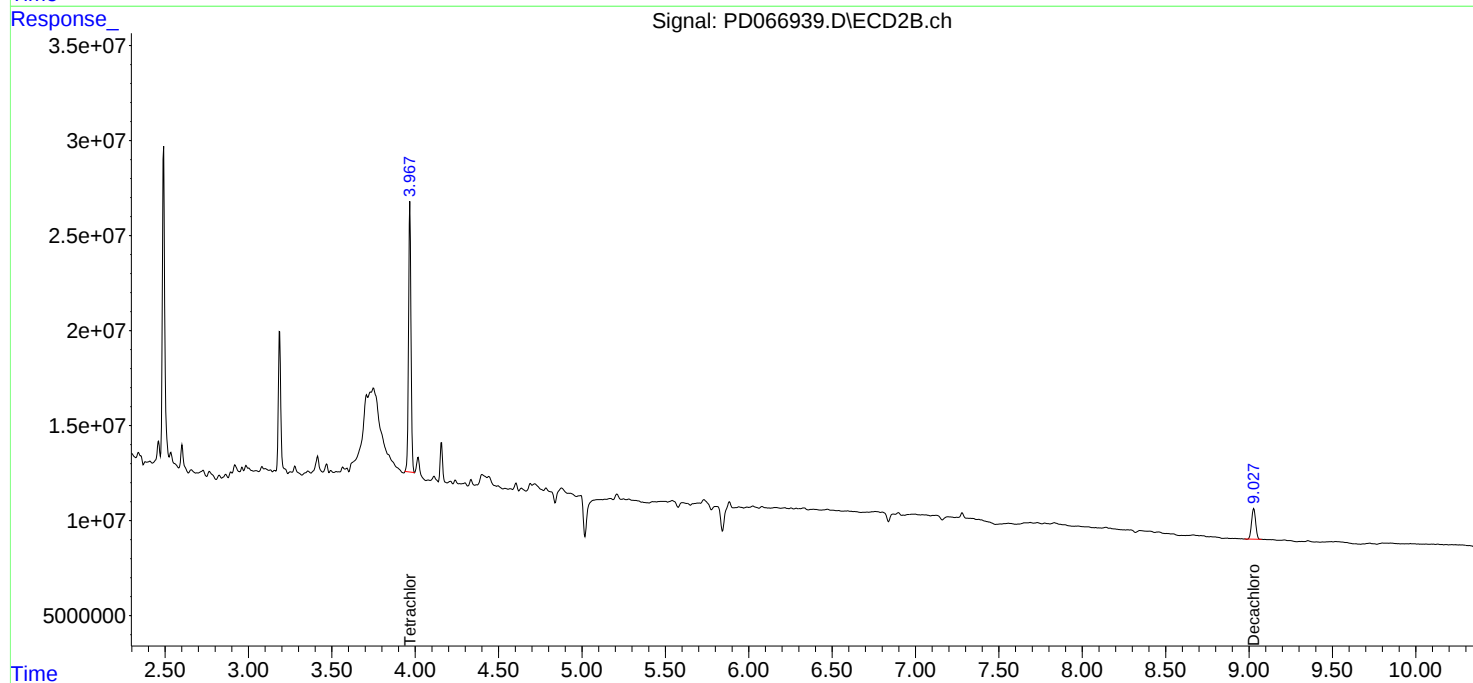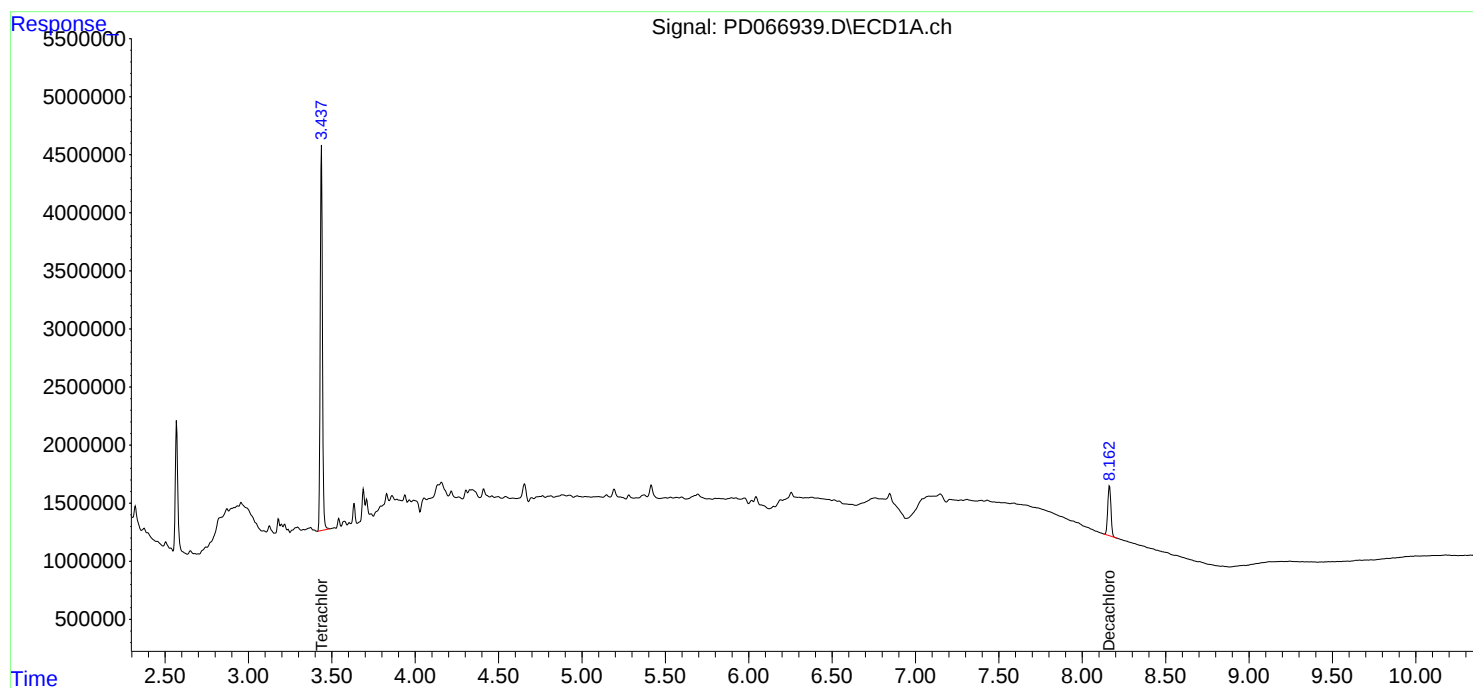


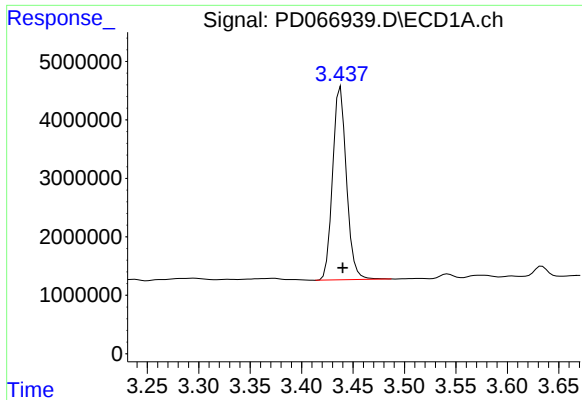

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 30944405
Conc: 16.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
MF-WATER-COMP

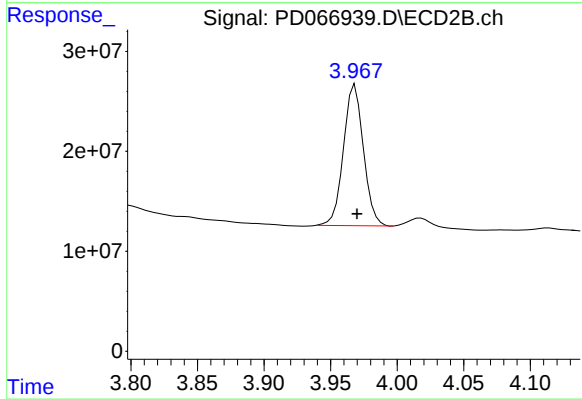


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.001 min
Response: 147251601
Conc: 18.20 ng/ml

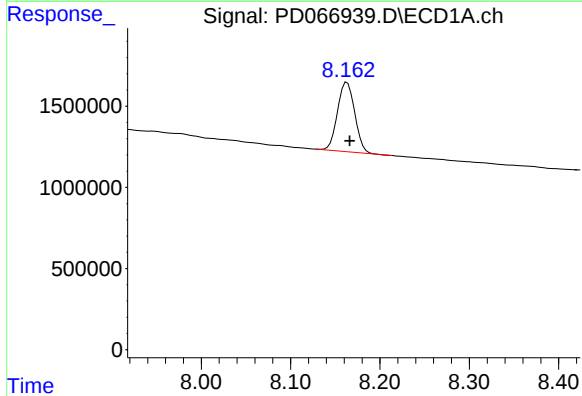

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: -0.003 min
Response: 5703956
Conc: 4.94 ng/ml

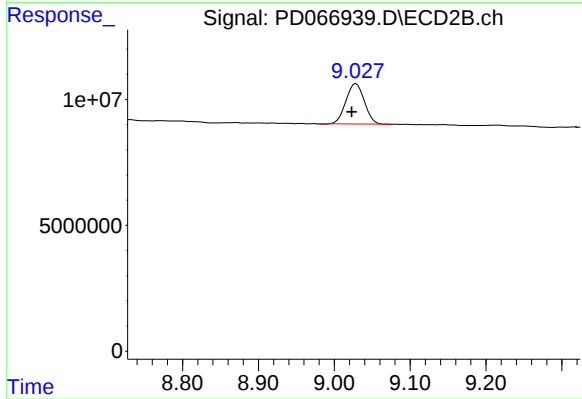

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.006 min
Response: 27015311
Conc: 5.02 ng/ml