

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111524\
 Data File : PD086693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 10:42
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:44:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 14:23:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.557	2.885	81657110	514.0E6	52.908	49.564
7) SA Decachlor...	9.088	8.089	107.7E6	536.7E6	52.864	47.290
Target Compounds						
2) Toxaphene-1	6.251	5.486	9771956	51764734	561.589	505.307
3) Toxaphene-2	6.452	5.658	15571342	31632004	592.794	459.778
4) Toxaphene-3	7.158	6.769	28160320	153.9E6	505.548	432.614
5) Toxaphene-4	7.574	7.211	35458807	113.9E6	573.701	452.150
6) Toxaphene-5	7.940	7.343	20884595	71387161	557.976	406.316 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111524\
Data File : PD086693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 10:42
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:44:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 14:23:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

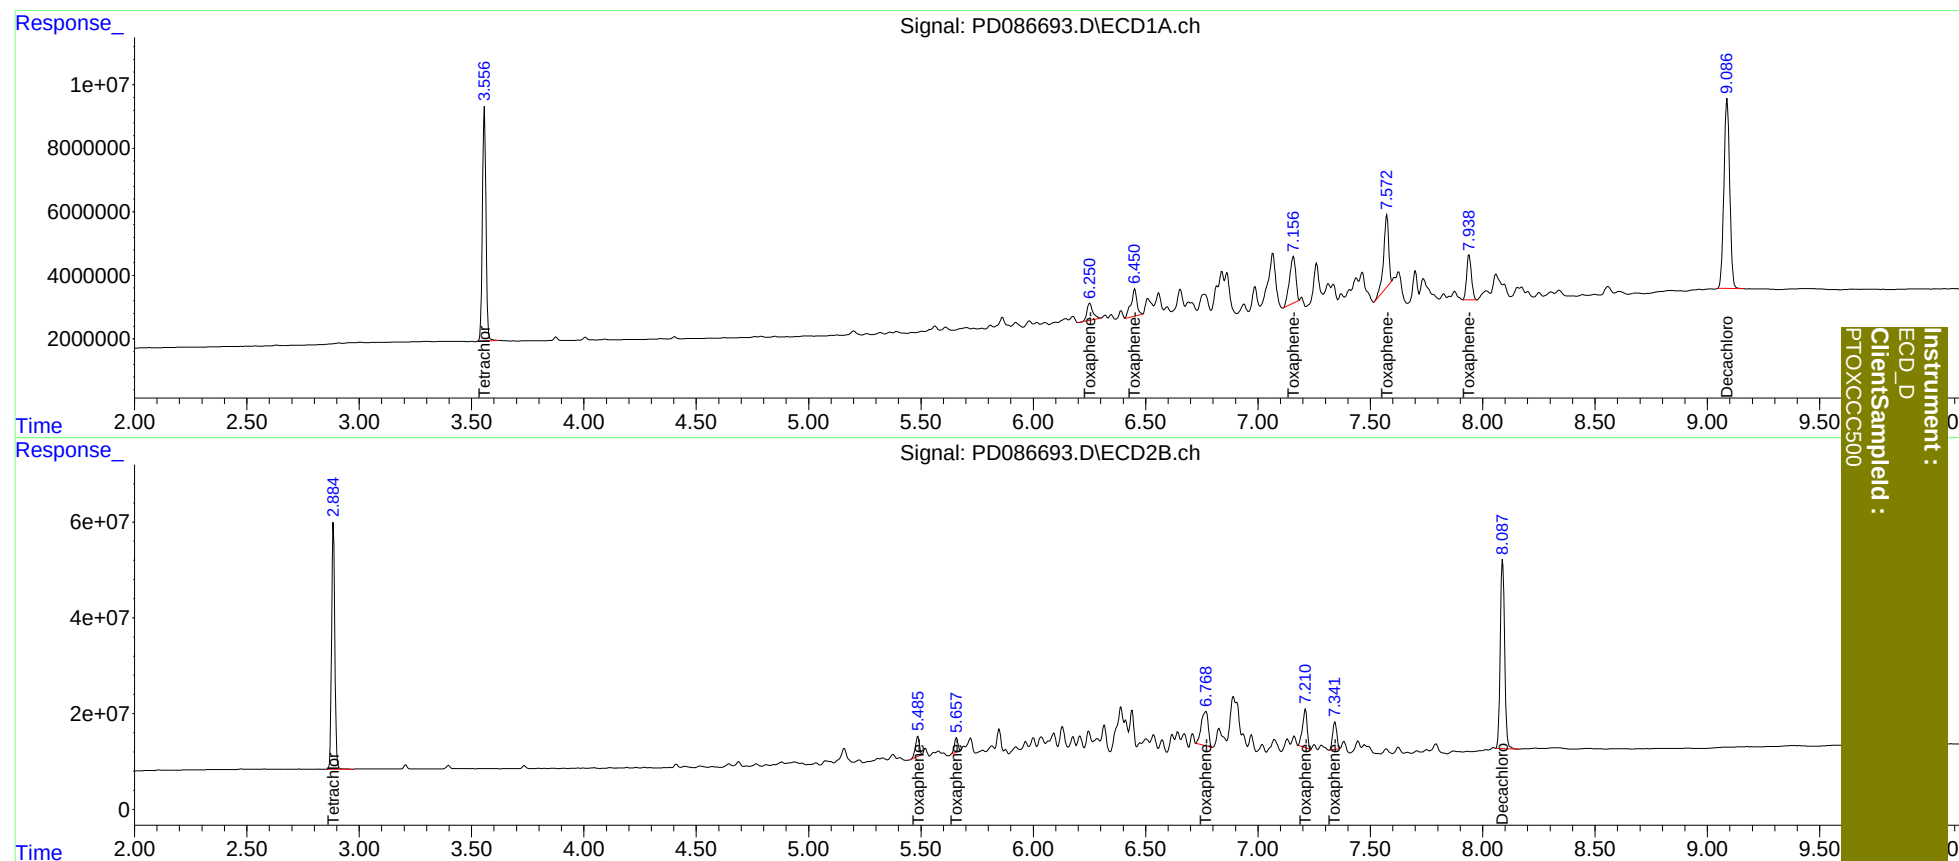

Instrument :
ECD_D
ClientSampled :
PTOXCCC500