

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
 Data File : PD091202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2025 22:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 04:29:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:28:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.873	240.4E6	3110.2E6	83.524	81.729
28)	SA Decachlor...	9.063	8.059	340.9E6	2764.2E6	81.453	81.131
Target Compounds							
23)	Chlordane-1	4.707	3.896	192.1E6	1269.3E6	847.850	804.834
24)	Chlordane-2	5.234	4.476	180.4E6	1266.5E6	816.978	793.134
25)	Chlordane-3	5.939	5.114	773.9E6	4225.8E6	862.382	804.691
26)	Chlordane-4	6.024	5.179	915.1E6	3495.2E6	848.683	802.667
27)	Chlordane-5	6.863	6.079	152.2E6	1511.8E6	857.282	805.549



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
Data File : PD091202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2025 22:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 04:29:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:28:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

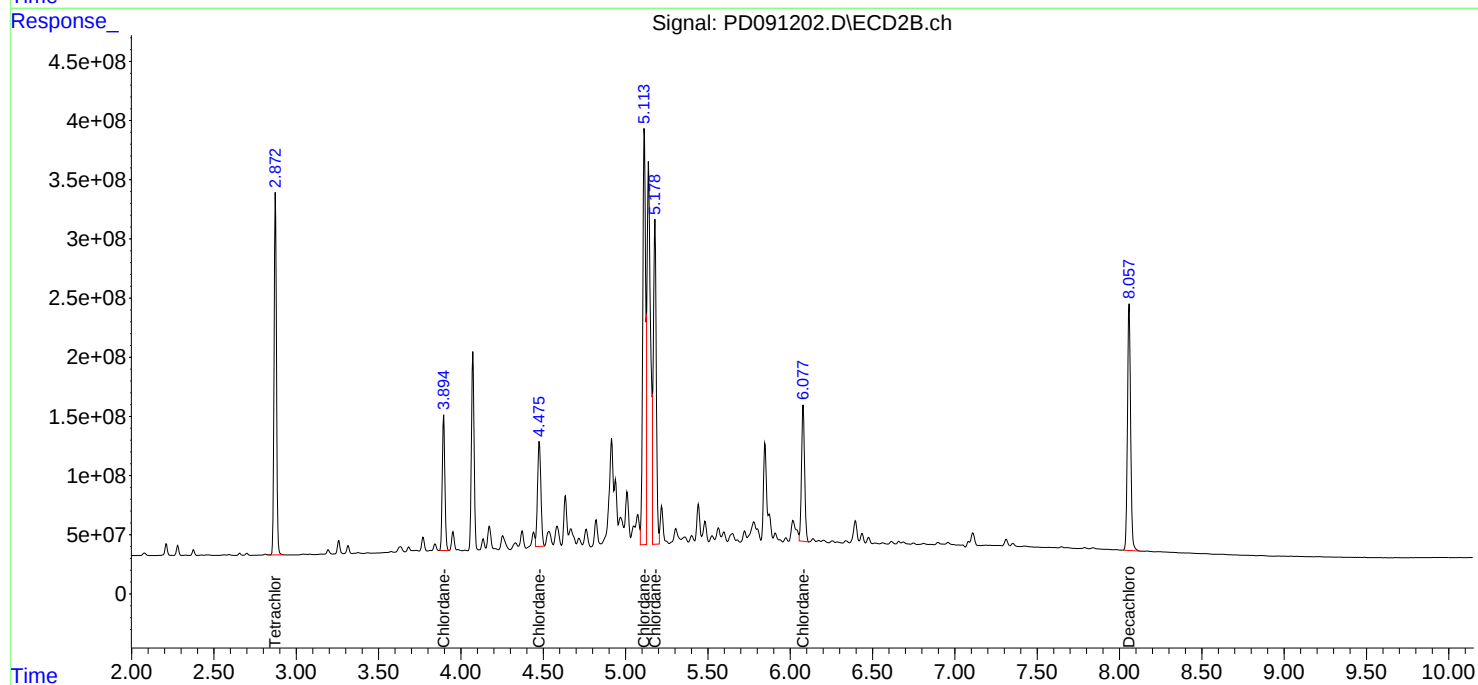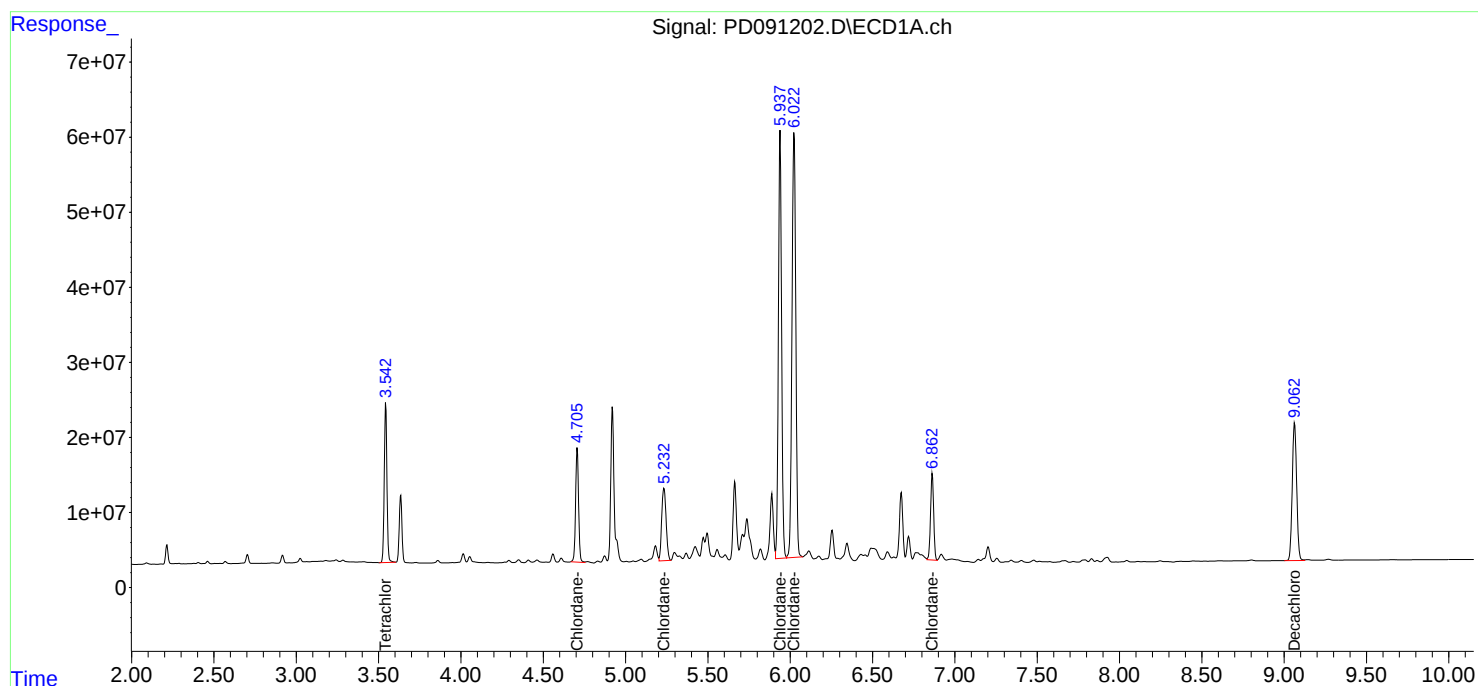


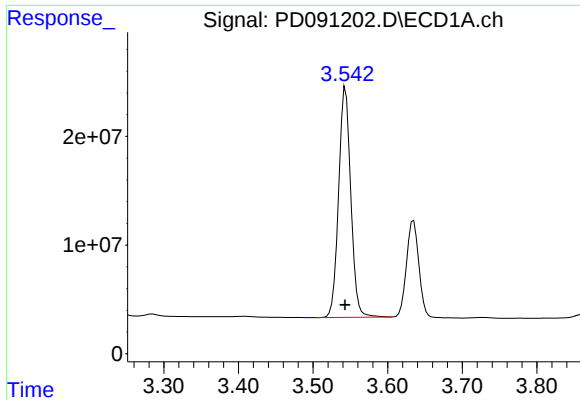

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 240366290
Conc: 83.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

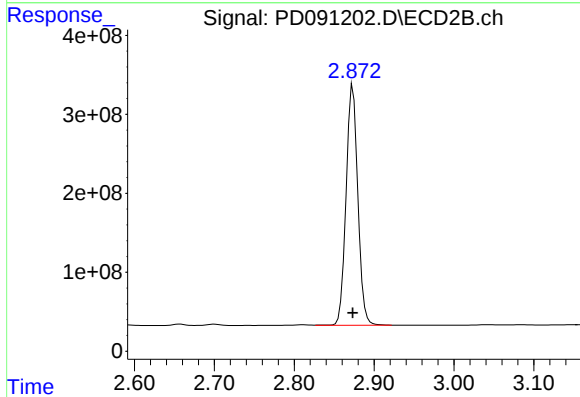


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: 0.000 min
Response: 3110170221
Conc: 81.73 ng/ml

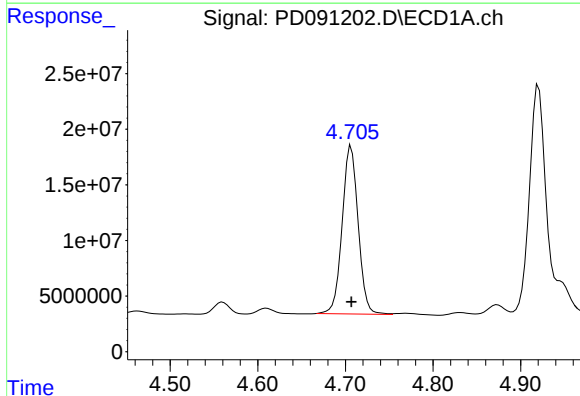


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 192087820
Conc: 847.85 ng/ml

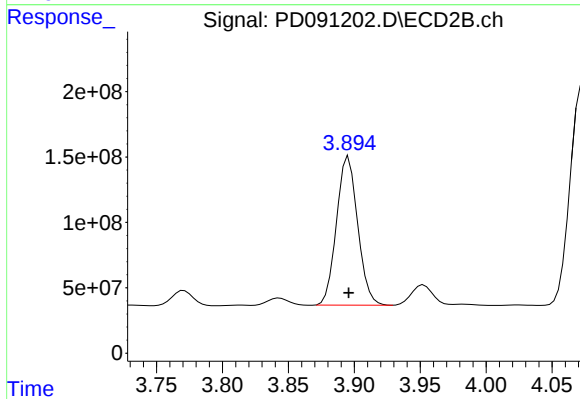

#23 Chlordane-1


R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 1269330674
Conc: 804.83 ng/ml

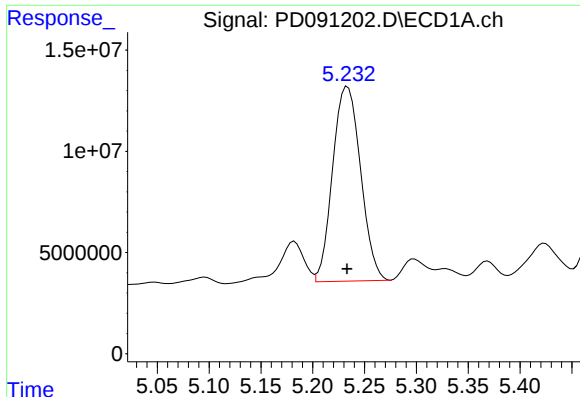

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 180419372
Conc: 816.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

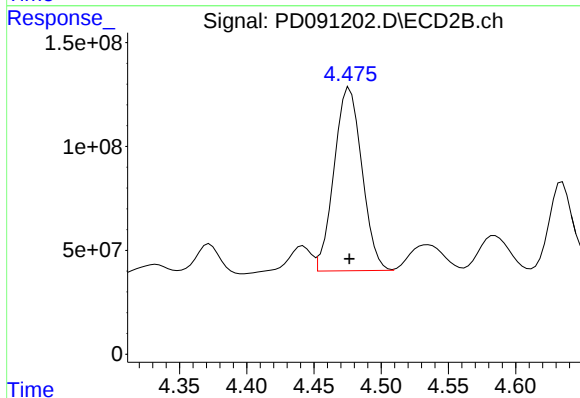


#24 Chlordane-2

R.T.: 4.476 min
Delta R.T.: 0.000 min
Response: 1266505011
Conc: 793.13 ng/ml

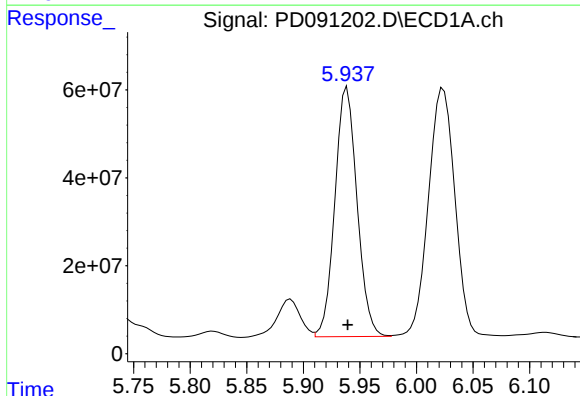


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 773906852
Conc: 862.38 ng/ml

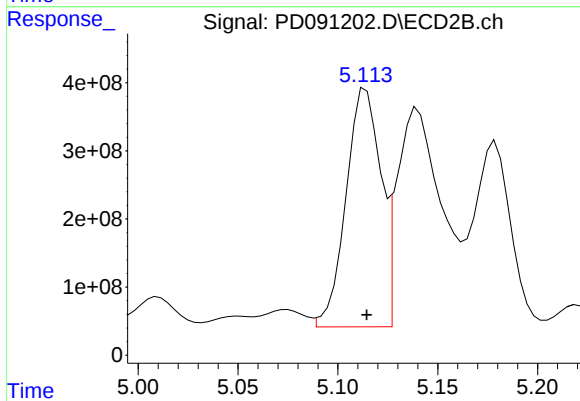

#25 Chlordane-3


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 4225791921
Conc: 804.69 ng/ml

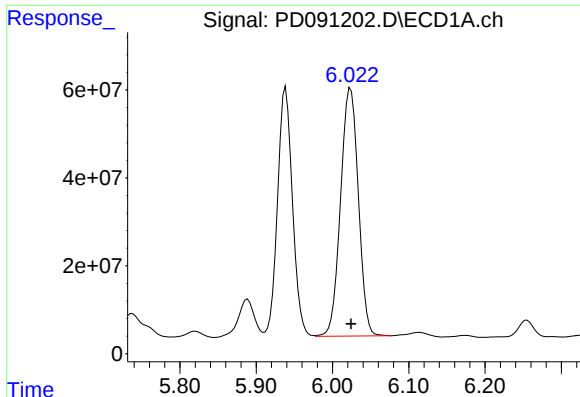

#26 Chlordane-4


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 915053418
Conc: 848.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

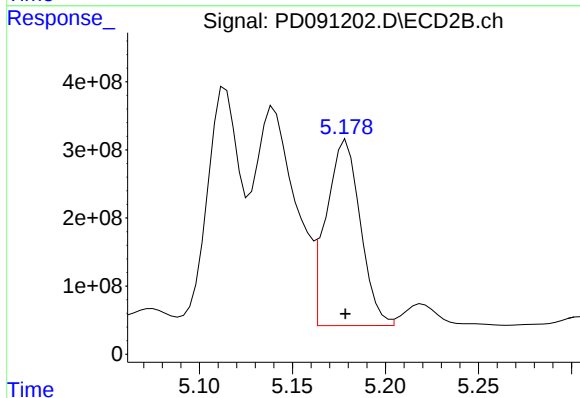


#26 Chlordane-4

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 3495225444
Conc: 802.67 ng/ml

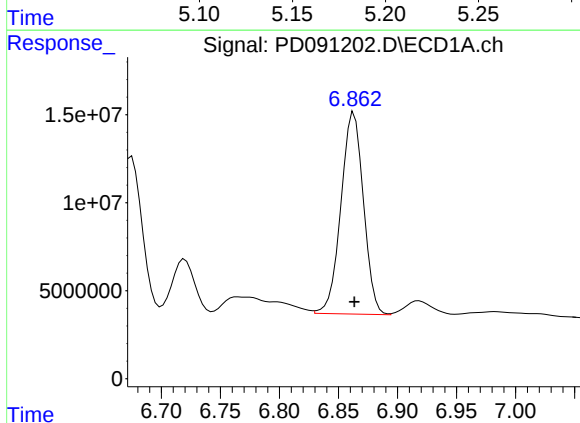


#27 Chlordane-5

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 152221189
Conc: 857.28 ng/ml

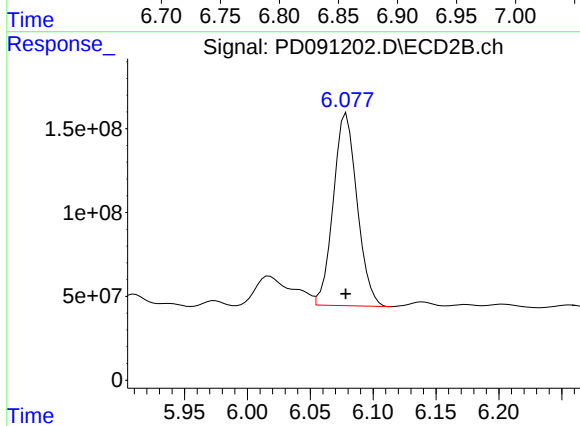

#27 Chlordane-5


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 1511846234
Conc: 805.55 ng/ml

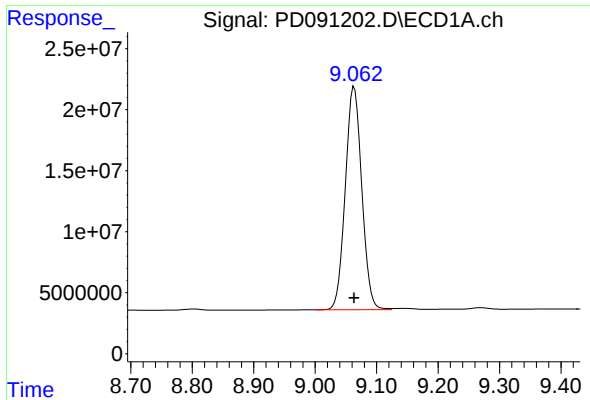

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 340941743
Conc: 81.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

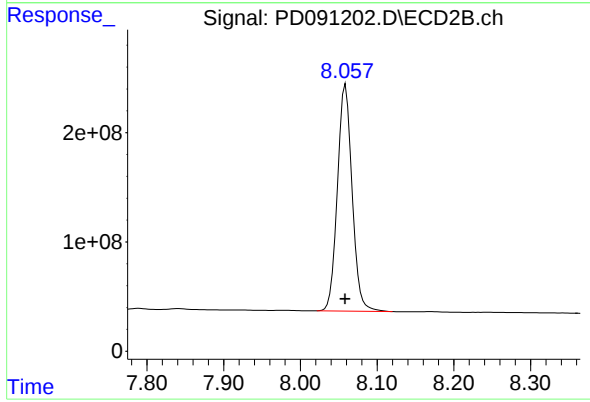

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: 0.000 min
Response: 2764170440
Conc: 81.13 ng/ml