

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
 Data File : PD091212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2025 00:49
 Operator : AR\AJ
 Sample : PCHLORICV050
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD111525CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 04:41:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:40:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.874	144.0E6	1897.0E6	45.917	45.899
28)	SA Decachlor...	9.063	8.059	208.1E6	1722.5E6	44.473	45.857
Target Compounds							
23)	Chlordane-1	4.707	3.896	114.2E6	783.3E6	464.144	455.309
24)	Chlordane-2	5.234	4.477	110.1E6	794.6E6	445.736	453.786
25)	Chlordane-3	5.939	5.115	447.1E6	2621.5E6	463.407	455.626
26)	Chlordane-4	6.024	5.179	540.3E6	2175.2E6	449.814	454.716
27)	Chlordane-5	6.863	6.079	88911954	936.5E6	450.023	461.495



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111525\
Data File : PD091212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2025 00:49
Operator : AR\AJ
Sample : PCHLORICV050
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD111525CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 04:41:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:40:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

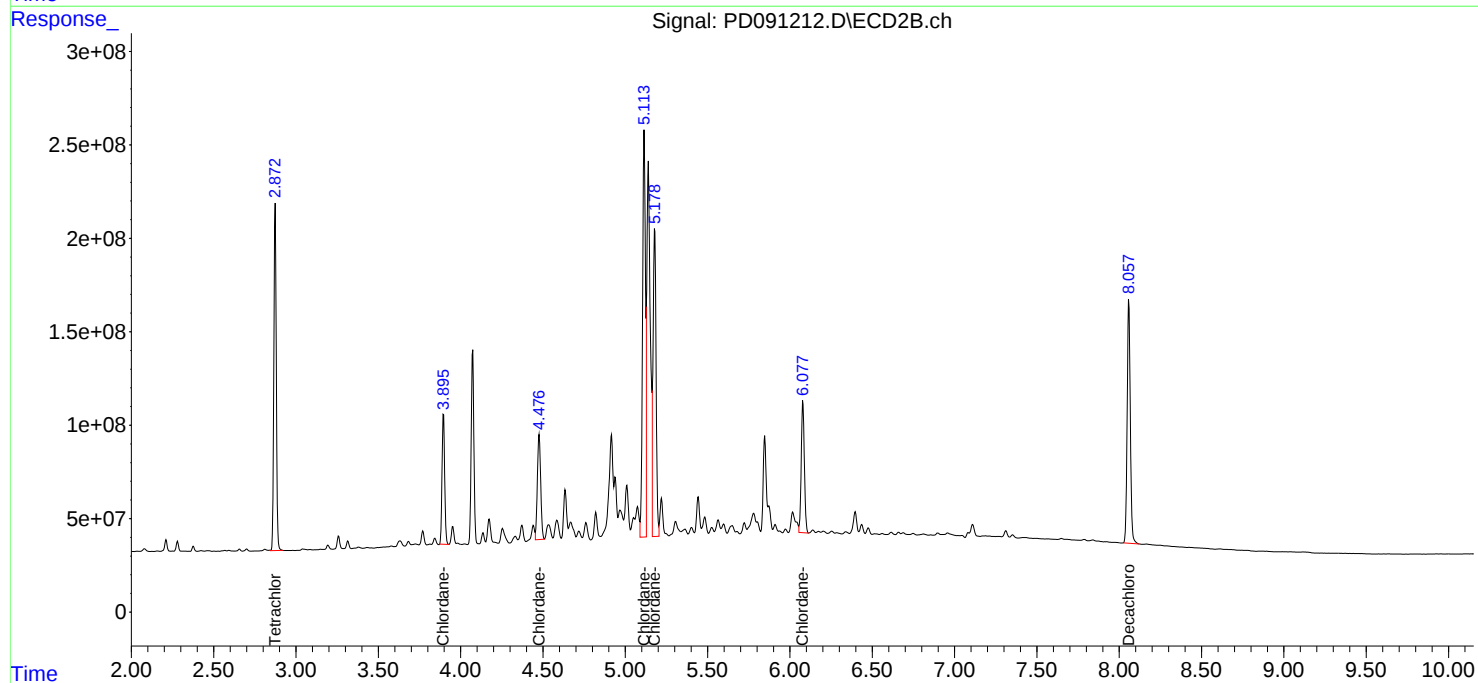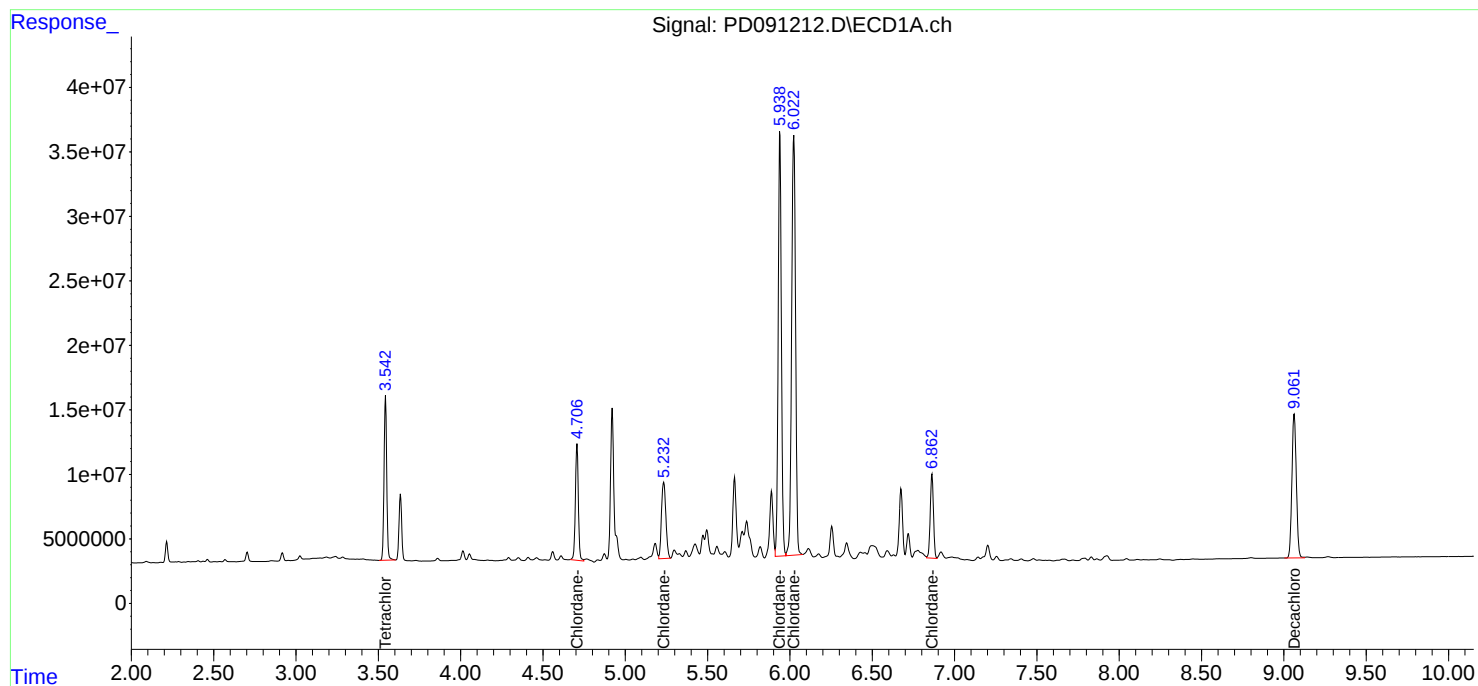


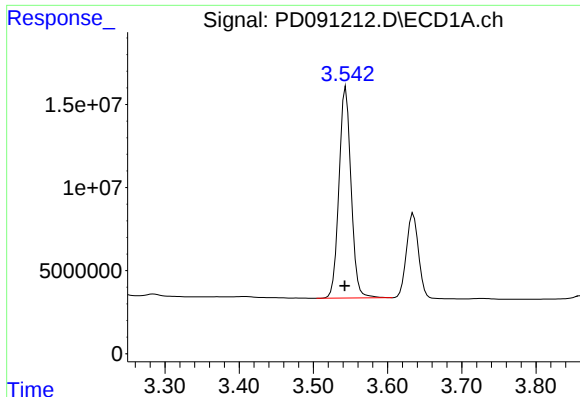

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.002 min
Response: 144027048
Conc: 45.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111525CHLOR

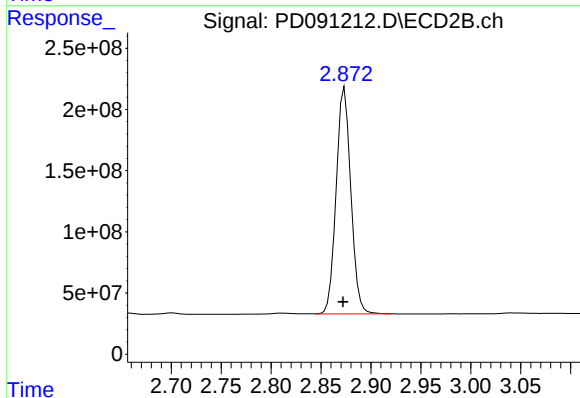


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.002 min
Response: 1897044359
Conc: 45.90 ng/ml

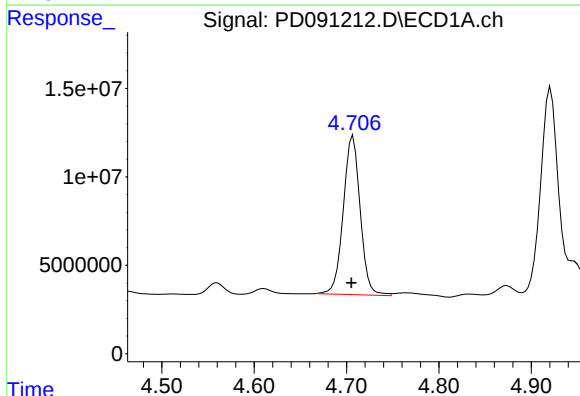


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.002 min
Response: 114205886
Conc: 464.14 ng/ml

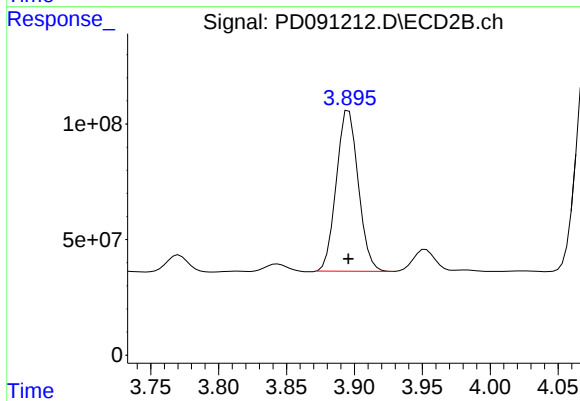

#23 Chlordane-1


R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 783265670
Conc: 455.31 ng/ml

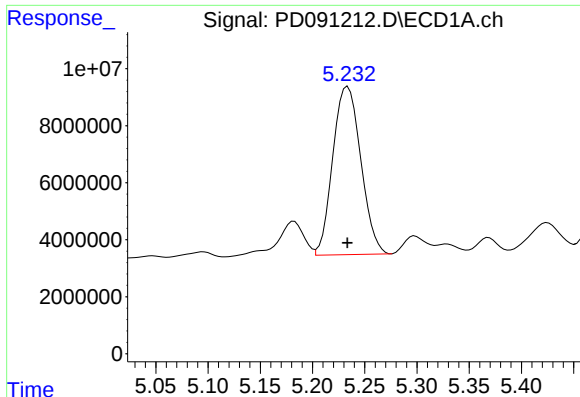

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 110065519
Conc: 445.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111525CHLOR

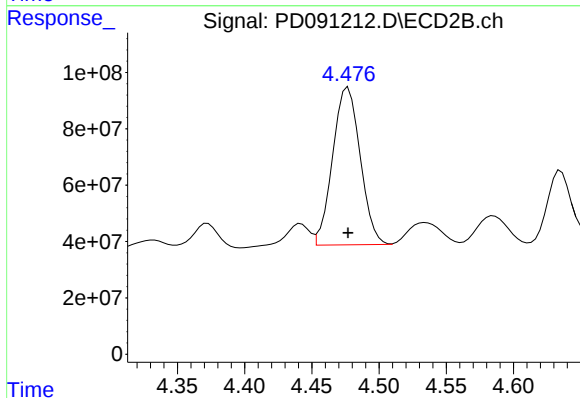


#24 Chlordane-2

R.T.: 4.477 min
Delta R.T.: 0.000 min
Response: 794593898
Conc: 453.79 ng/ml

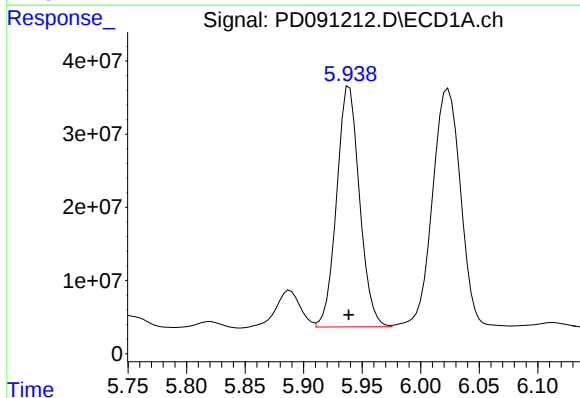


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 447116334
Conc: 463.41 ng/ml

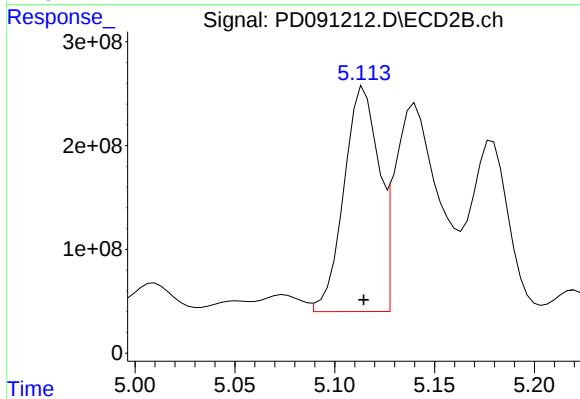

#25 Chlordane-3


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 2621481238
Conc: 455.63 ng/ml

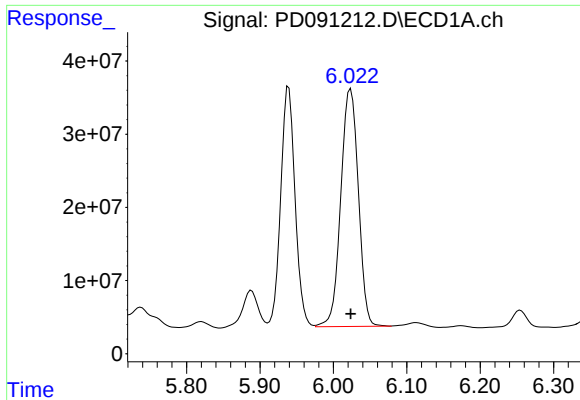

#26 Chlordane-4


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 540318465
Conc: 449.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111525CHLOR

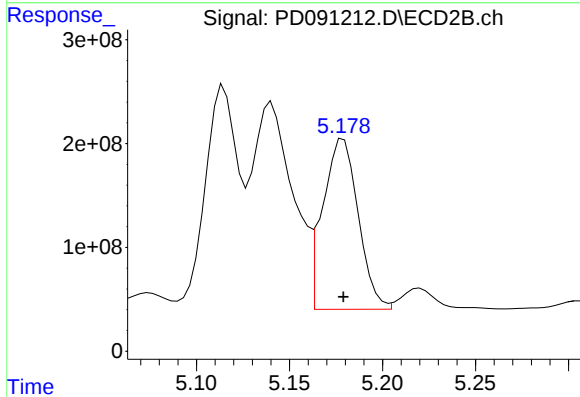


#26 Chlordane-4

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 2175161491
Conc: 454.72 ng/ml

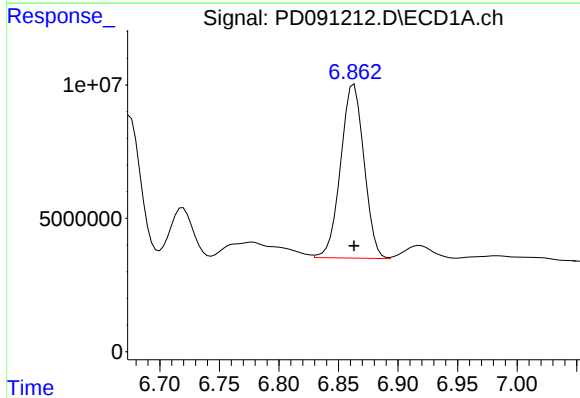


#27 Chlordane-5

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 88911954
Conc: 450.02 ng/ml

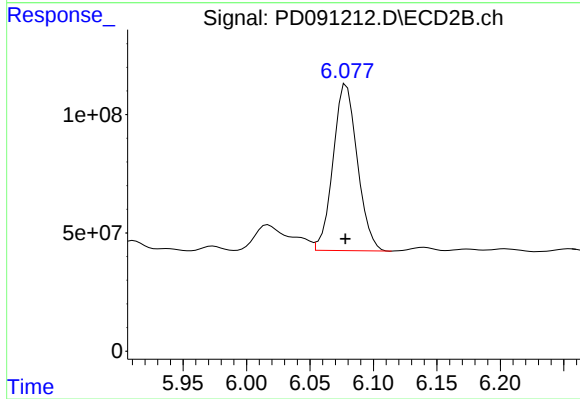

#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 936467238
Conc: 461.50 ng/ml

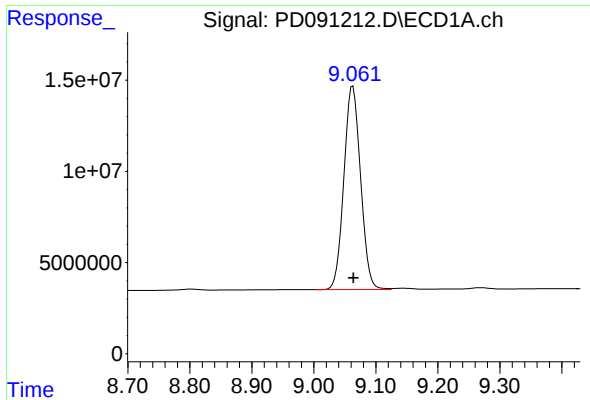

#28 Decachlorobiphenyl


R.T.: 9.063 min

Delta R.T.: 0.000 min

Response: 208069476

Conc: 44.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111525CHLOR

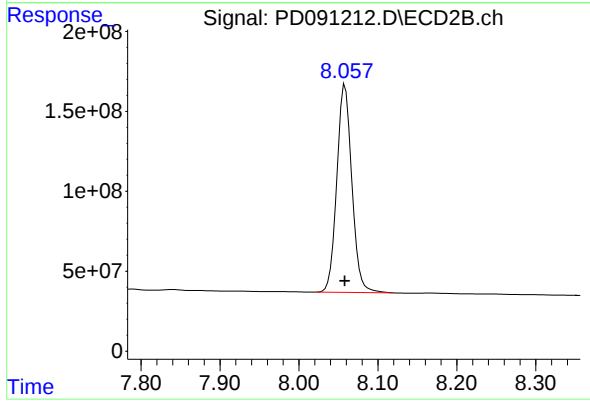

#28 Decachlorobiphenyl

R.T.: 8.059 min

Delta R.T.: 0.000 min

Response: 1722541005

Conc: 45.86 ng/ml