

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
 Data File : PD050342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Nov 2018 22:13
 Operator : AJ\SJ
 Sample : RESCHK
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:21:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	4.043	30813759	603.8E6	21.175	21.922
28)	SA Decachlor...	7.835	9.151	33143436	464.6E6	22.389	22.953
Target Compounds							
9)	A Endosulfan I	5.178	6.290	20490935	332.2E6	10.169	11.704
10)	B gamma-Chl...	5.074	6.166	22021672	368.0E6	9.993	11.613
12)	B 4,4'-DDE	5.301	6.395	42363895	644.8E6	20.671	21.929
13)	MA Dieldrin	5.415	6.548	46696511	678.4E6	21.145	22.514
19)	B Endosulfa...	6.307	7.323	37201119	508.6E6	20.056	20.876
20)	A Methoxychlor	6.582	7.644	102.3E6	1106.3E6	107.200	99.501
21)	B Endrin ke...	6.783	7.796	39122894	442.5E6	18.099	19.091



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
Data File : PD050342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Nov 2018 22:13
Operator : AJ\SJ
Sample : RESCHK
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:21:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

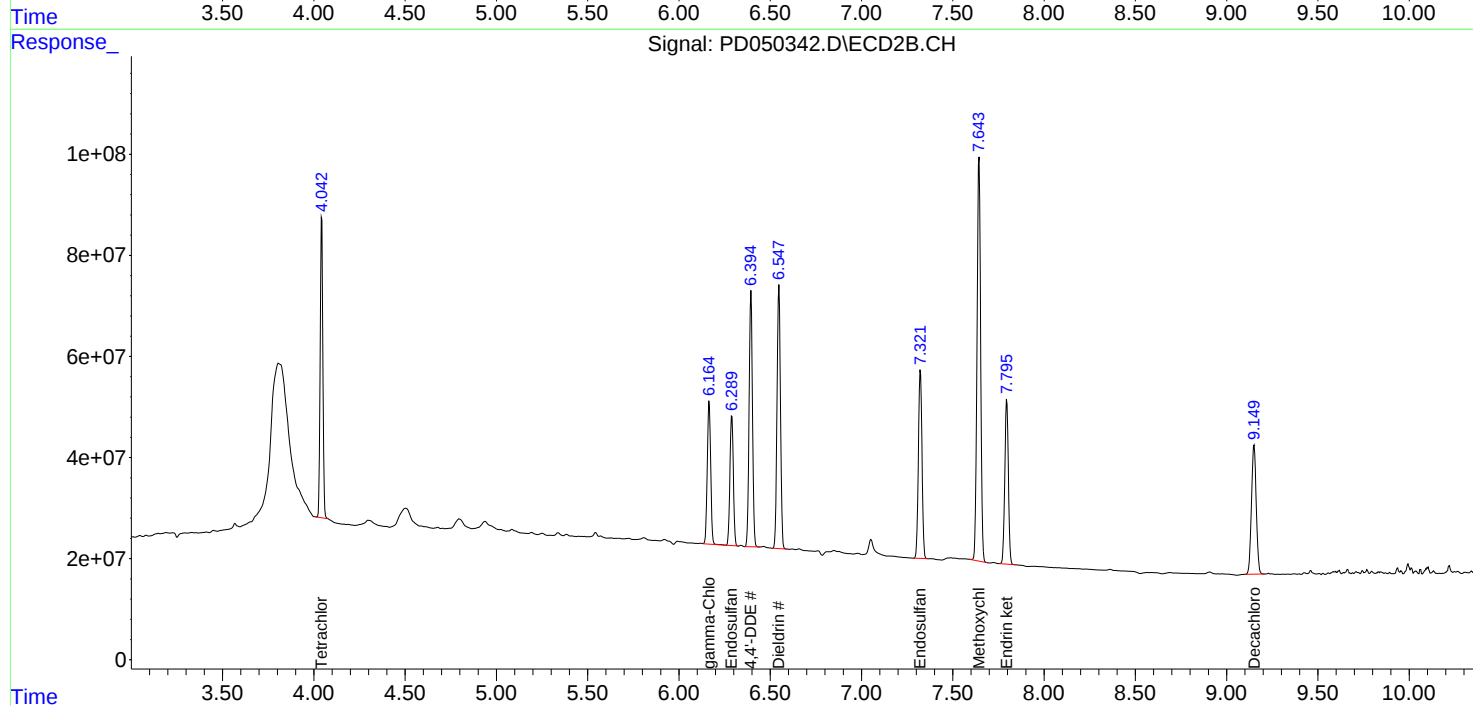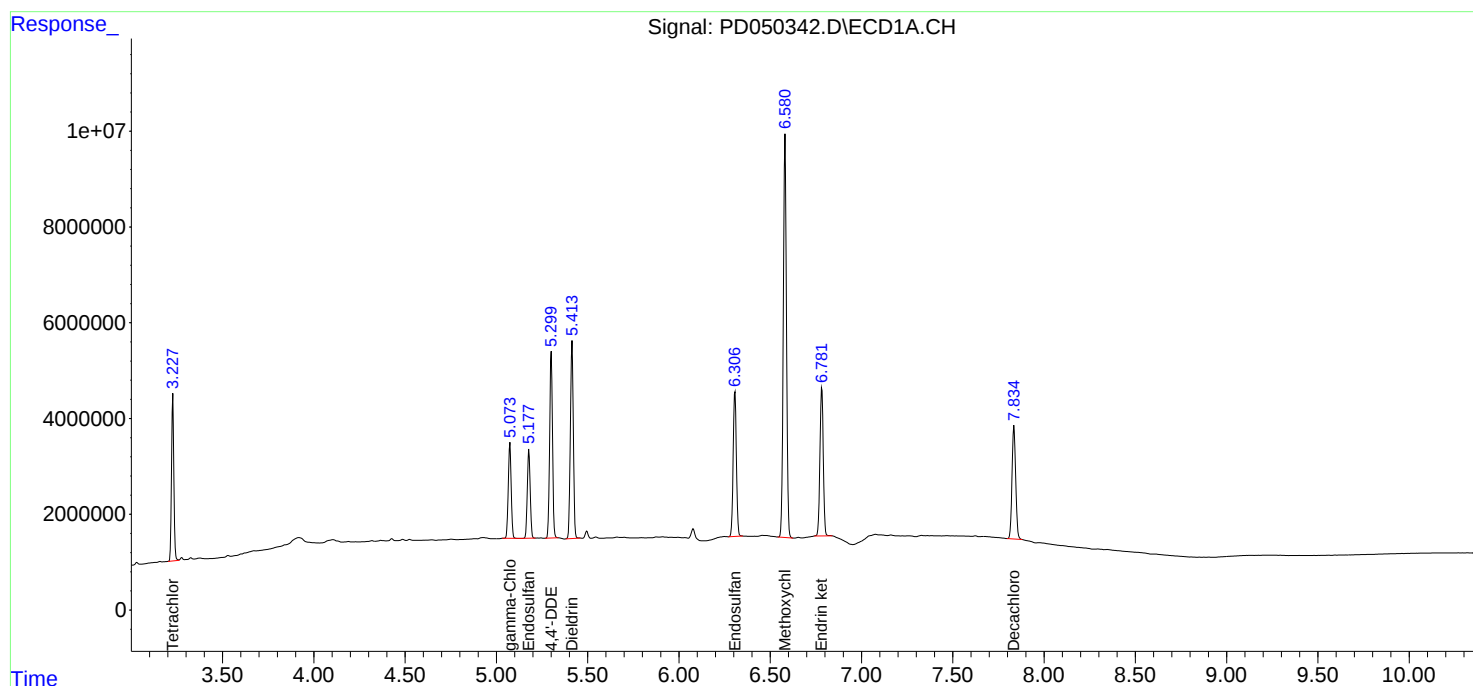


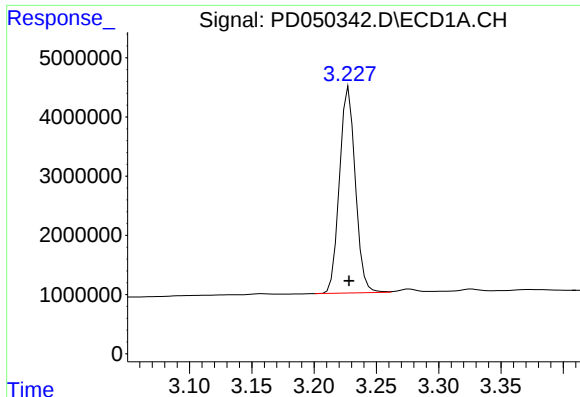

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 30813759
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

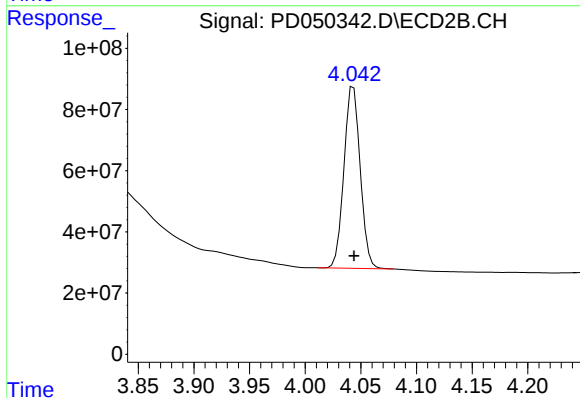


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 603815842
Conc: 21.92 ng/ml

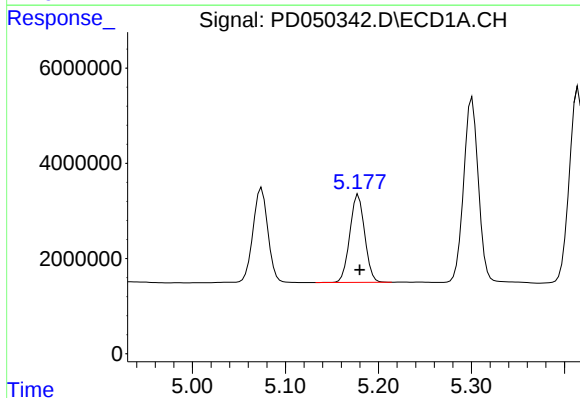


#9 Endosulfan I

R.T.: 5.178 min
Delta R.T.: -0.001 min
Response: 20490935
Conc: 10.17 ng/ml

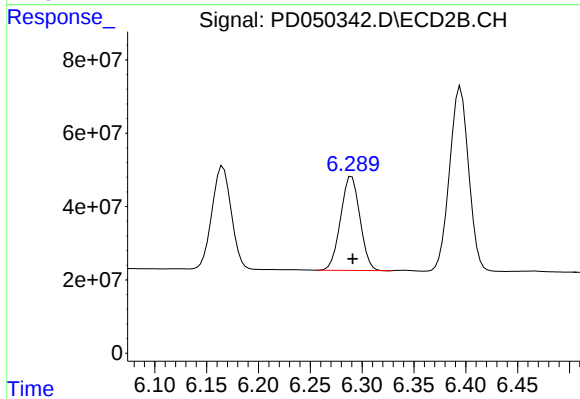

#9 Endosulfan I


R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 332197903
Conc: 11.70 ng/ml

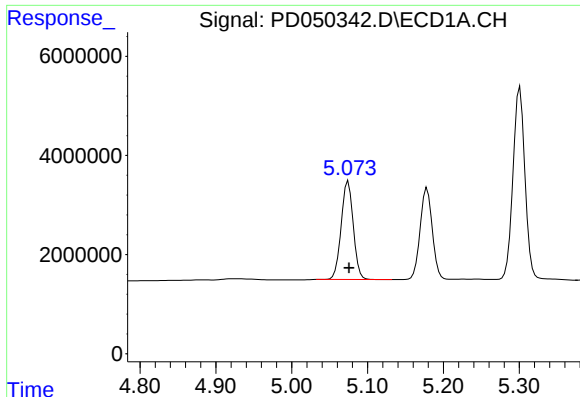

#10 gamma-Chlordane


R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 22021672
Conc: 9.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

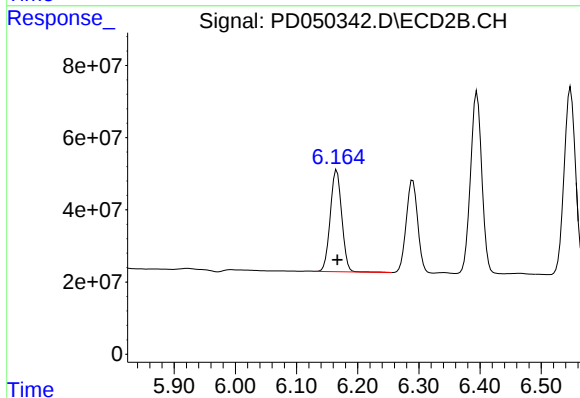


#10 gamma-Chlordane

R.T.: 6.166 min
Delta R.T.: -0.001 min
Response: 368033148
Conc: 11.61 ng/ml

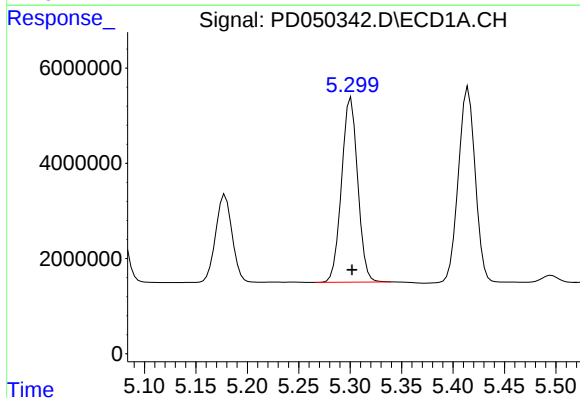


#12 4,4'-DDE

R.T.: 5.301 min
Delta R.T.: 0.000 min
Response: 42363895
Conc: 20.67 ng/ml

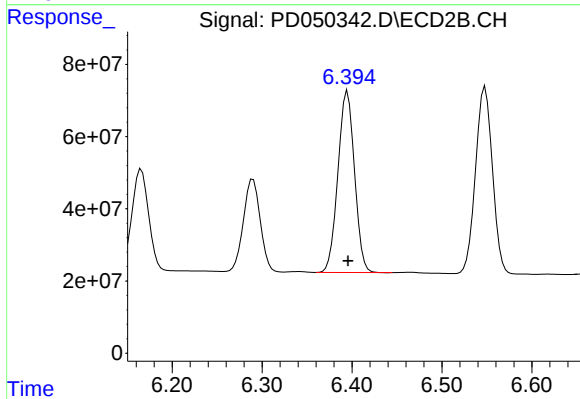

#12 4,4'-DDE


R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 644837937
Conc: 21.93 ng/ml

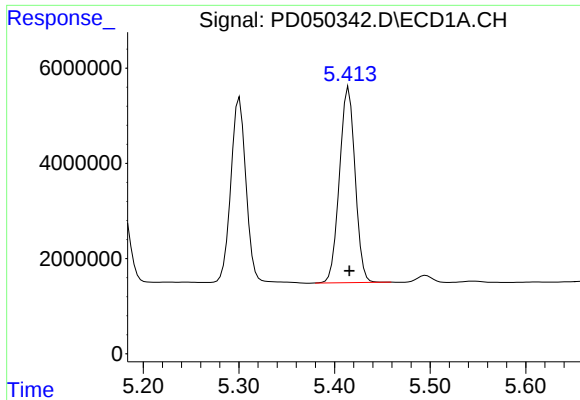

#13 Dieldrin


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 46696511
Conc: 21.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

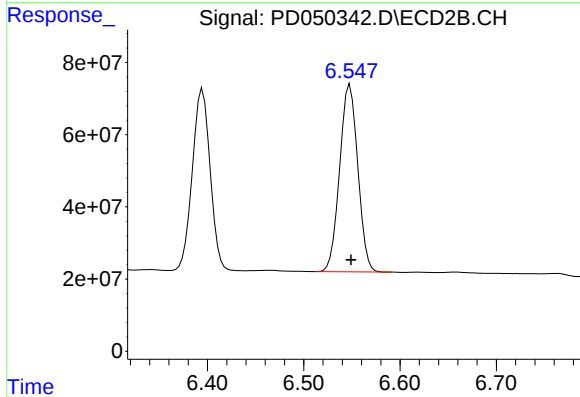


#13 Dieldrin

R.T.: 6.548 min
Delta R.T.: 0.000 min
Response: 678430669
Conc: 22.51 ng/ml

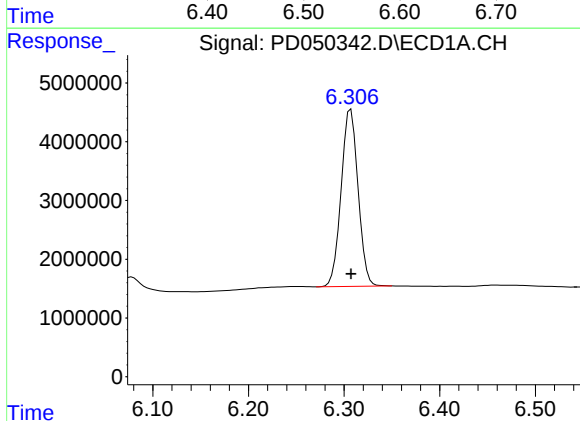


#19 Endosulfan Sulfate

R.T.: 6.307 min
Delta R.T.: 0.000 min
Response: 37201119
Conc: 20.06 ng/ml

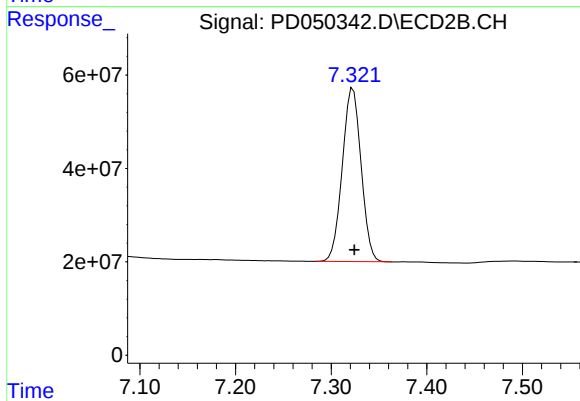

#19 Endosulfan Sulfate


R.T.: 7.323 min
Delta R.T.: -0.001 min
Response: 508593740
Conc: 20.88 ng/ml

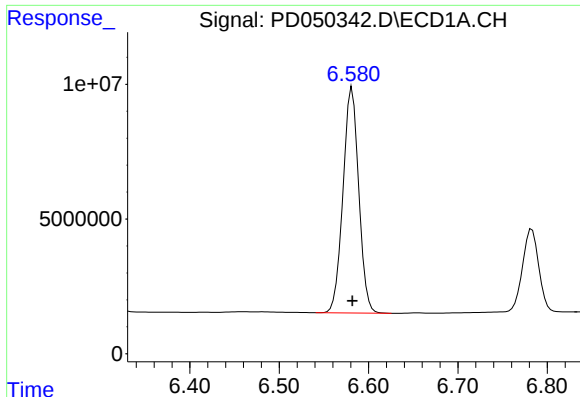

#20 Methoxychlor


R.T.: 6.582 min
Delta R.T.: 0.000 min
Response: 102324852
Conc: 107.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

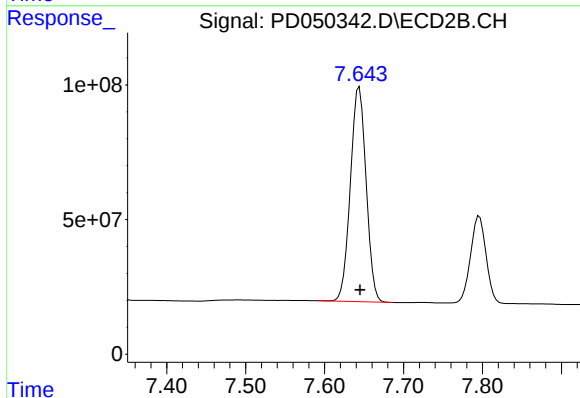


#20 Methoxychlor

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 1106338204
Conc: 99.50 ng/ml

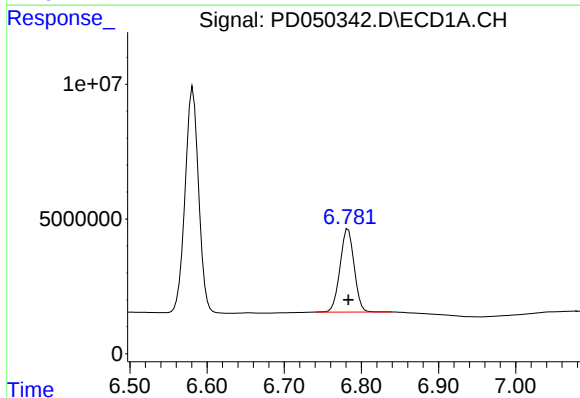


#21 Endrin ketone

R.T.: 6.783 min
Delta R.T.: 0.000 min
Response: 39122894
Conc: 18.10 ng/ml

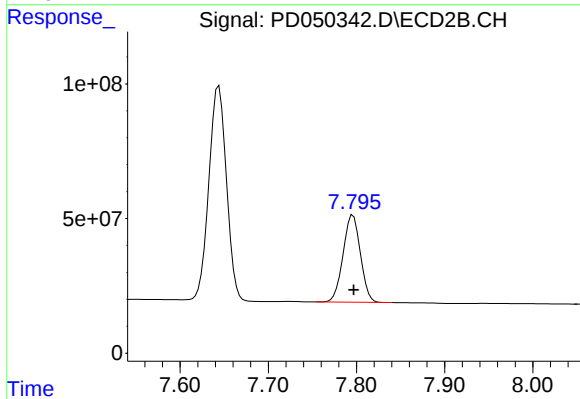

#21 Endrin ketone


R.T.: 7.796 min
Delta R.T.: 0.000 min
Response: 442481135
Conc: 19.09 ng/ml

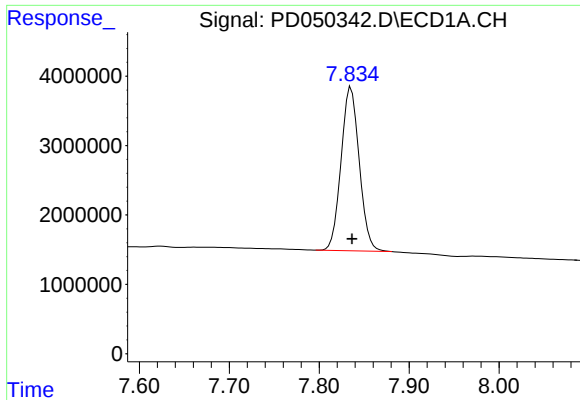

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.001 min
Response: 33143436
Conc: 22.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

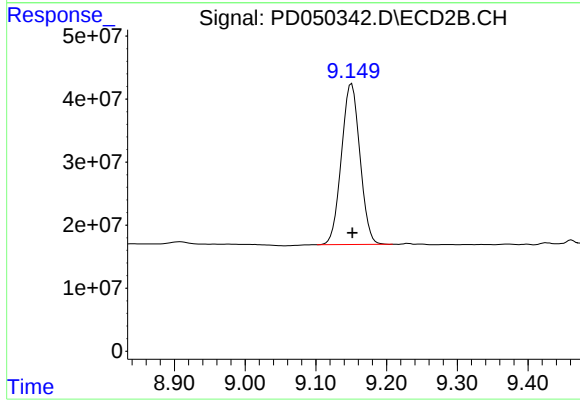

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: -0.001 min
Response: 464619338
Conc: 22.95 ng/ml