

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
 Data File : PD050396.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2018 12:13
 Operator : AJ\SJ
 Sample : J5952-05
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VTW-03(4-6)

Manual Integrations
 APPROVED

Sohil
 11/16/2018 3:58:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 12:40:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	4.043	9283556	190.6E6	6.380	6.918
28)	SA Decachlor...	7.836	9.150	10942831	221.5E6	7.392m	10.943m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
Data File : PD050396.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2018 12:13
Operator : AJ\SJ
Sample : J5952-05
Misc :
ALS Vial : 68 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
VTW-03(4-6)


Manual Integrations
APPROVED

Sohil
11/16/2018 3:58:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 12:40:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

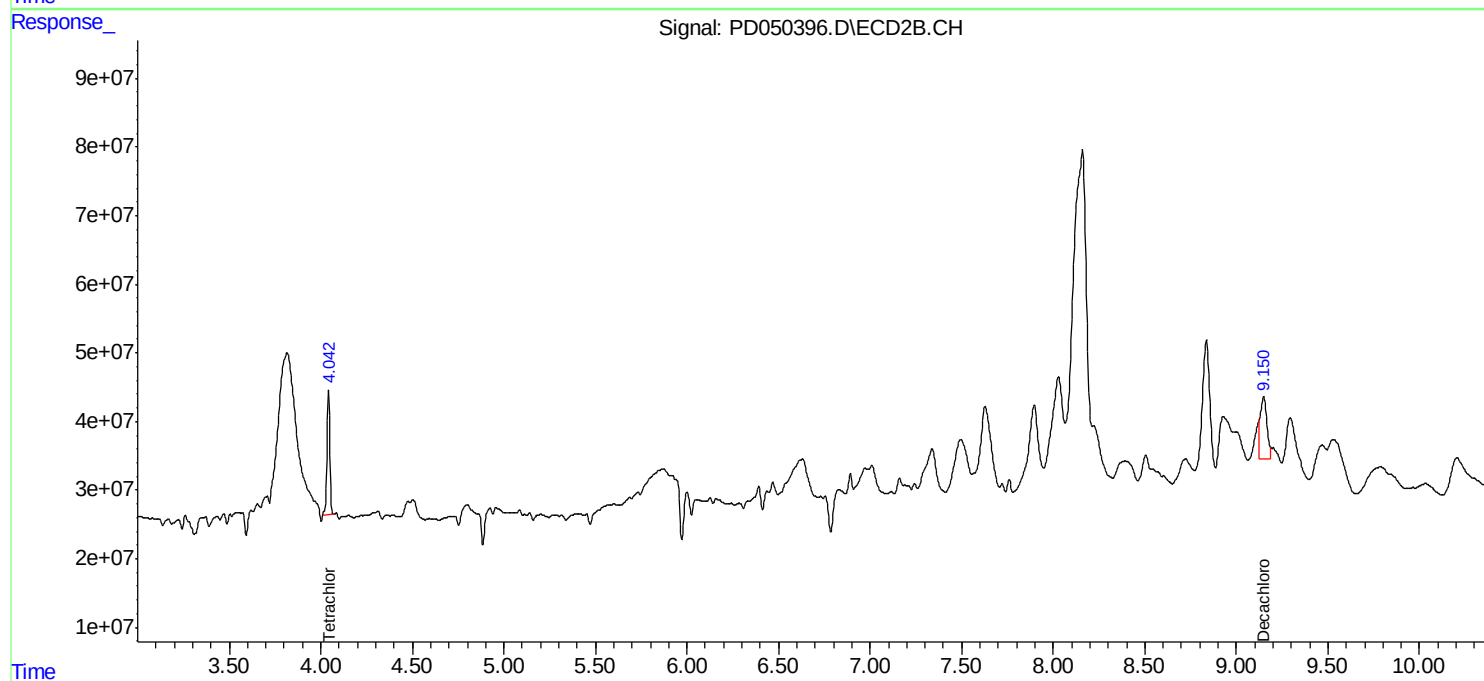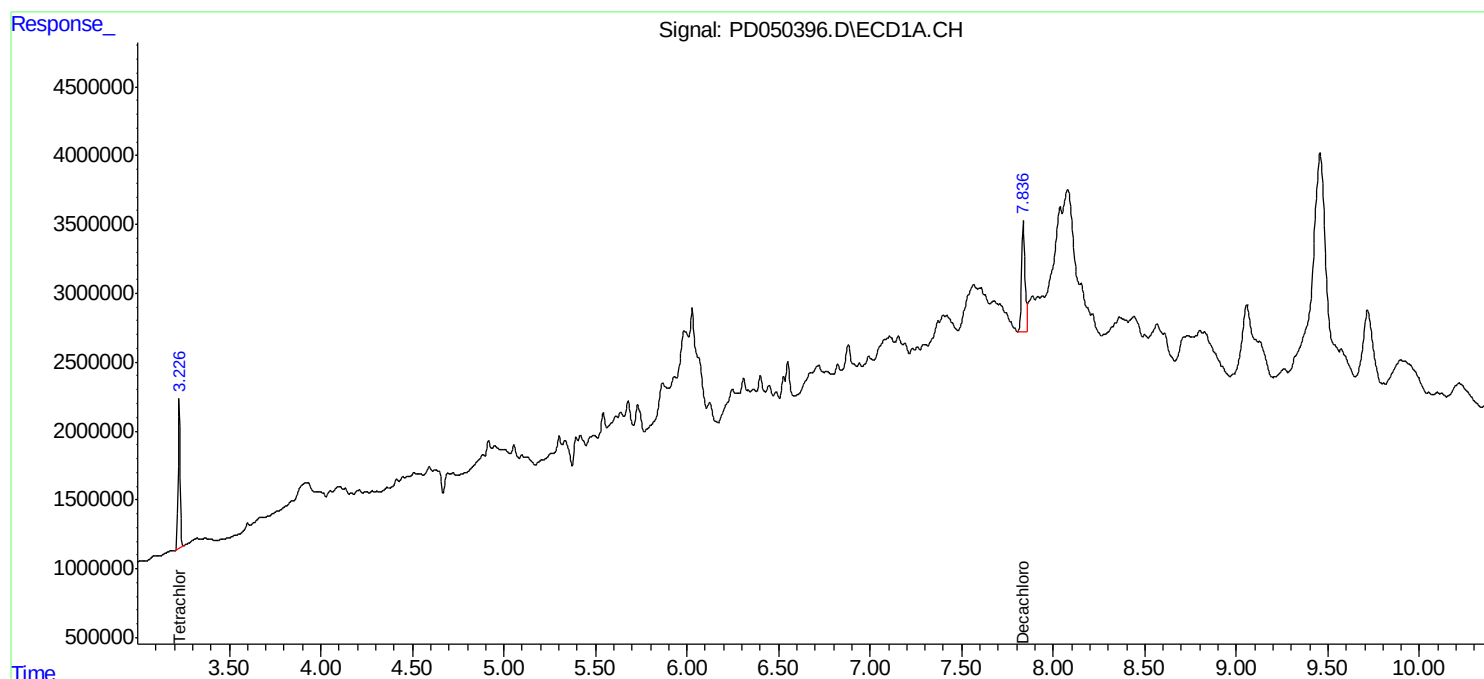

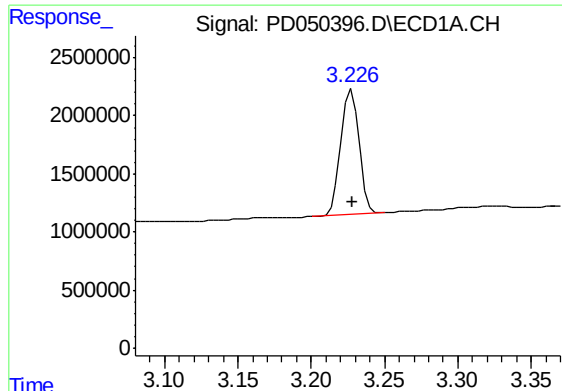


#1 Tetrachloro-m-xylene

R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 9283556
Conc: 6.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
VTW-03(4-6)


Manual Integrations
APPROVED

Sohil
11/16/2018 3:58:17 PM

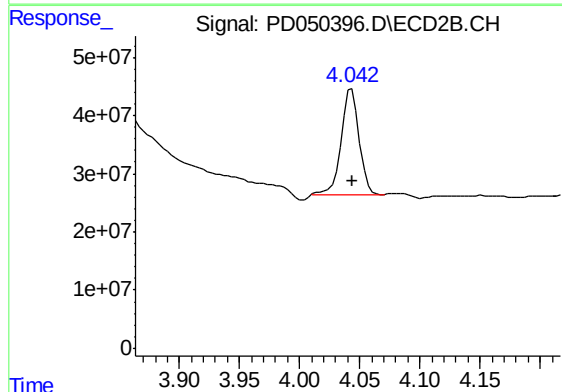


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 190556625
Conc: 6.92 ng/ml

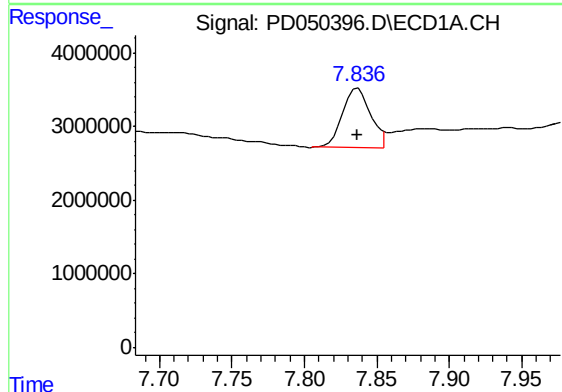

#28 Decachlorobiphenyl

R.T.: 7.836 min
Delta R.T.: -0.001 min
Response: 10942831
Conc: 7.39 ng/ml m

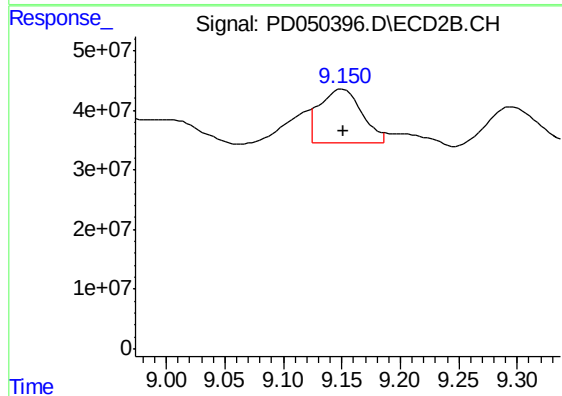

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: -0.002 min
Response: 221503162
Conc: 10.94 ng/ml m