

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
 Data File : PD050398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2018 12:41
 Operator : AJ\SJ
 Sample : J5952-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VTW-02(4-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 13:10:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	4.043	12531690	250.3E6	8.612	9.087
28)	SA Decachlor...	7.836	9.153	17524807	149.2E6	11.838	7.373 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111618\
Data File : PD050398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2018 12:41
Operator : AJ\SJ
Sample : J5952-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
VTW-02(4-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 13:10:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

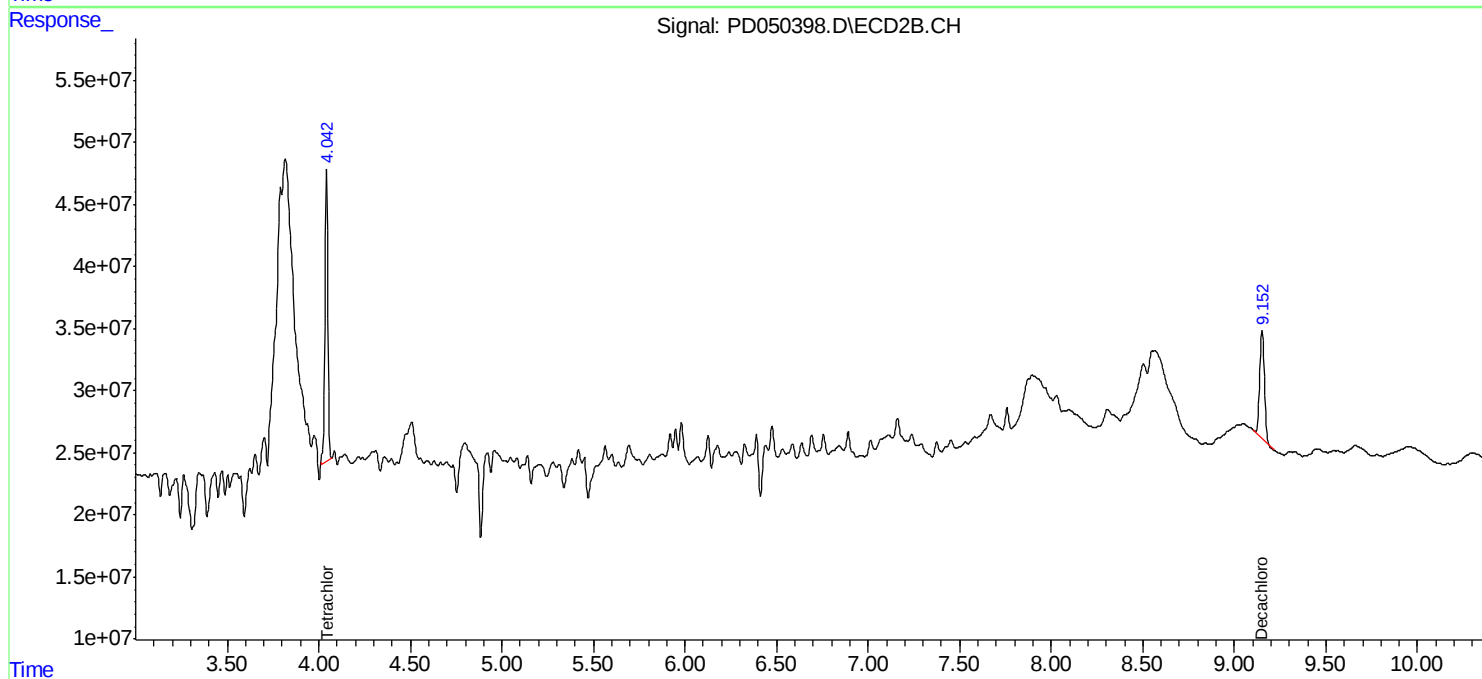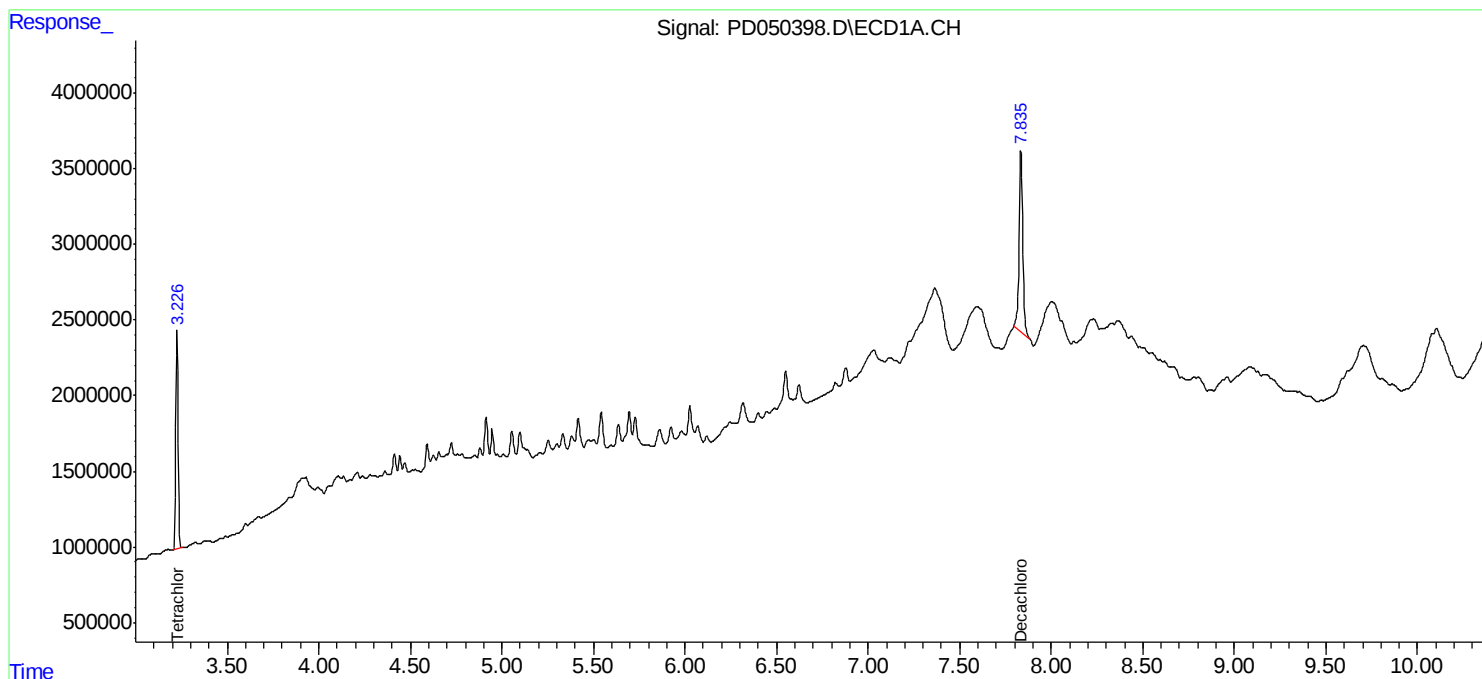


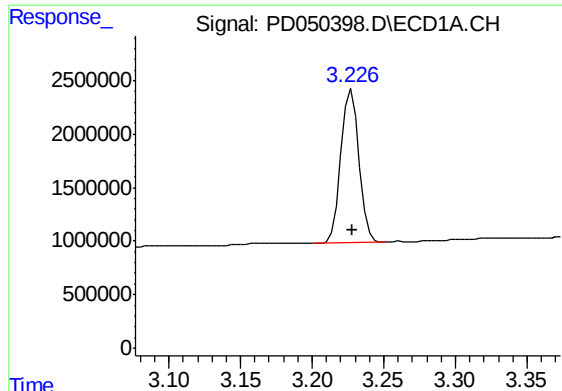

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 12531690
Conc: 8.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
VTW-02(4-6)

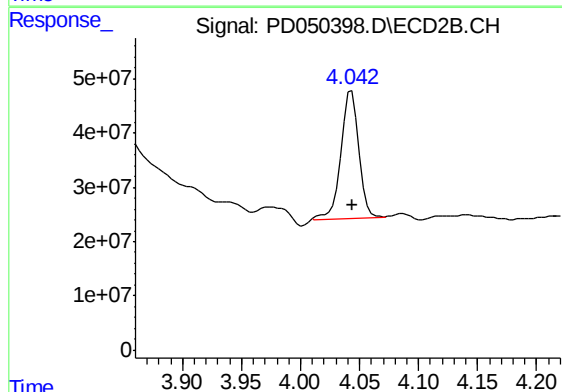


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 250291184
Conc: 9.09 ng/ml

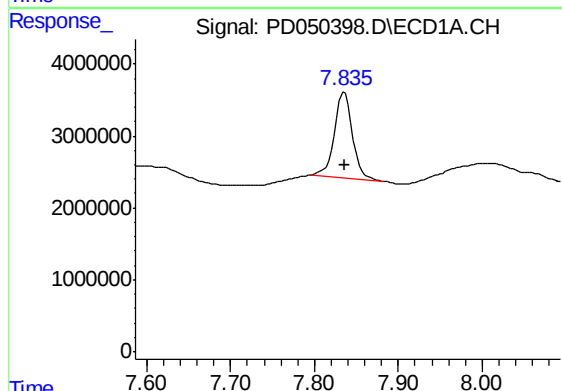

#28 Decachlorobiphenyl

R.T.: 7.836 min
Delta R.T.: 0.000 min
Response: 17524807
Conc: 11.84 ng/ml

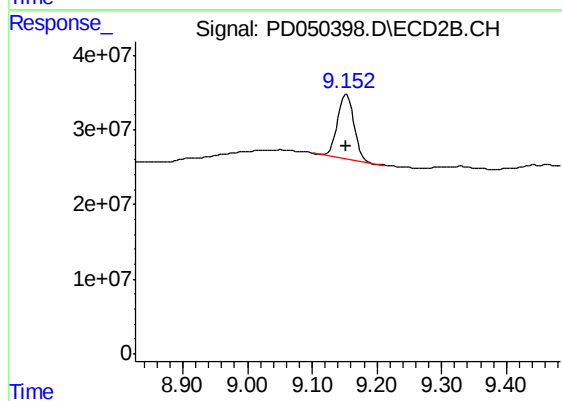

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.001 min
Response: 149248826
Conc: 7.37 ng/ml