

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111621\
 Data File : PD066965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2021 10:46
 Operator : AR\AJ
 Sample : M4623-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENTRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/17/2021
 Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:46:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.435	3.967	21671536	82267160	11.615m	10.166
28) SA Decachlor...	8.162	9.027	3523151	16561907	3.049	3.075m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111621\
Data File : PD066965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2021 10:46
Operator : AR\AJ
Sample : M4623-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/17/2021
Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:46:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

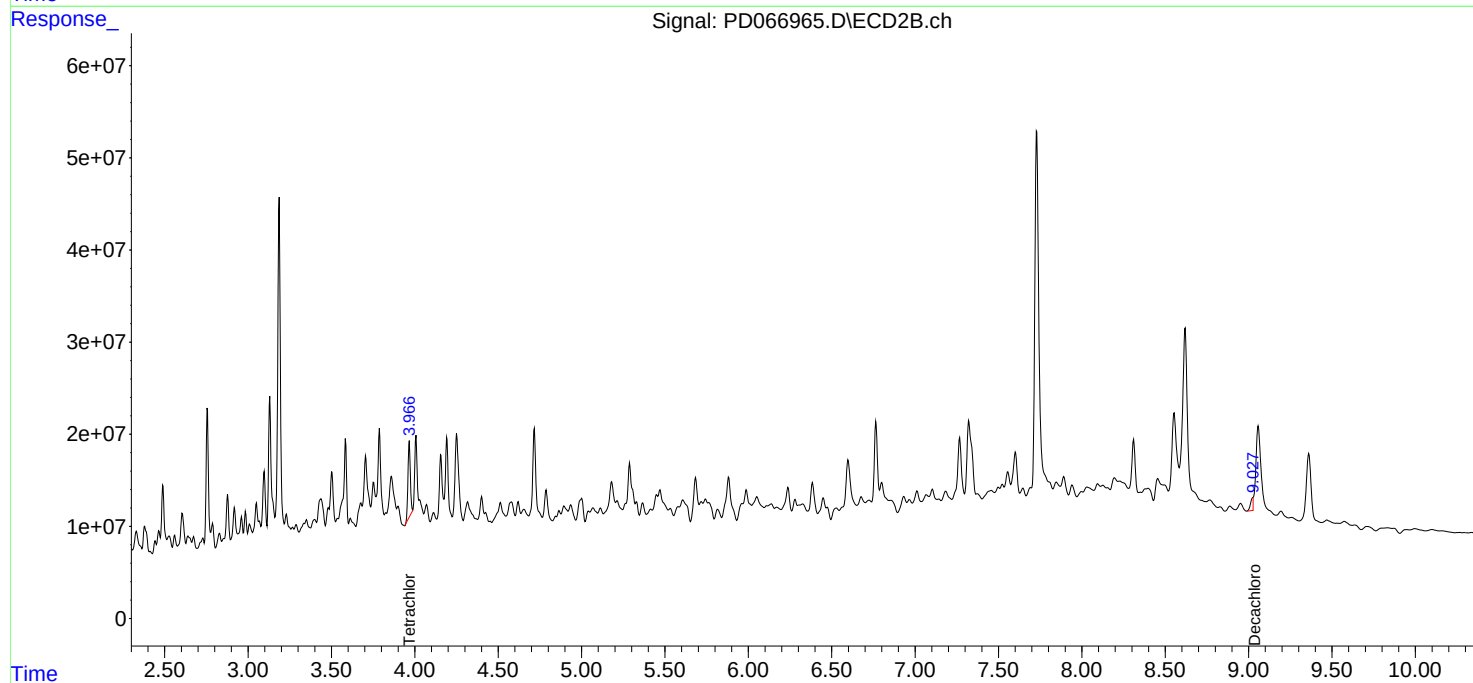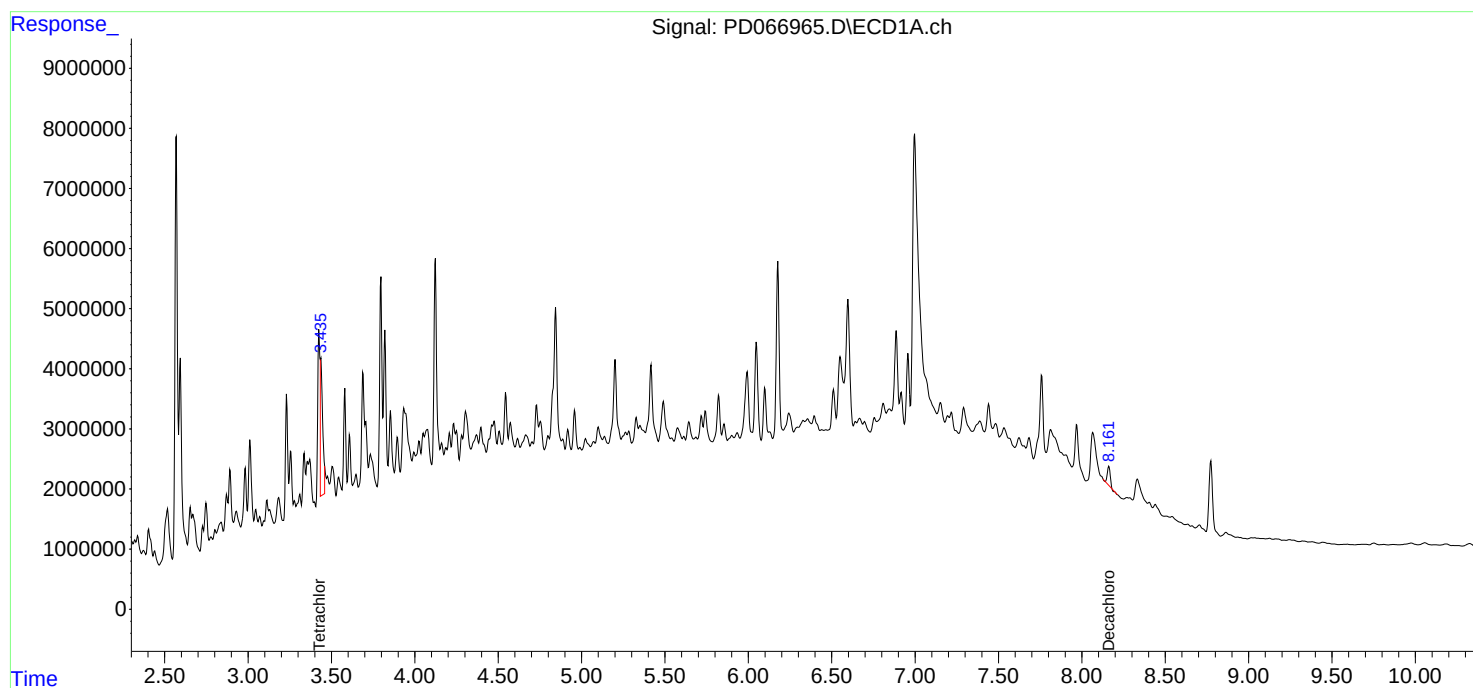

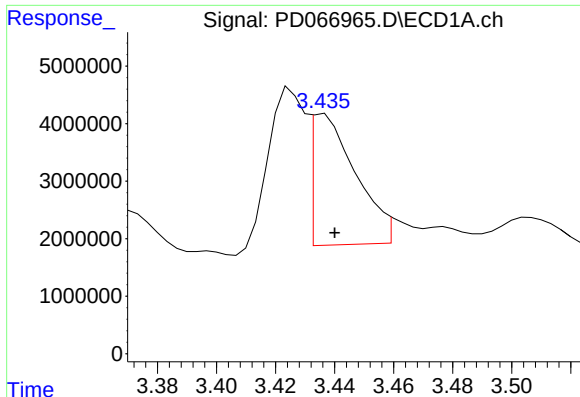


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.005 min
Response: 21671536
Conc: 11.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/17/2021
Supervised By :mohammad ahmed 11/18/2021

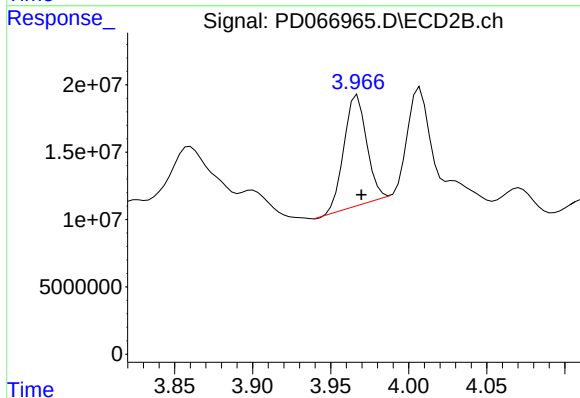


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.003 min
Response: 82267160
Conc: 10.17 ng/ml

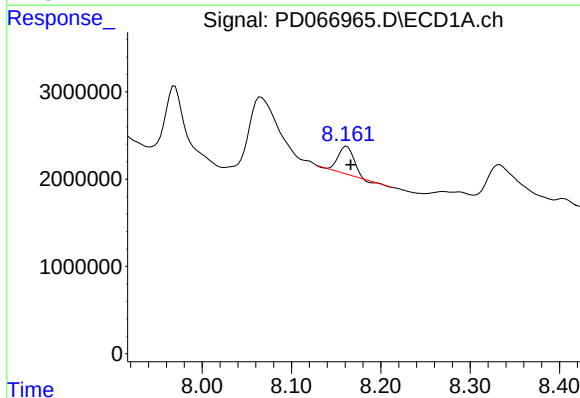

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: -0.004 min
Response: 3523151
Conc: 3.05 ng/ml

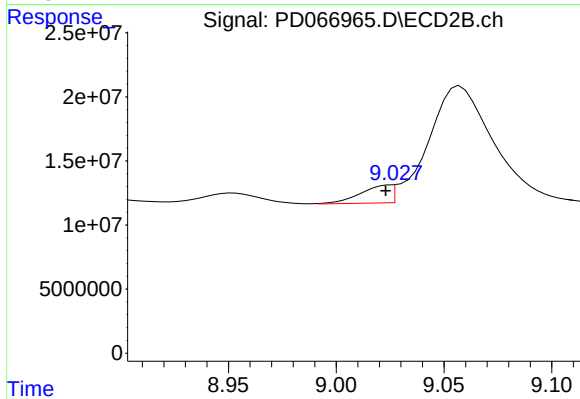

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.004 min
Response: 16561907
Conc: 3.07 ng/ml m