

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
 Data File : PD073022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 18:49
 Operator : AR\AJ
 Sample : PTOXICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 08:46:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 08:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.699	3.460	109.2E6	2801.9E6	50.000	50.000
7) SA Decachlor...	7.829	8.913	103.6E6	656.6E6	50.000	50.000
Target Compounds						
2) Toxaphene-1	5.245	5.767	7486262	66039656	500.000	500.000
3) Toxaphene-2	5.605	6.145	7887339	114.5E6	500.000	500.000
4) Toxaphene-3	6.520	7.056	23272356	225.2E6	500.000	500.000
5) Toxaphene-4	6.649	7.144	39965062	166.3E6	500.000	500.000
6) Toxaphene-5	6.960	7.841	22015918	172.6E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
Data File : PD073022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 18:49
Operator : AR\AJ
Sample : PTOXICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 08:46:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
Quant Title : GC Extractables
Qlast Update : Thu Nov 17 08:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Signal: PD073022.D\ECD1A.ch

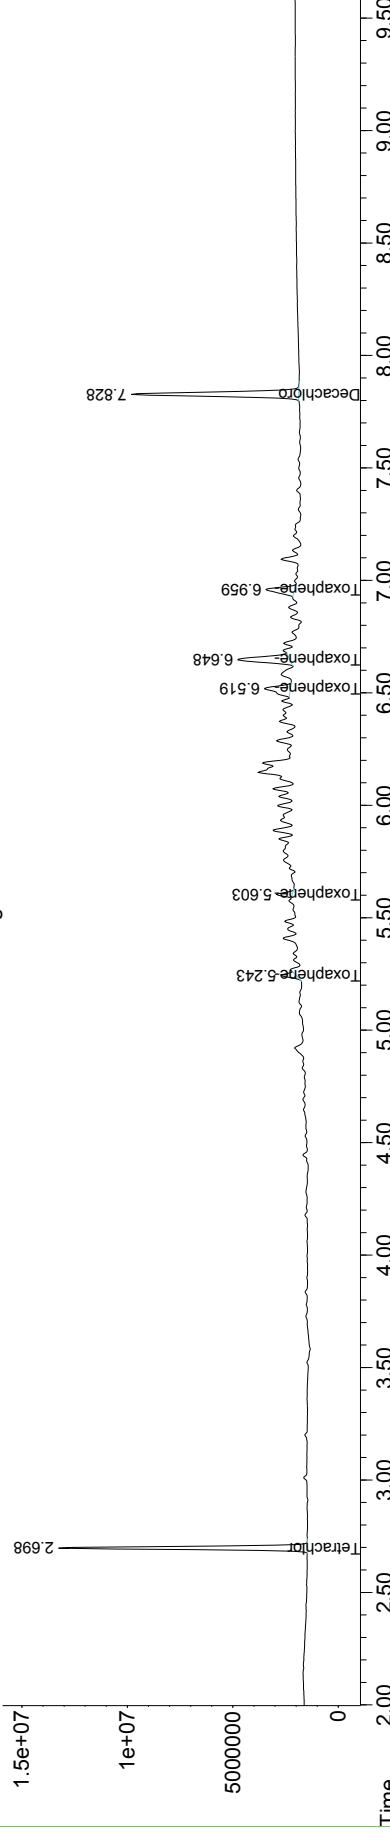

Signal: PD073022.D\ECD2B.ch

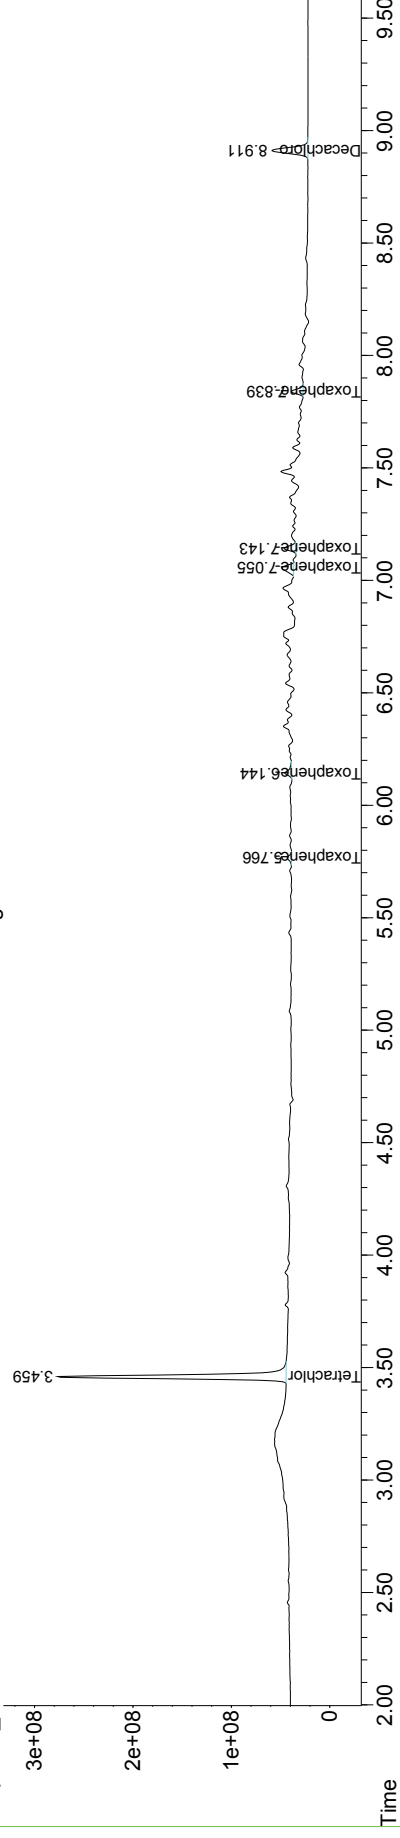

Instrument :
ECD_D
ClientSampleId :
PTOXICC500