

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
 Data File : PD073016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 17:30
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:12:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 02:12:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.459	181.5E6	4021.0E6	74.594	74.818
28)	SA Decachlor...	7.834	8.915	147.2E6	926.7E6	74.115	74.798
Target Compounds							
23)	Chlordane-1	3.697	4.609	58658780	973.9E6	735.935	697.482
24)	Chlordane-2	4.274	5.141	64831801	841.2E6	711.839	738.481
25)	Chlordane-3	4.904	5.849	220.3E6	2756.0E6	742.790	748.837
26)	Chlordane-4	4.966	5.925	214.9E6	3173.8E6	735.879	748.629
27)	Chlordane-5	5.863	6.783	71021651	542.0E6	741.494	749.408



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
Data File : PD073016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 17:30
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:12:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 02:12:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

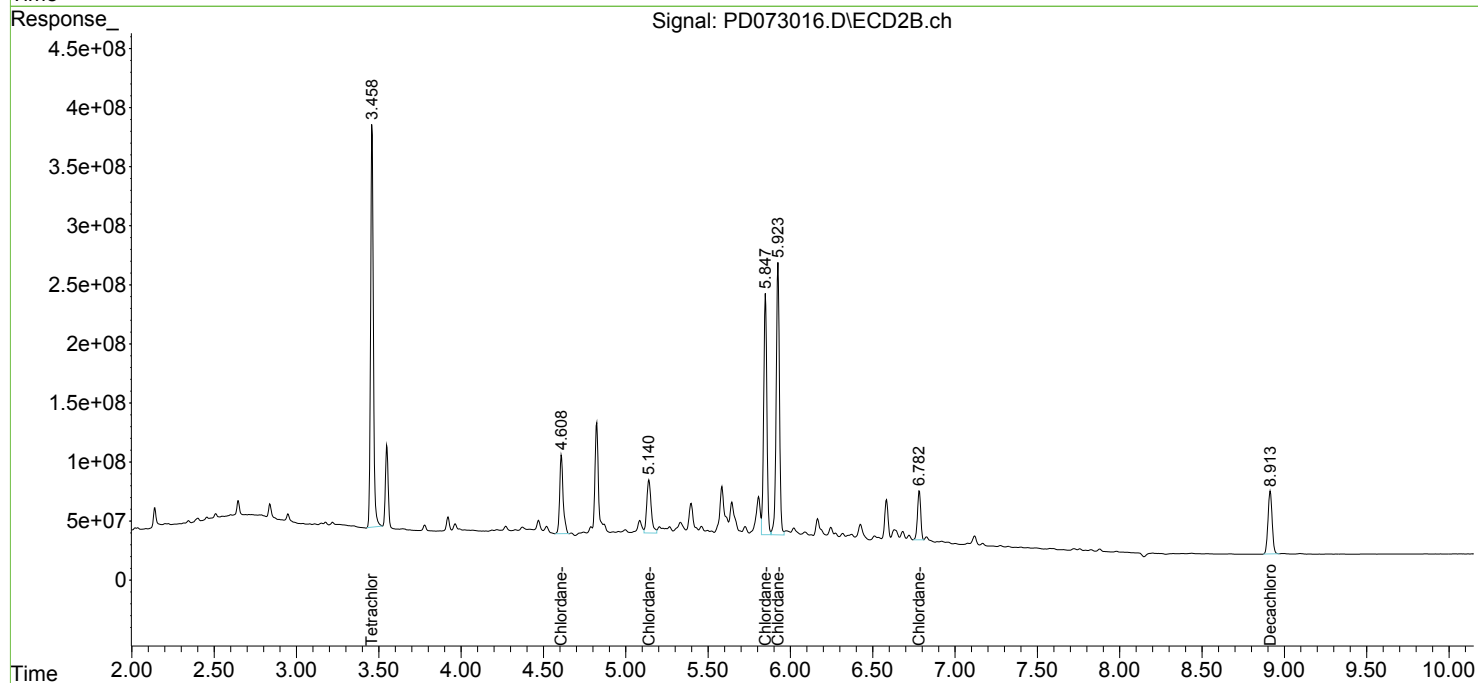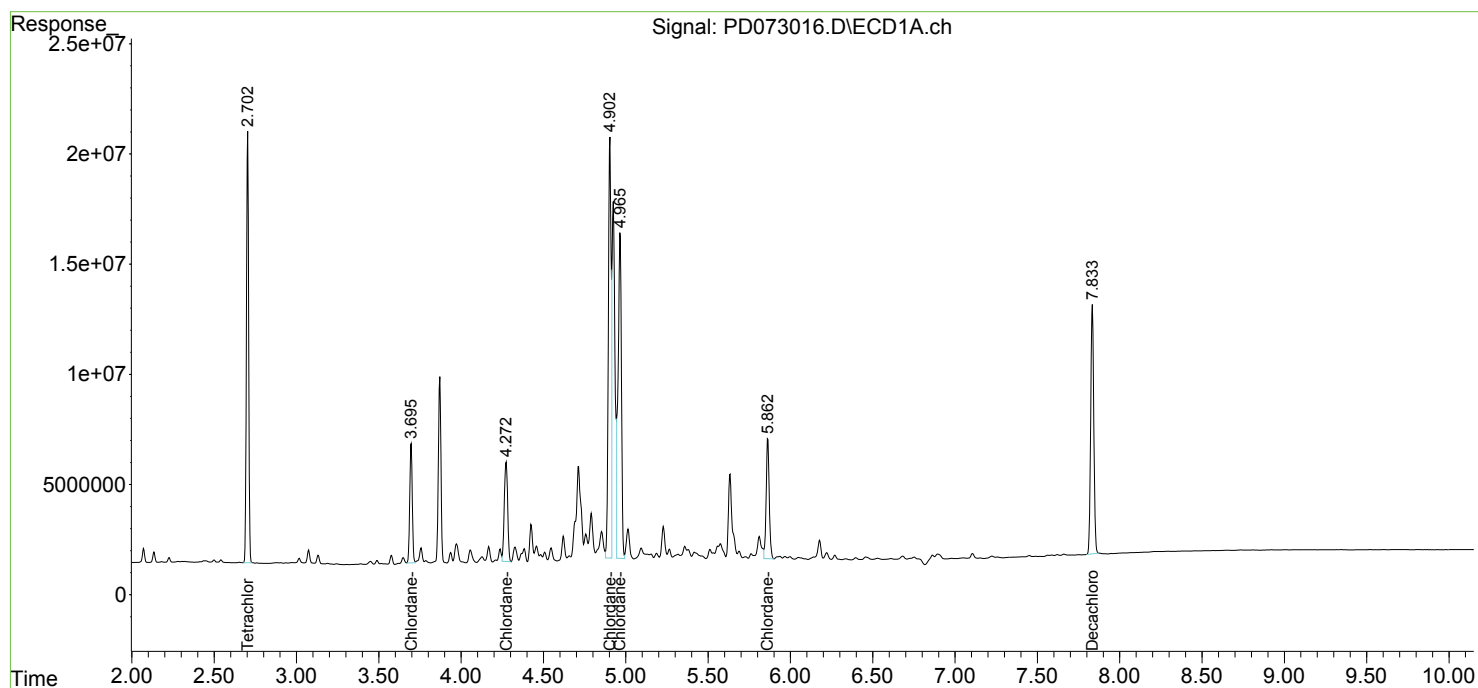


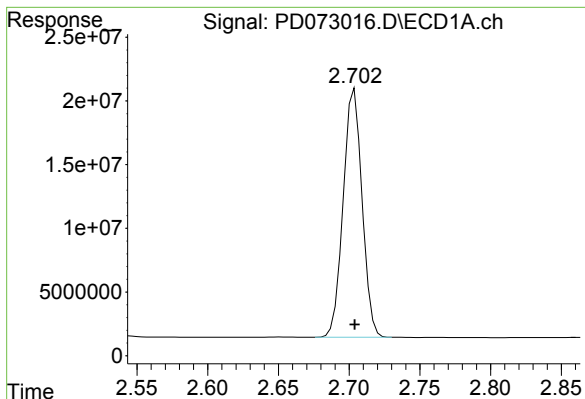

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 181494776
Conc: 74.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

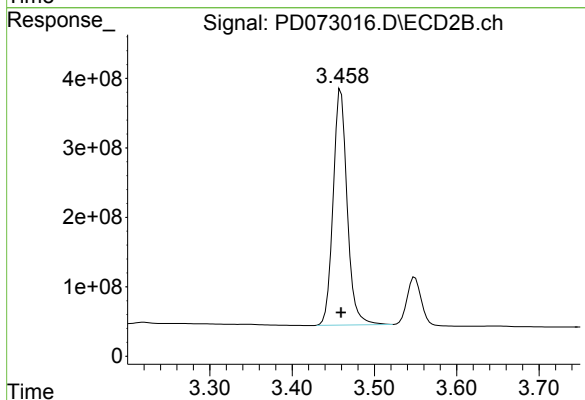


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 4021036413
Conc: 74.82 ng/ml

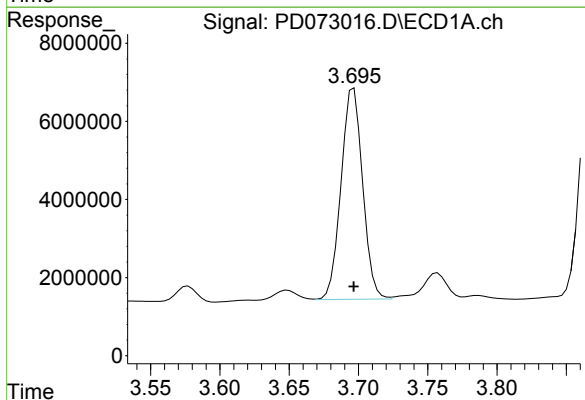


#23 Chlordane-1

R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 58658780
Conc: 735.94 ng/ml

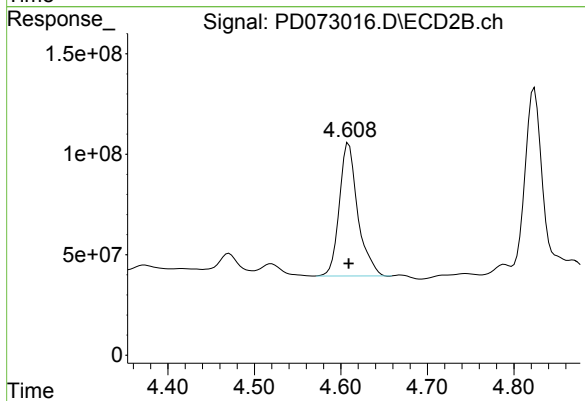

#23 Chlordane-1


R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 973862330
Conc: 697.48 ng/ml

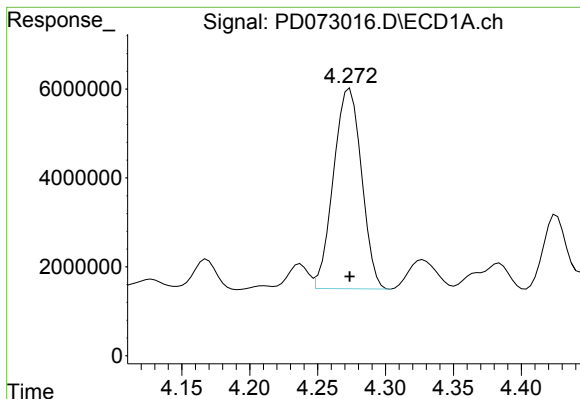

#24 Chlordane-2


R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 64831801
Conc: 711.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

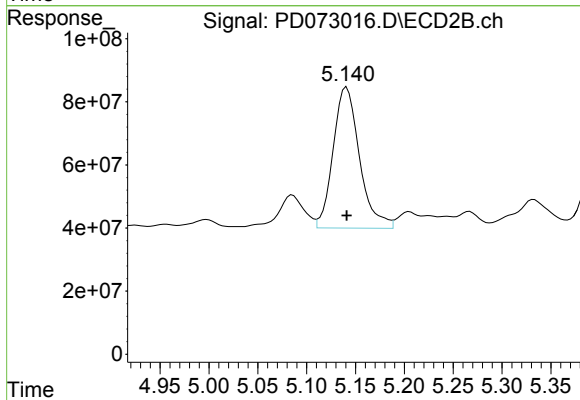


#24 Chlordane-2

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 841203917
Conc: 738.48 ng/ml

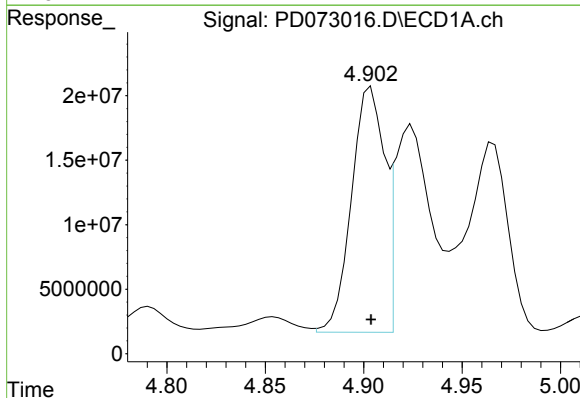


#25 Chlordane-3

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 220275682
Conc: 742.79 ng/ml

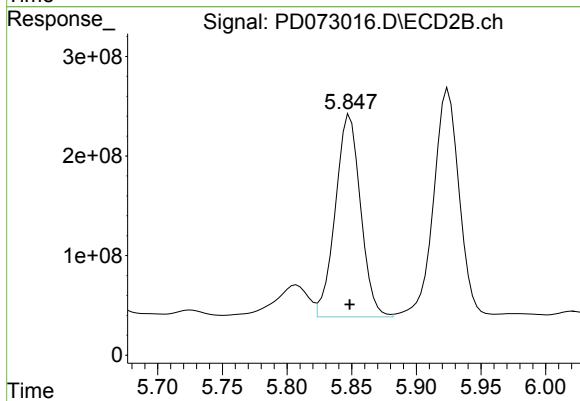

#25 Chlordane-3


R.T.: 5.849 min
Delta R.T.: 0.000 min
Response: 2756002109
Conc: 748.84 ng/ml

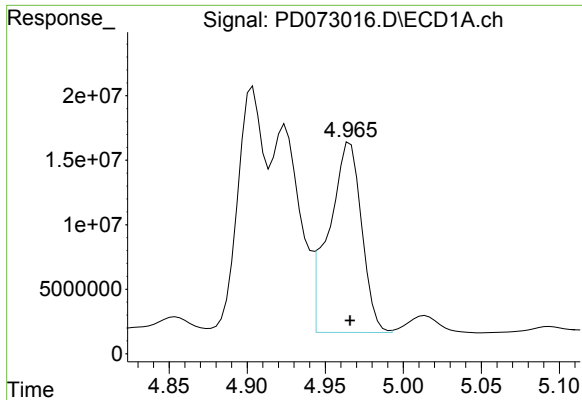

#26 Chlordane-4


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 214902906
Conc: 735.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

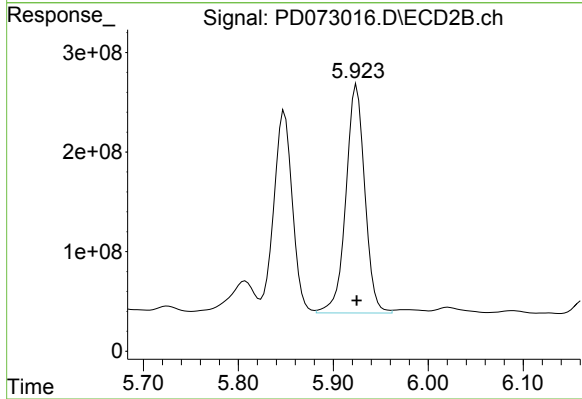


#26 Chlordane-4

R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 3173773532
Conc: 748.63 ng/ml

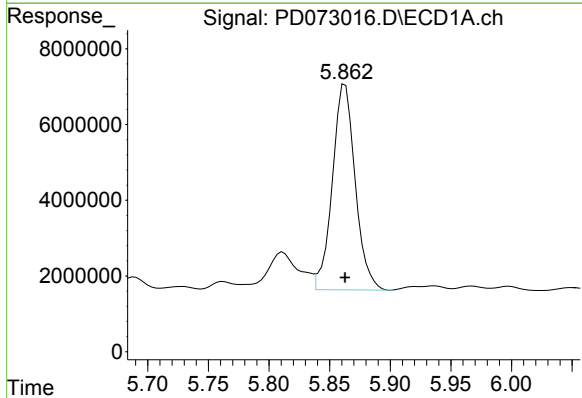


#27 Chlordane-5

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 71021651
Conc: 741.49 ng/ml

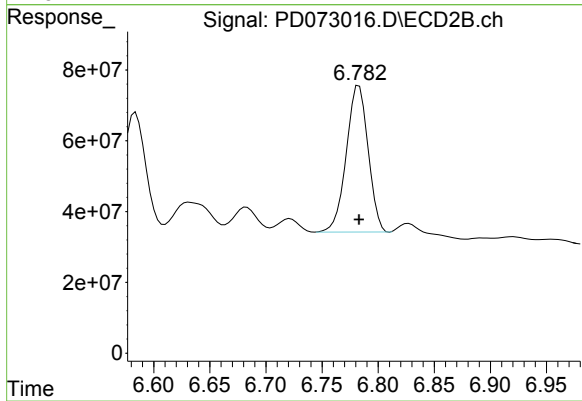

#27 Chlordane-5


R.T.: 6.783 min
Delta R.T.: 0.000 min
Response: 541981910
Conc: 749.41 ng/ml

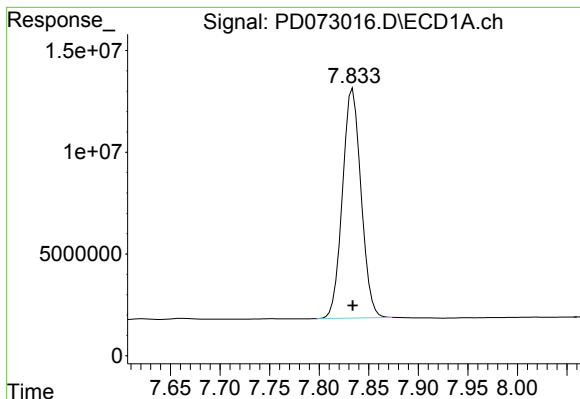

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: 0.000 min
Response: 147230715
Conc: 74.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

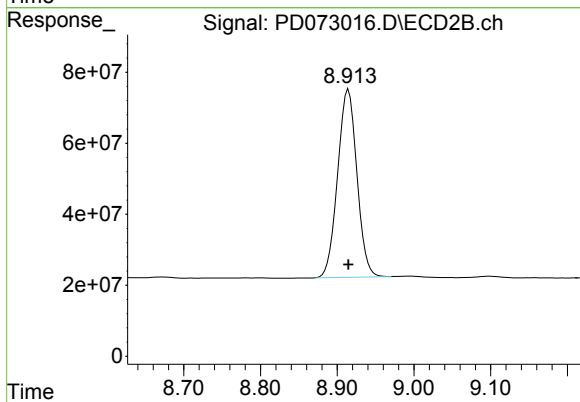

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.000 min
Response: 926679517
Conc: 74.80 ng/ml