

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
 Data File : PD073018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 17:56
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:14:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 02:14:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.460	56825152	1389.0E6	23.746	25.628
28)	SA Decachlor...	7.829	8.912	52332935	328.0E6	25.995	26.087
Target Compounds							
23)	Chlordane-1	3.690	4.609	20060716	404.3E6	251.260	278.520
24)	Chlordane-2	4.267	5.141	25202181	328.1E6	269.515	277.508
25)	Chlordane-3	4.897	5.848	69306877	944.0E6	237.579	254.834
26)	Chlordane-4	4.960	5.924	69073019	1092.3E6	239.754	255.692
27)	Chlordane-5	5.857	6.782	23523611	186.2E6	246.682	255.599



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
Data File : PD073018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 17:56
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:14:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 02:14:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

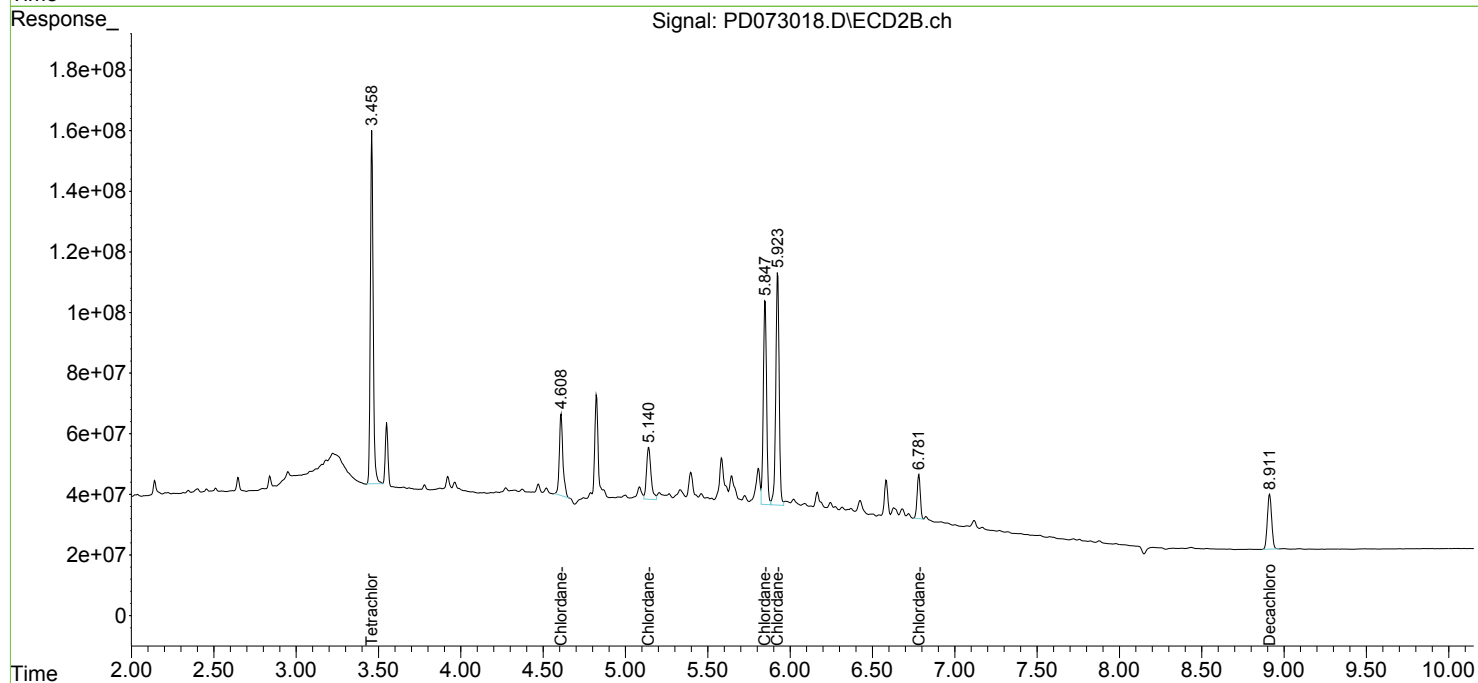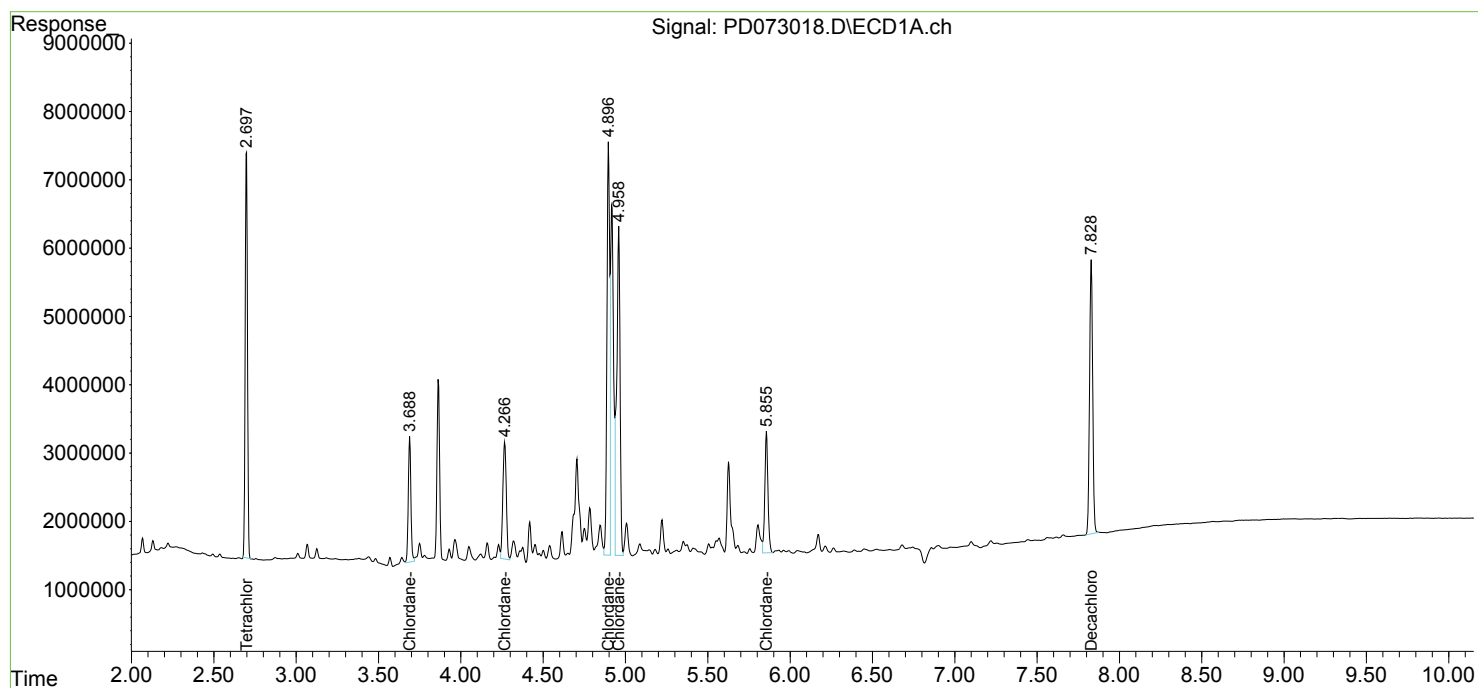


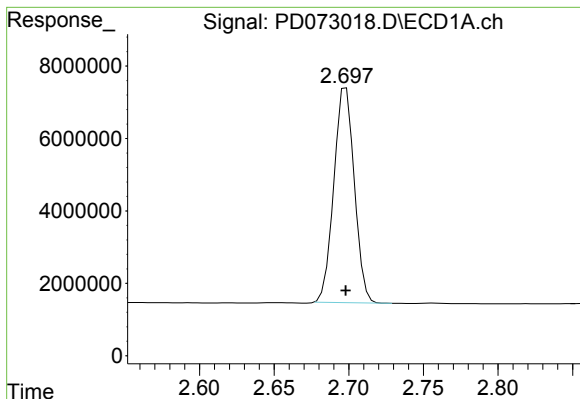

#1 Tetrachloro-m-xylene


R.T.: 2.698 min
Delta R.T.: 0.000 min
Response: 56825152
Conc: 23.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

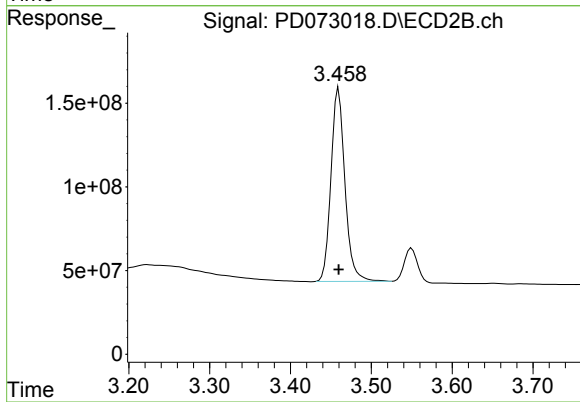


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 1388996409
Conc: 25.63 ng/ml

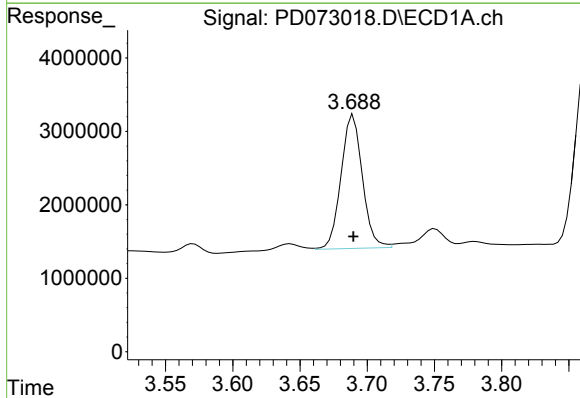


#23 Chlordane-1

R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 20060716
Conc: 251.26 ng/ml

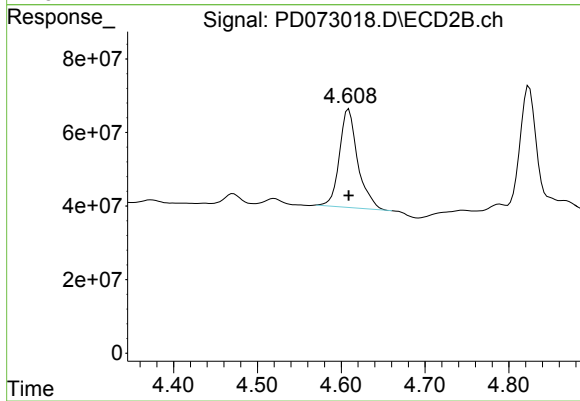

#23 Chlordane-1


R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 404258200
Conc: 278.52 ng/ml

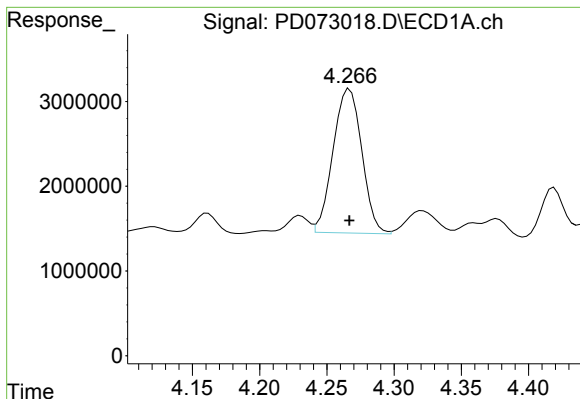

#24 Chlordane-2


R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 25202181
Conc: 269.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

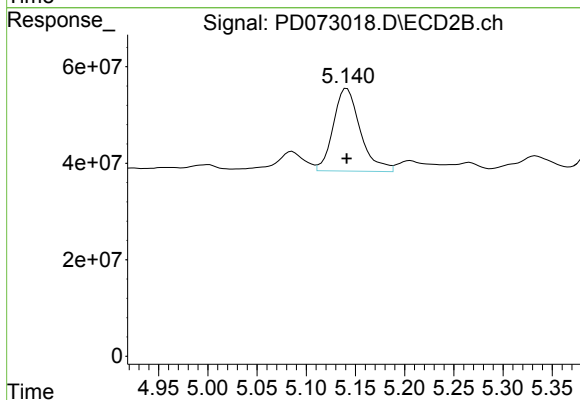


#24 Chlordane-2

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 328145389
Conc: 277.51 ng/ml

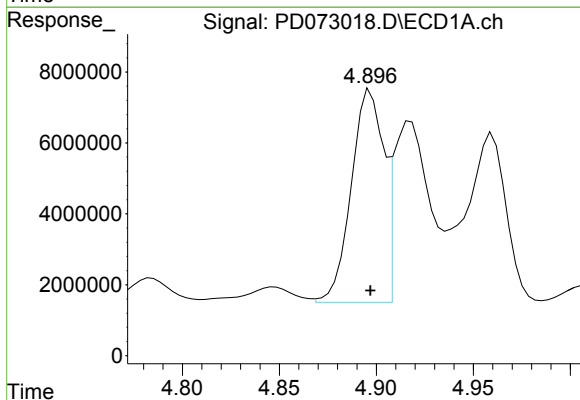


#25 Chlordane-3

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 69306877
Conc: 237.58 ng/ml

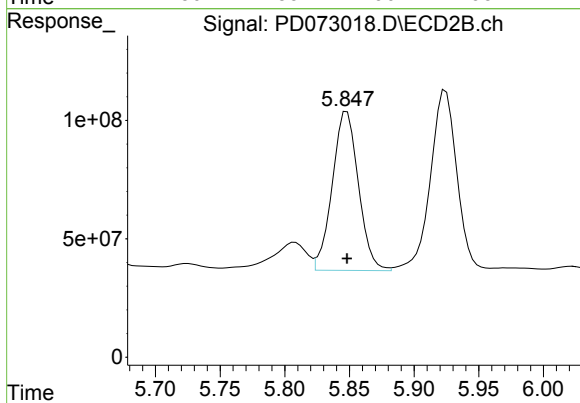

#25 Chlordane-3


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 943967828
Conc: 254.83 ng/ml

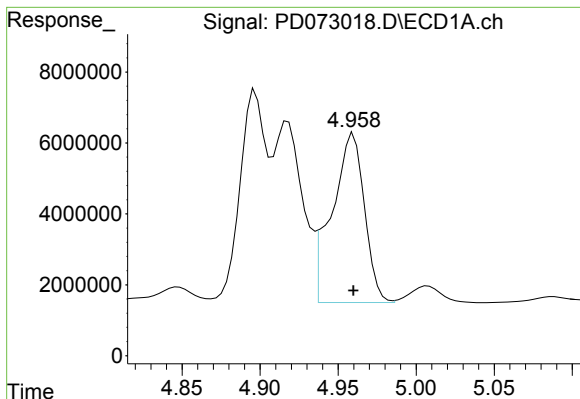

#26 Chlordane-4


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 69073019
Conc: 239.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

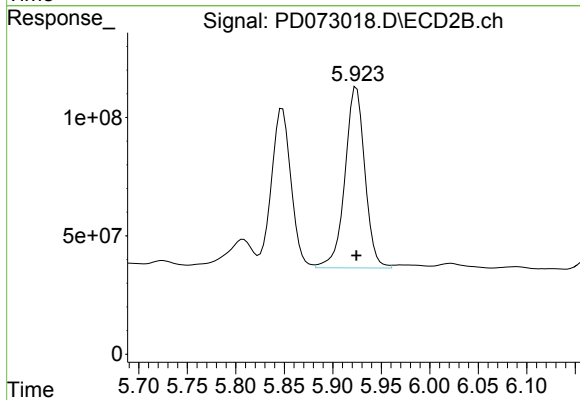


#26 Chlordane-4

R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 1092282272
Conc: 255.69 ng/ml

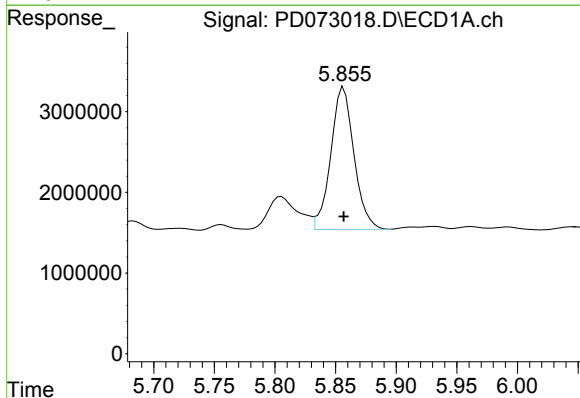


#27 Chlordane-5

R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 23523611
Conc: 246.68 ng/ml

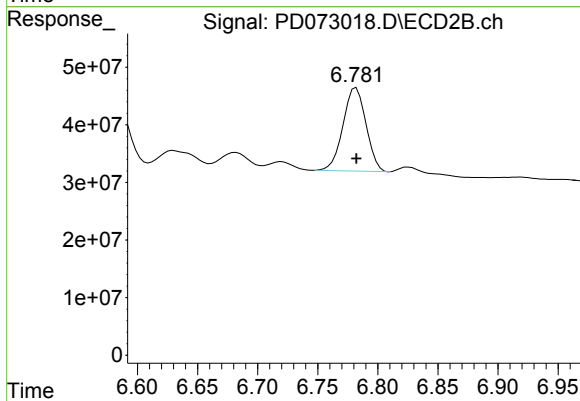

#27 Chlordane-5


R.T.: 6.782 min
Delta R.T.: 0.000 min
Response: 186242969
Conc: 255.60 ng/ml

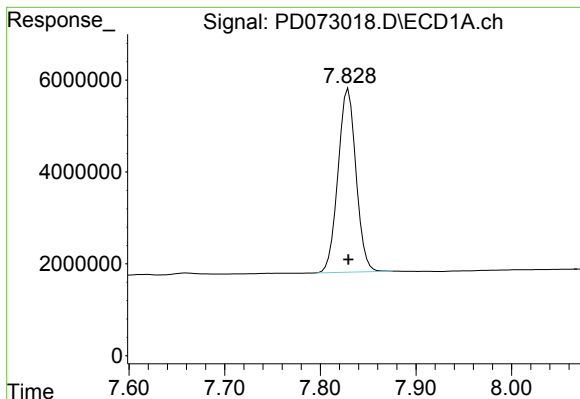

#28 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 52332935
Conc: 25.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

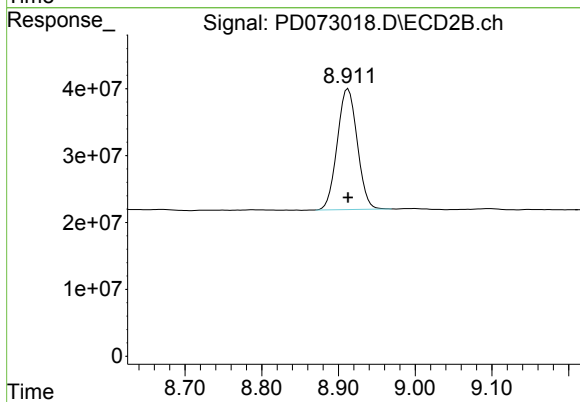

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.000 min
Response: 327953398
Conc: 26.09 ng/ml