

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
 Data File : PD073019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 18:10
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 02:16:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 02:16:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	12105466	318.2E6	5.047	5.673
28)	SA Decachlor...	7.830	8.914	12120401	74722616	5.784	5.728
Target Compounds							
23)	Chlordane-1	3.688	4.607	4790222	101.3E6	57.830m	64.867m
24)	Chlordane-2	4.265	5.139	5804699	70210534	58.632m	55.013m
25)	Chlordane-3	4.897	5.847	14562532	211.9E6	49.936	55.197m
26)	Chlordane-4	4.959	5.924	15063787	248.4E6	51.813	55.913m
27)	Chlordane-5	5.857	6.783	5080071	39476709	52.584	53.287



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
Data File : PD073019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 18:10
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 02:16:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 02:16:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

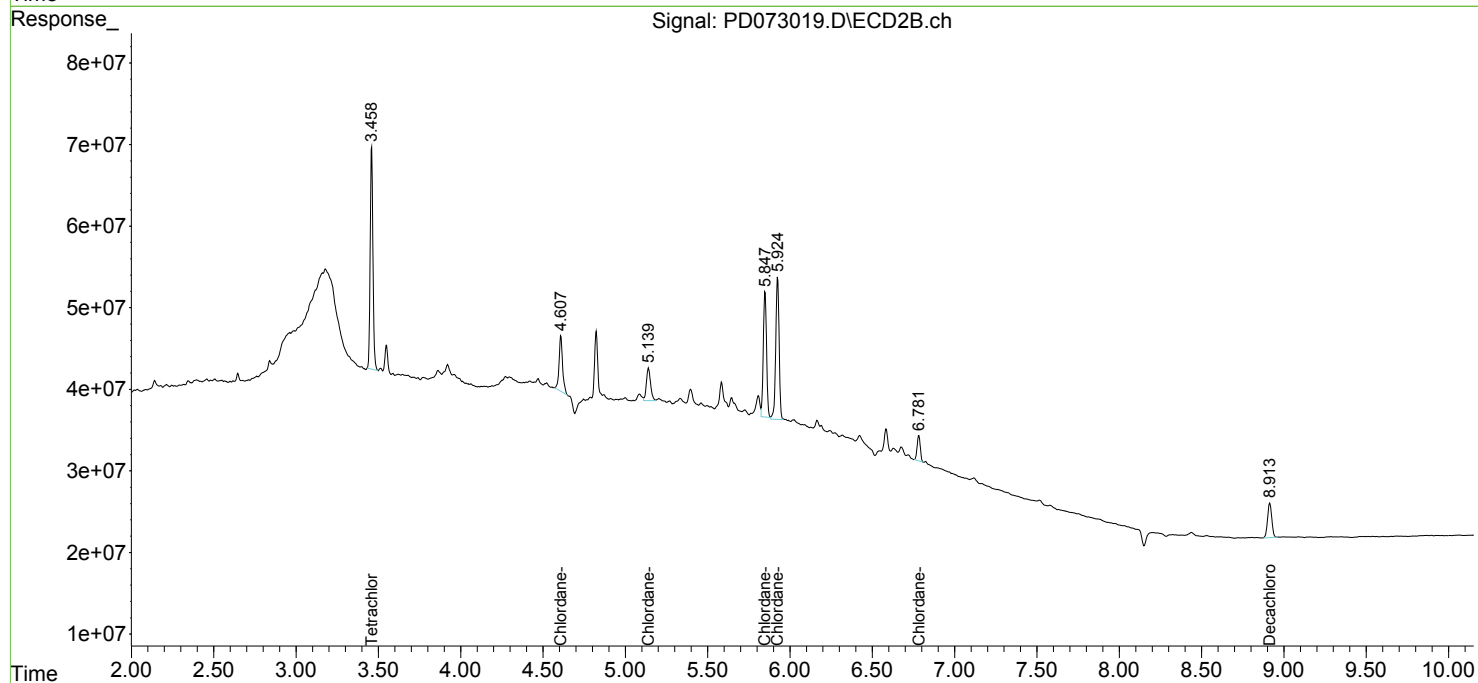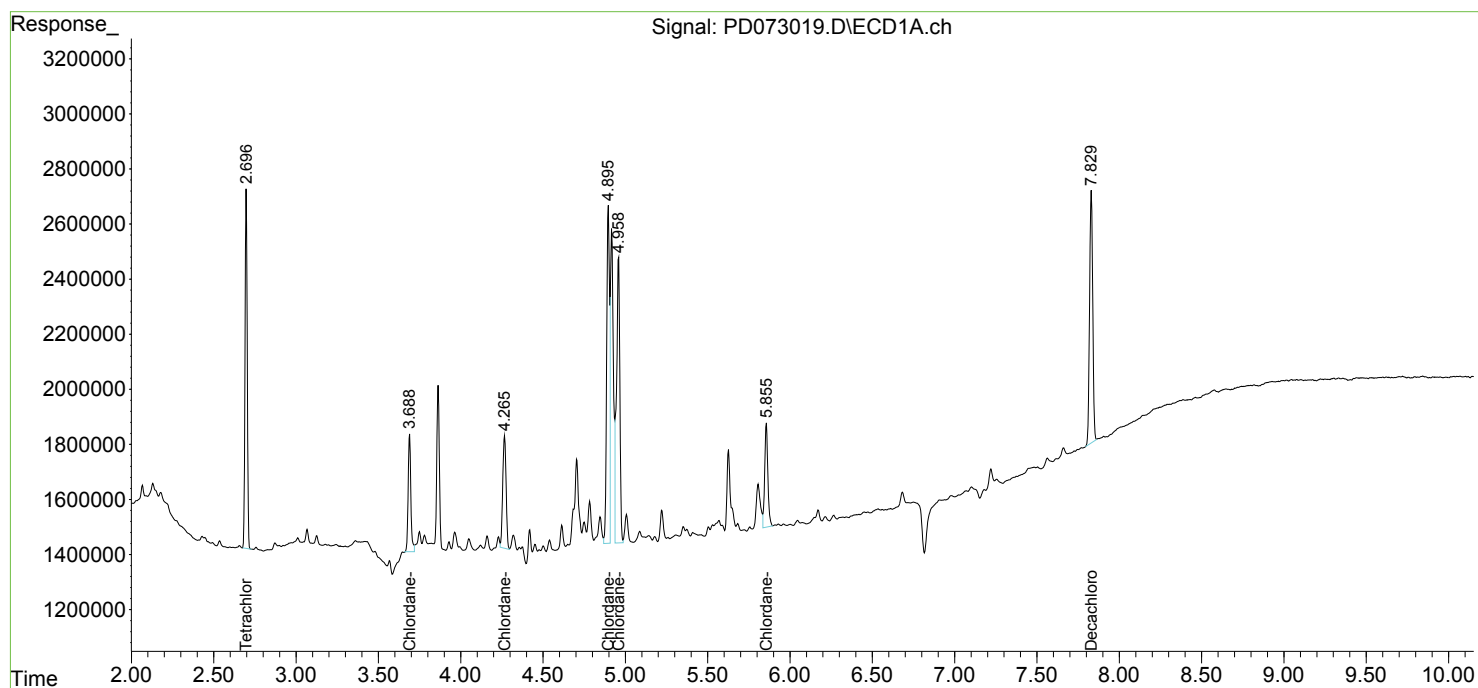


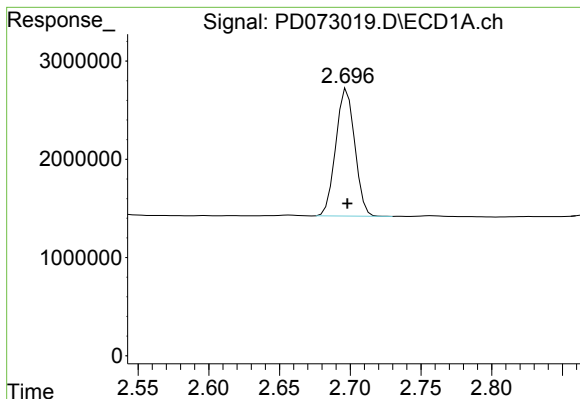

#1 Tetrachloro-m-xylene


R.T.: 2.698 min
Delta R.T.: 0.000 min
Response: 12105466
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

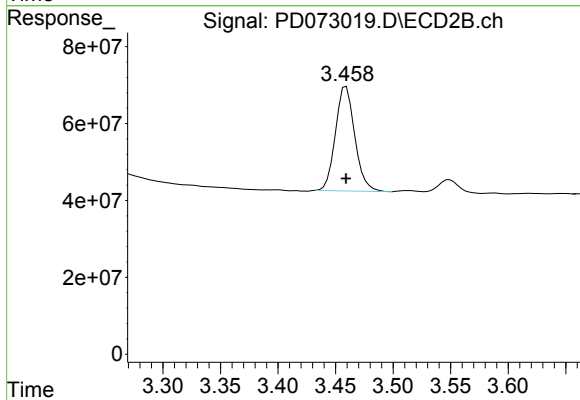


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 318173449
Conc: 5.67 ng/ml

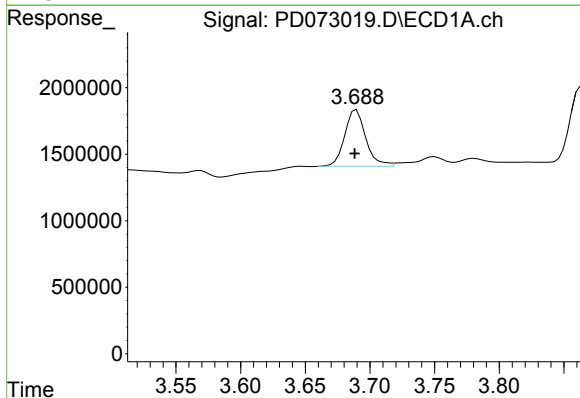


#23 Chlordane-1

R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 4790222
Conc: 57.83 ng/ml m

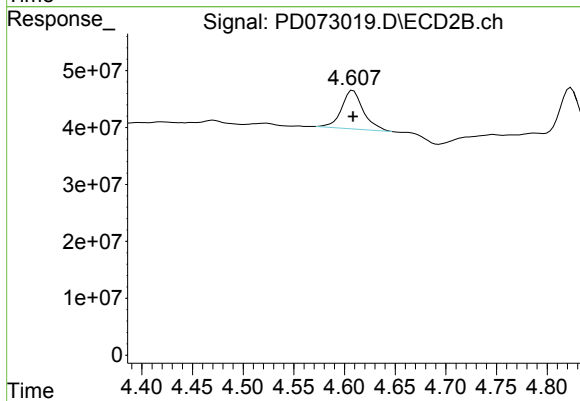

#23 Chlordane-1


R.T.: 4.607 min
Delta R.T.: -0.001 min
Response: 101338857
Conc: 64.87 ng/ml m

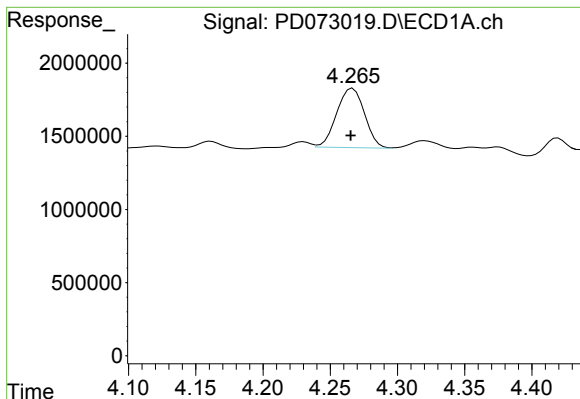

#24 Chlordane-2


R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 5804699
Conc: 58.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

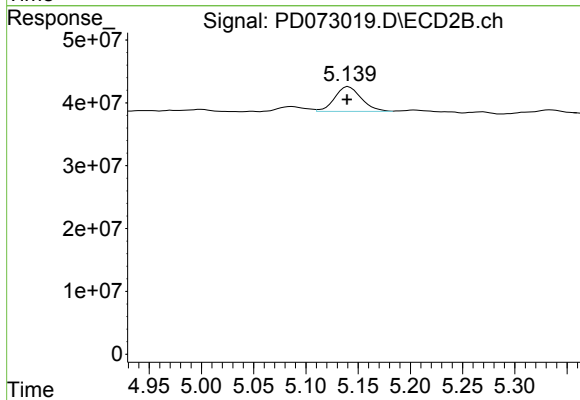


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 70210534
Conc: 55.01 ng/ml m

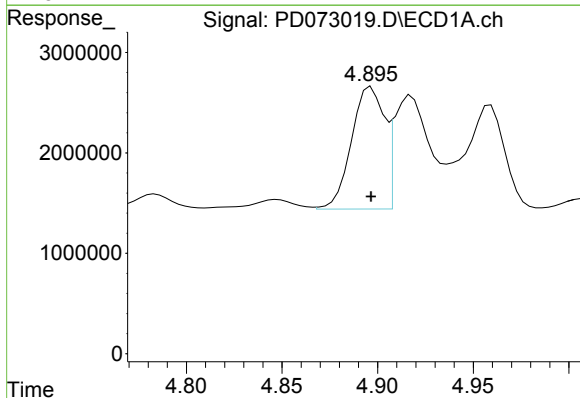


#25 Chlordane-3

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 14562532
Conc: 49.94 ng/ml

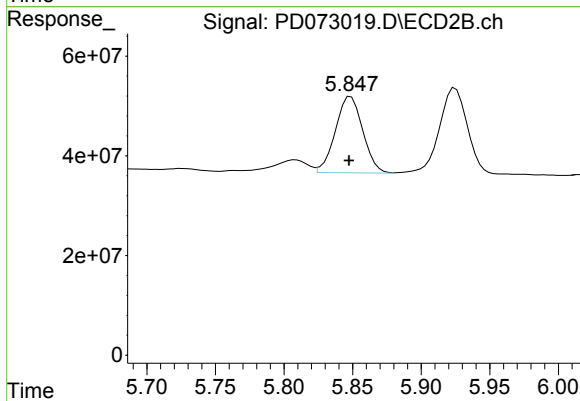

#25 Chlordane-3


R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 211883569
Conc: 55.20 ng/ml m

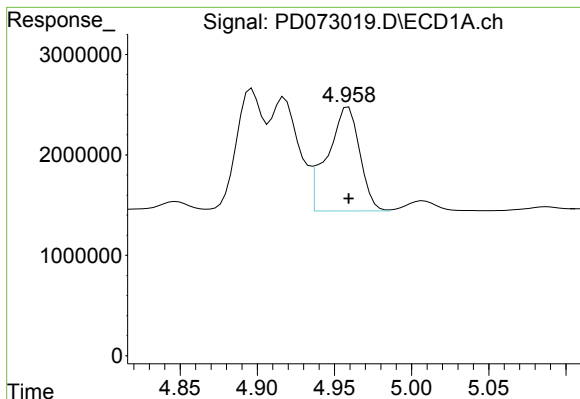

#26 Chlordane-4


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 15063787
Conc: 51.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

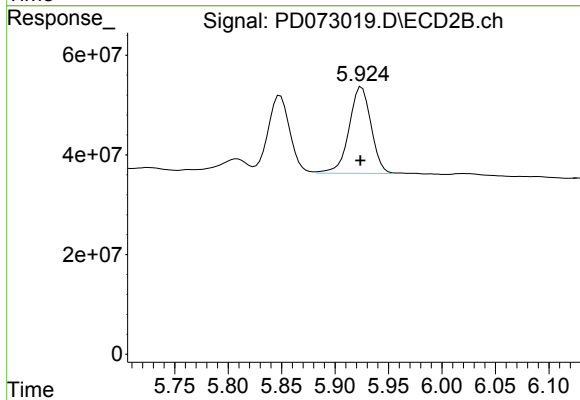


#26 Chlordane-4

R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 248365401
Conc: 55.91 ng/ml m

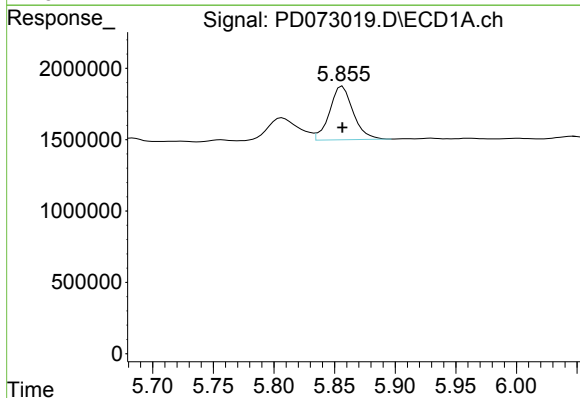


#27 Chlordane-5

R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 5080071
Conc: 52.58 ng/ml

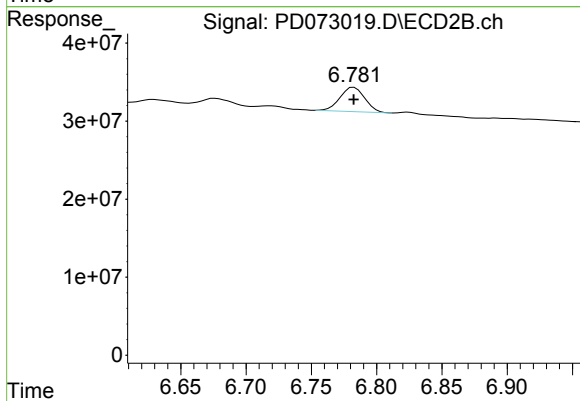

#27 Chlordane-5


R.T.: 6.783 min
Delta R.T.: 0.000 min
Response: 39476709
Conc: 53.29 ng/ml

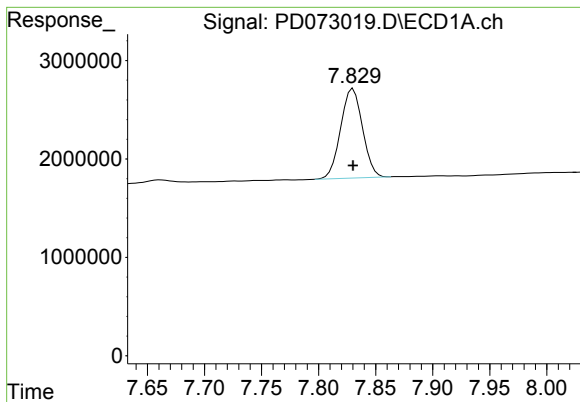

#28 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: 0.000 min
Response: 12120401
Conc: 5.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

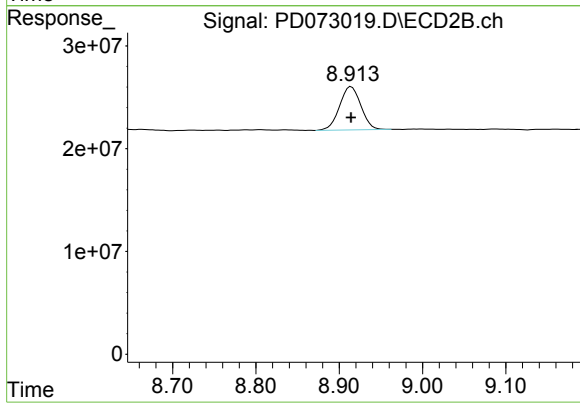

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 74722616
Conc: 5.73 ng/ml