

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
 Data File : PD073026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 19:43
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD111622CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 03:28:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 03:26:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	116.8E6	2635.0E6	55.048	47.562
28)	SA Decachlor...	7.828	8.913	99657885	635.7E6	48.383	49.737
Target Compounds							
23)	Chlordane-1	3.690	4.609	40155376	738.1E6	483.605	471.181
24)	Chlordane-2	4.267	5.139	47257694	520.3E6	482.091	424.107m
25)	Chlordane-3	4.897	5.848	142.9E6	1820.1E6	490.029	477.607
26)	Chlordane-4	4.960	5.925	142.9E6	2099.7E6	491.355	476.026
27)	Chlordane-5	5.857	6.782	41864498	372.7E6	433.343	503.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111622\
Data File : PD073026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 19:43
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD111622CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 03:28:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 03:26:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

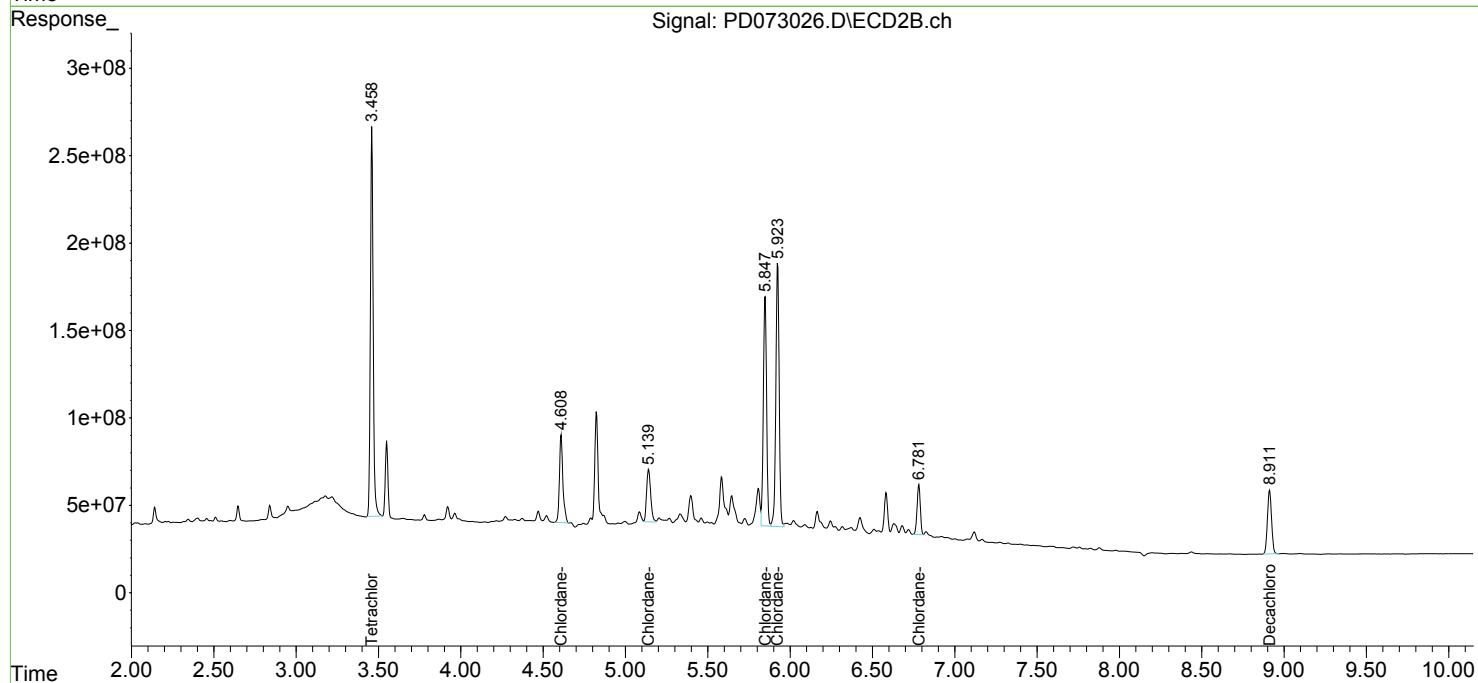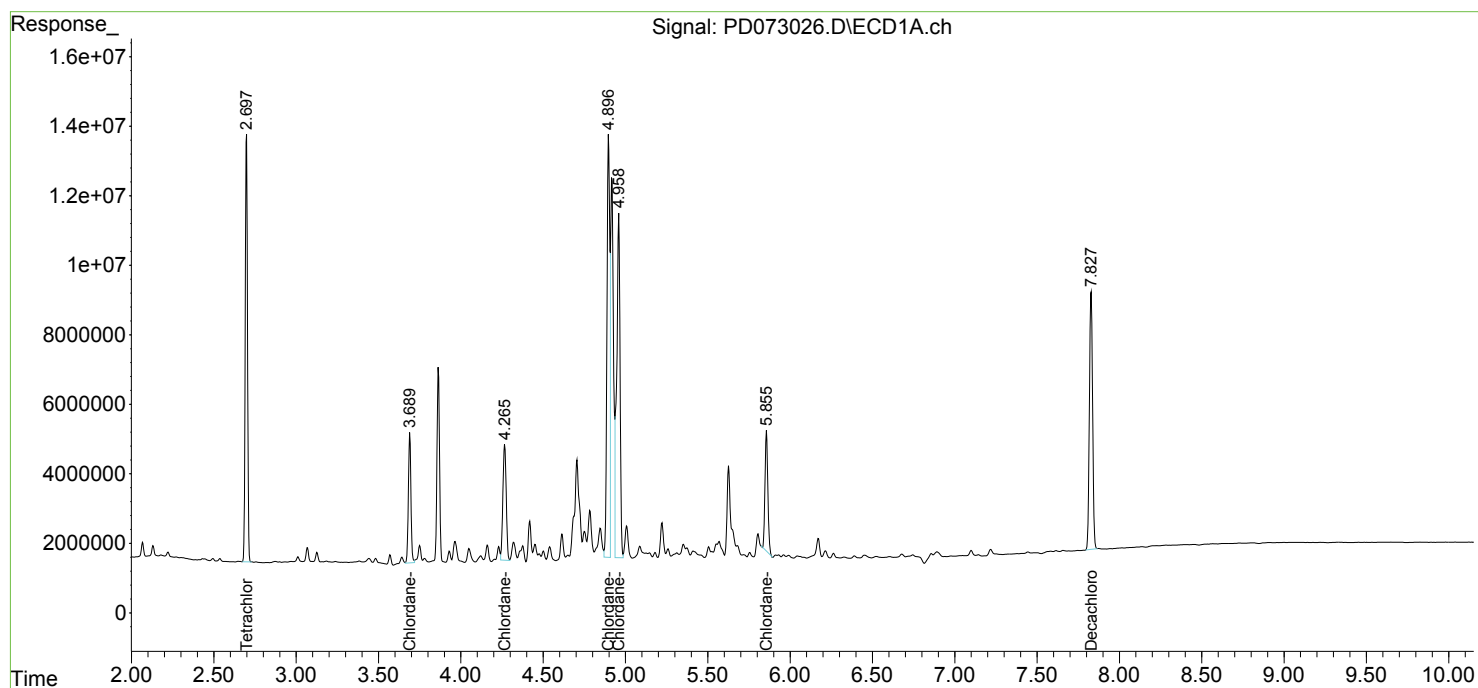


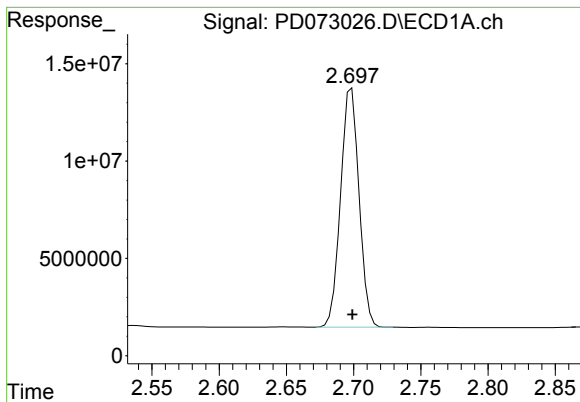

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 116815793
Conc: 55.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111622CHLOR

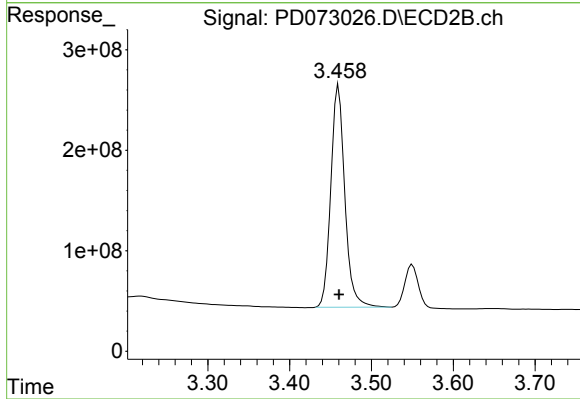


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 2634971391
Conc: 47.56 ng/ml

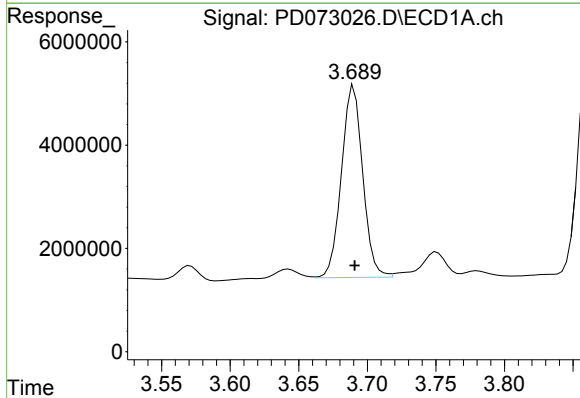


#23 Chlordane-1

R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 40155376
Conc: 483.61 ng/ml

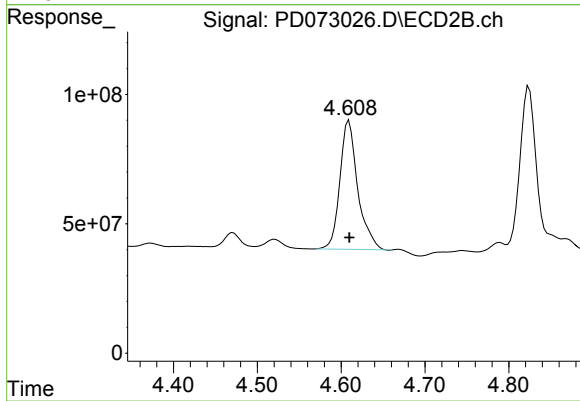

#23 Chlordane-1


R.T.: 4.609 min
Delta R.T.: 0.000 min
Response: 738111864
Conc: 471.18 ng/ml

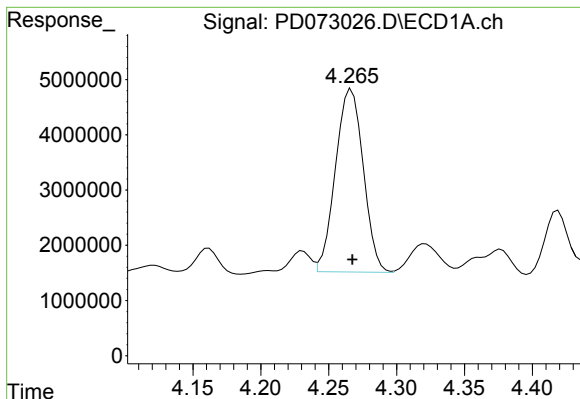

#24 Chlordane-2


R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 47257694
Conc: 482.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111622CHLOR

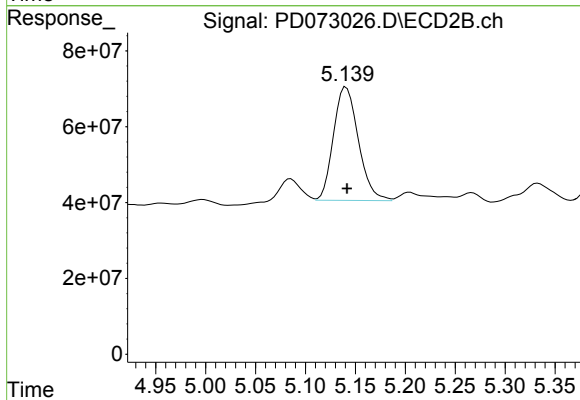


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: -0.002 min
Response: 520302714
Conc: 424.11 ng/ml m

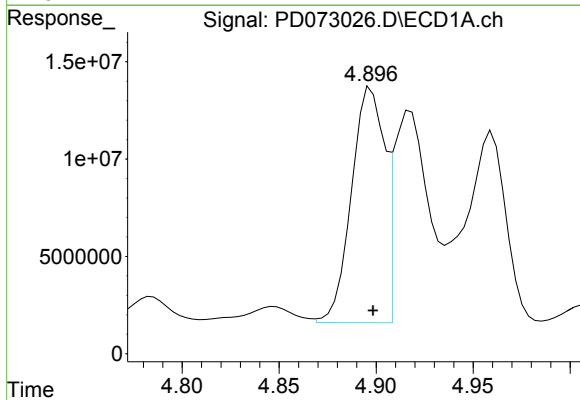


#25 Chlordane-3

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 142905668
Conc: 490.03 ng/ml

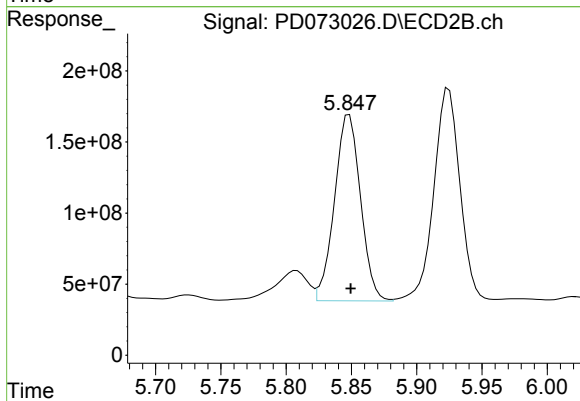

#25 Chlordane-3


R.T.: 5.848 min
Delta R.T.: -0.001 min
Response: 1820129529
Conc: 477.61 ng/ml

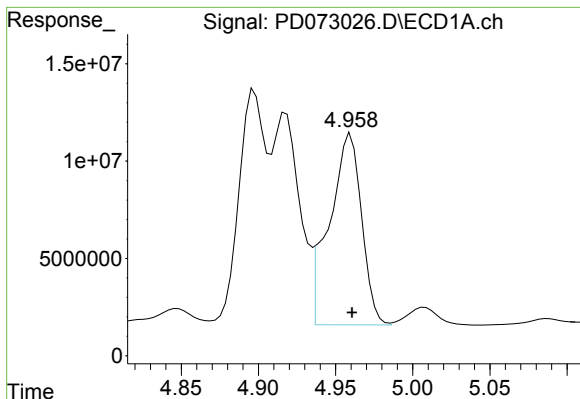

#26 Chlordane-4


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 142854058
Conc: 491.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111622CHLOR

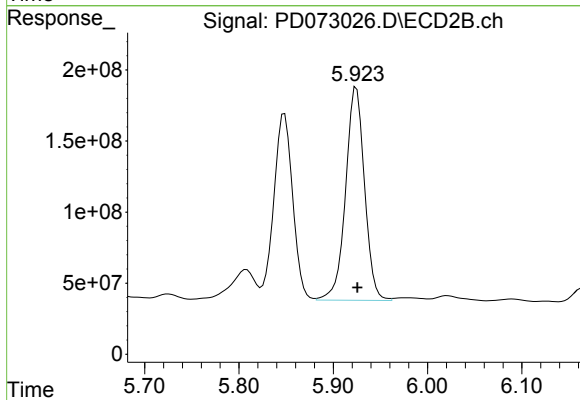


#26 Chlordane-4

R.T.: 5.925 min
Delta R.T.: -0.001 min
Response: 2099727145
Conc: 476.03 ng/ml

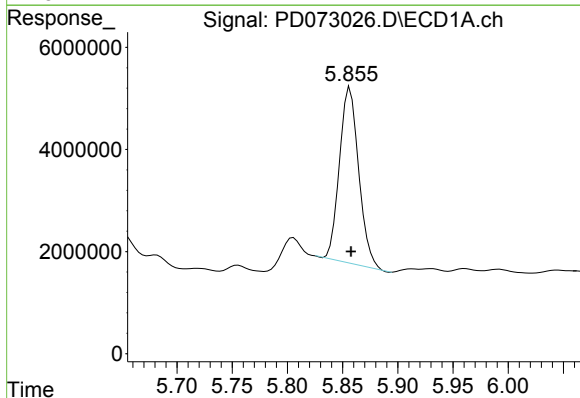


#27 Chlordane-5

R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 41864498
Conc: 433.34 ng/ml

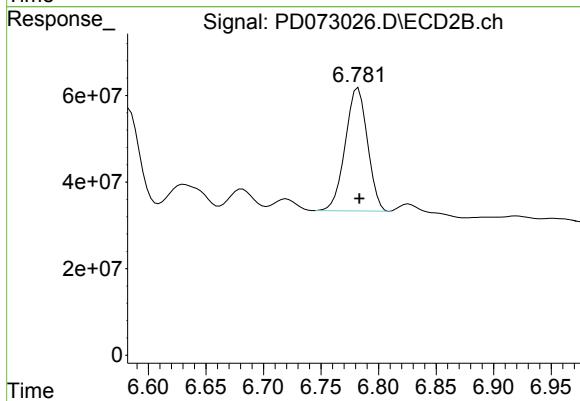

#27 Chlordane-5


R.T.: 6.782 min
Delta R.T.: 0.000 min
Response: 372669668
Conc: 503.04 ng/ml

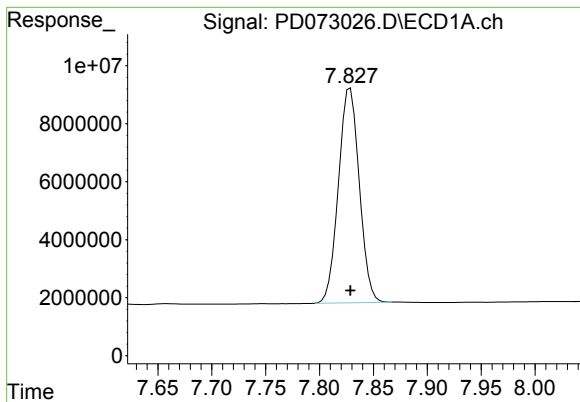

#28 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 99657885
Conc: 48.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD111622CHLOR

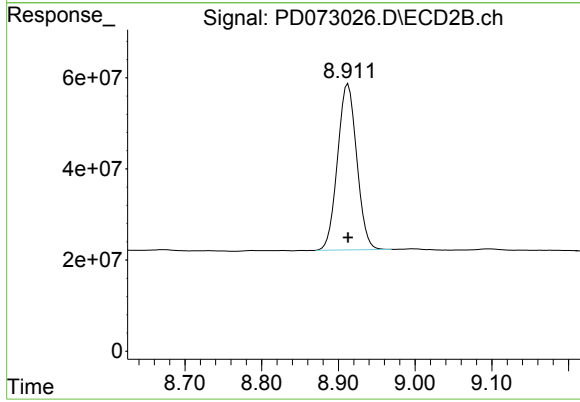

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 635707298
Conc: 49.74 ng/ml