

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
 Data File : PD086721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 18:49
 Operator : AR\AJ
 Sample : P4803-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AQ5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:32:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.887	38477570	163.1E6	25.622	15.682 #
2)	SA Decachlor...	9.089	8.090	42831468	181.2E6	19.356	15.276
Target Compounds							
6)	B beta-BHC	0.000	3.988f	0	213.3E6	N.D.	31.174
8)	B Heptachlo...	0.000	4.922f	0	32064.4E6	N.D.	2325.479
10)	B trans-Chl...	0.000	5.084f	0	6747.1E6	N.D.	466.013


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
Data File : PD086721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 18:49
Operator : AR\AJ
Sample : P4803-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

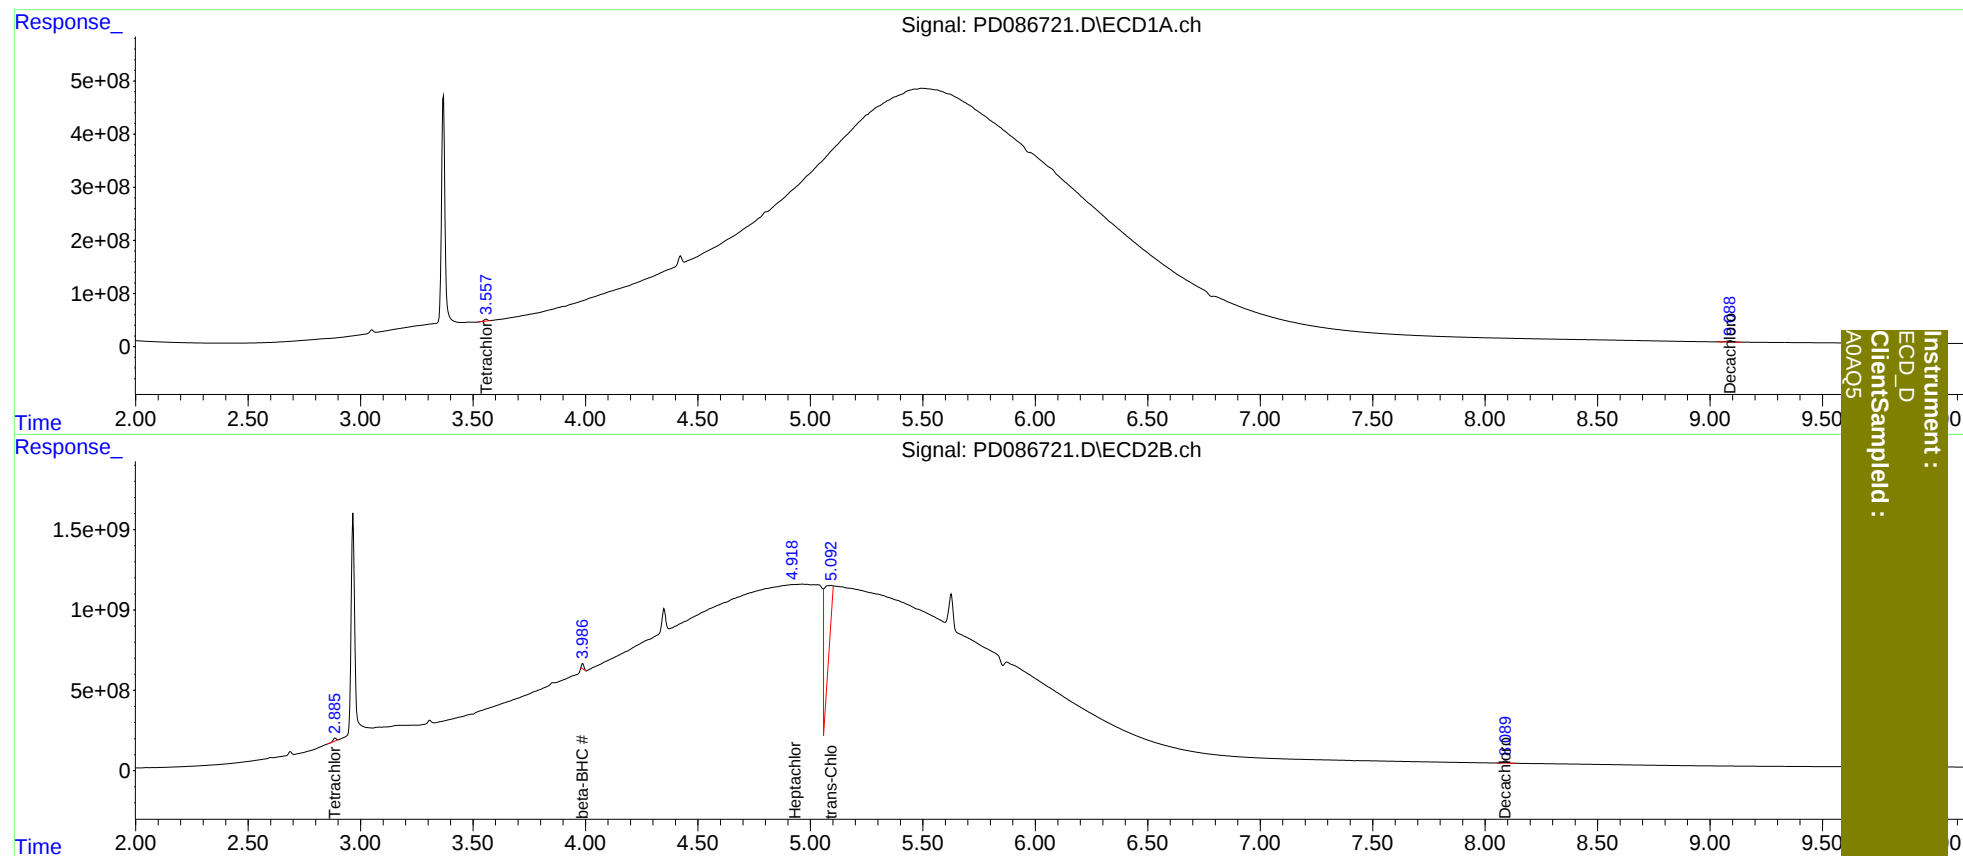


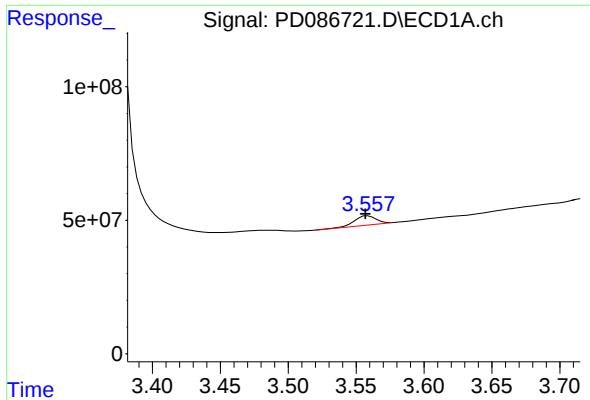

#1 Tetrachloro-m-xylene


R.T.: 3.559 min
Delta R.T.: 0.002 min
Response: 38477570
Conc: 25.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
A0AQ5

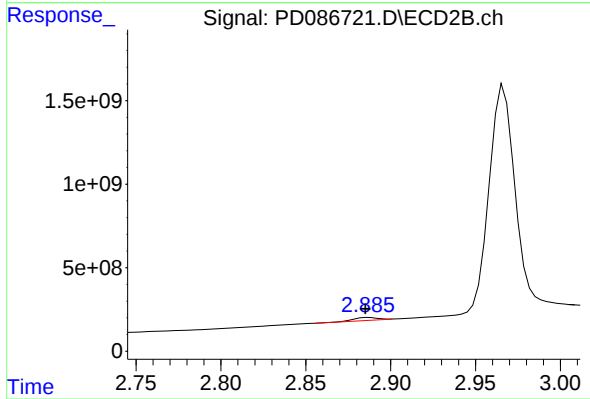


#1 Tetrachloro-m-xylene

R.T.: 2.887 min
Delta R.T.: 0.002 min
Response: 163055136
Conc: 15.68 ng/ml

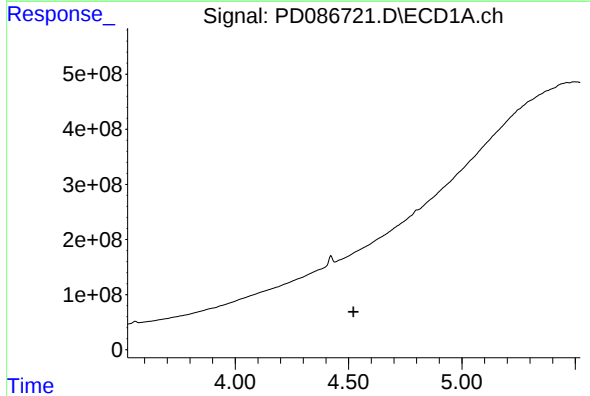


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.522 min
Response: 0
Conc: N.D.

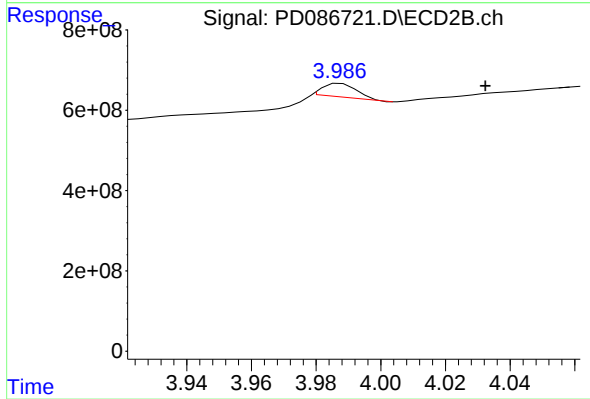

#6 beta-BHC


R.T.: 3.988 min
Delta R.T.: -0.045 min
Response: 213263717
Conc: 31.17 ng/ml

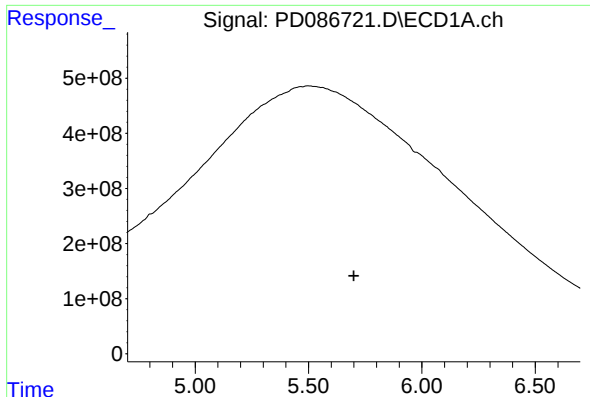

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
A0AQ5

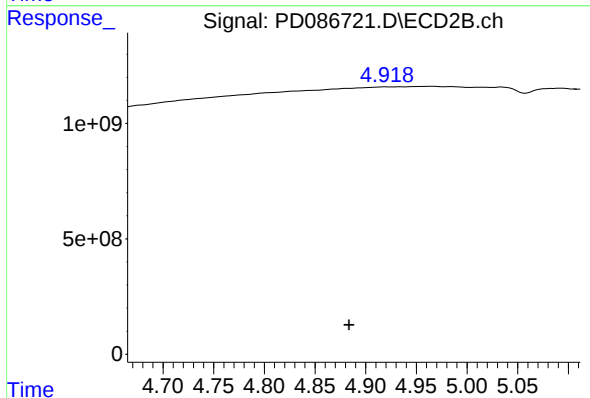


#8 Heptachlor epoxide

R.T.: 4.922 min
Delta R.T.: 0.039 min
Response: 32064447802
Conc: 2325.48 ng/ml

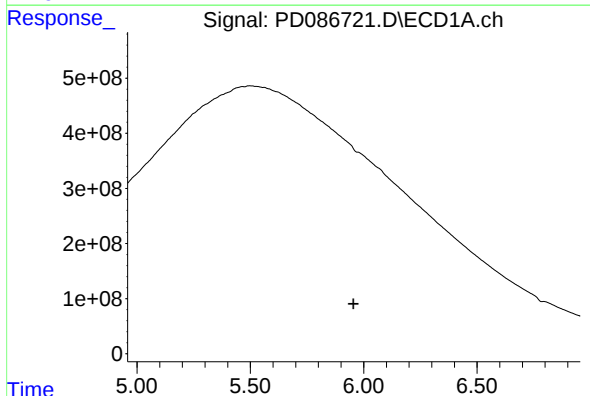


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.955 min
Response: 0
Conc: N.D.

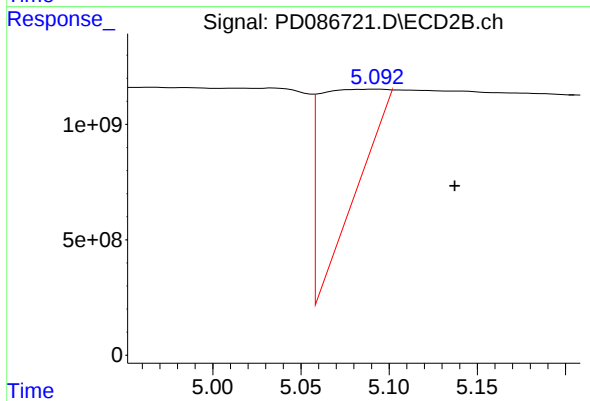

#10 trans-Chlordane

R.T.: 5.084 min
Delta R.T.: -0.054 min
Response: 6747148107
Conc: 466.01 ng/ml

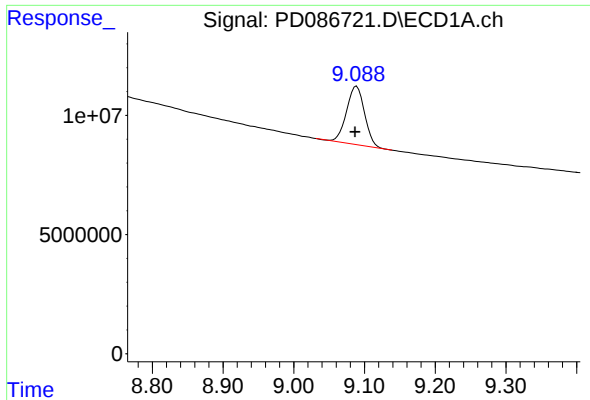

#27 Decachlorobiphenyl


R.T.: 9.089 min

Delta R.T.: 0.002 min

Response: 42831468

Conc: 19.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
A0AQ5

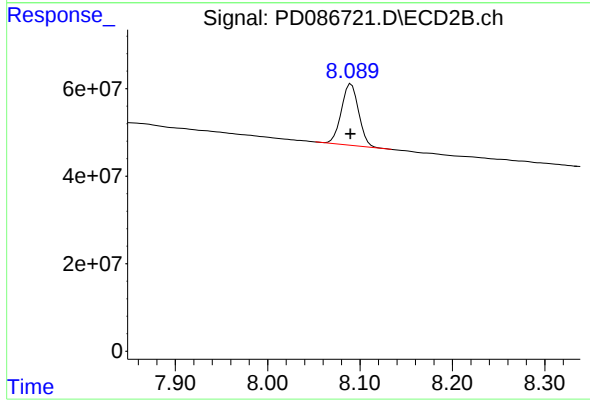

#27 Decachlorobiphenyl

R.T.: 8.090 min

Delta R.T.: 0.000 min

Response: 181223800

Conc: 15.28 ng/ml