

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
 Data File : PD086717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 17:53
 Operator : AR\AJ
 Sample : P4803-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AQ2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:30:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.884	34705548	234.7E6	23.110m	22.571
27)	SA Decachlor...	9.089	8.090	49662450	261.6E6	22.443	22.049
Target Compounds							
2)	A alpha-BHC	4.007	3.397	4982.4E6	11658.8E6	1733.245	718.918 #
3)	MA gamma-BHC...	4.339	3.736	1540.6E6	5411.2E6	543.751	356.578 #
4)	MA Heptachlor	4.939	4.093	1808.7E6	5956.0E6	628.937	379.484 #
5)	MB Aldrin	5.282	4.382	4866.5E6	9974.4E6	1808.564	677.173 #
6)	B beta-BHC	4.522	4.032	1322.0E6	5140.4E6	1065.751	751.406 #
7)	B delta-BHC	4.771	4.269	1947.7E6	6560.9E6	689.065	430.220 #
8)	B Heptachlo...	5.701	4.884	2072.0E6	6800.4E6	817.101	493.201 #
9)	A Endosulfan I	6.083	5.258	4803.2E6	13821.1E6	1985.351m	1049.848m#
10)	B trans-Chl...	5.956	5.138	1442.1E6	5493.2E6	581.382	379.405 #
11)	B cis-Chlor...	6.036	5.200	2337.3E6	8178.4E6	931.044m	578.745m#
12)	B 4,4'-DDE	6.206	5.388	2641.0E6	9054.5E6	1104.231	680.327 #
13)	MA Dieldrin	6.358	5.525	4397.7E6	13058.9E6	1640.333	932.690 #
14)	MA Endrin	6.585	5.801	3737.4E6	11299.5E6	1667.427	880.381 #
15)	B Endosulfa...	6.796	6.092	2060.6E6	7259.5E6	863.284	591.136 #
16)	A 4,4'-DDD	6.715	5.942	1406.8E6	5349.2E6	723.464	476.708 #
17)	MA 4,4'-DDT	7.031	6.196	938.7E6	3868.9E6	462.145	324.241 #
18)	B Endrin al...	6.925	6.270	2709.6E6	8639.8E6	1554.262	910.278 #
19)	B Endosulfa...	7.159	6.494	1441.9E6	5398.8E6	677.968	456.572 #
20)	A Methoxychlor	7.504	6.768	398.5E6	1741.7E6	350.552	317.065
21)	B Endrin ke...	7.640	7.003	4645.6E6	13407.8E6	1906.910	1020.527 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
Data File : PD086717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 17:53
Operator : AR\AJ
Sample : P4803-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:30:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

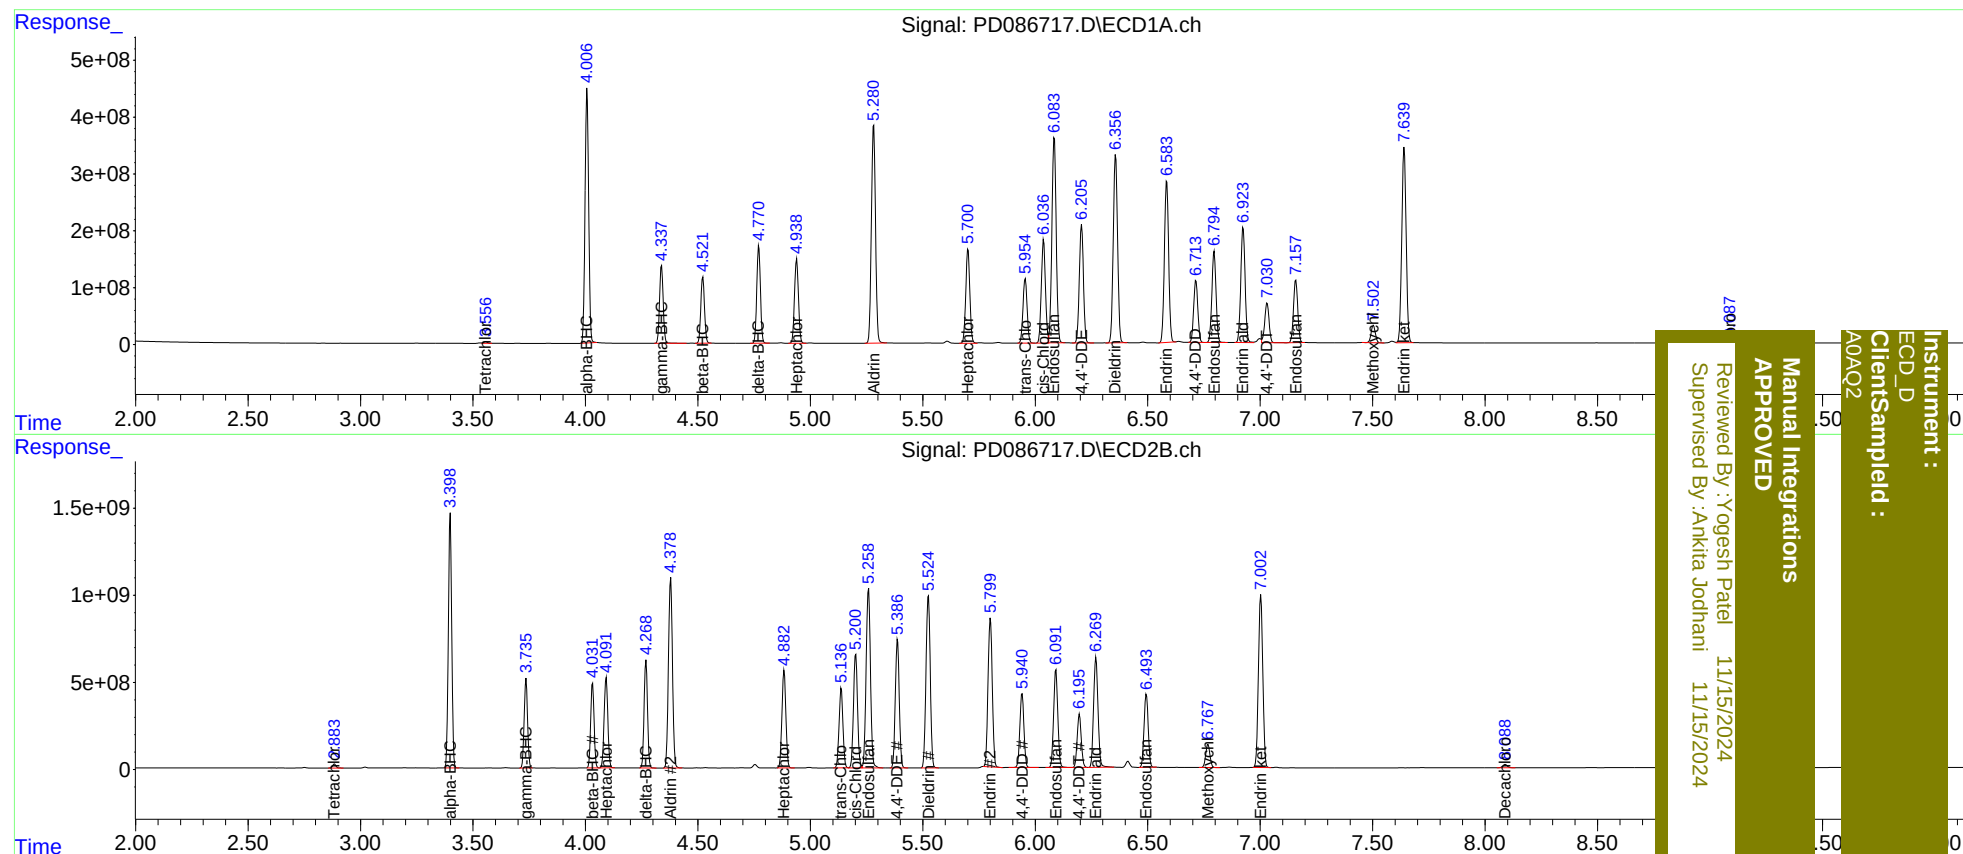

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/15/2024
Supervised By : Ankita Jodhani 11/15/2024

Instrument :
ECD_D
ClientSampled :
A0A02