

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
 Data File : PD086736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 22:19
 Operator : AR\AJ
 Sample : P4829-03MS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29S4MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:37:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.886	32386397	222.2E6	21.566m	21.373
27)	SA Decachlor...	9.091	8.091	43680002	222.2E6	19.739	18.733
Target Compounds							
2)	A alpha-BHC	4.008	3.400	170.7E6	836.4E6	59.390	51.577
3)	MA gamma-BHC...	4.340	3.737	170.0E6	787.2E6	60.003	51.873
4)	MA Heptachlor	4.940	4.093	156.4E6	685.0E6	54.393	43.648
5)	MB Aldrin	5.282	4.380	148.9E6	704.2E6	55.331	47.808
6)	B beta-BHC	4.523	4.032	65094027	328.3E6	52.476	47.989
7)	B delta-BHC	4.772	4.270	111.6E6	539.1E6	39.470	35.348
8)	B Heptachlo...	5.702	4.884	147.6E6	704.4E6	58.225	51.087
9)	A Endosulfan I	6.085	5.257	137.9E6	661.7E6	57.012m	50.264m
10)	B trans-Chl...	5.957	5.138	139.7E6	708.1E6	56.307	48.911
11)	B cis-Chlor...	6.037	5.201	146.2E6	702.6E6	58.220m	49.716m
12)	B 4,4'-DDE	6.207	5.388	284.2E6	1338.9E6	118.806	100.599
13)	MA Dieldrin	6.359	5.525	316.8E6	1385.9E6	118.177	98.982
14)	MA Endrin	6.586	5.802	263.0E6	1260.7E6	117.327	98.227
15)	B Endosulfa...	6.797	6.093	259.3E6	1205.4E6	108.649	98.158
16)	A 4,4'-DDD	6.716	5.943	230.0E6	1122.1E6	118.301	100.002
17)	MA 4,4'-DDT	7.032	6.198	232.4E6	1110.1E6	114.438m	93.036
18)	B Endrin al...	6.926	6.272	192.8E6	893.2E6	110.593	94.104
19)	B Endosulfa...	7.160	6.496	232.8E6	1110.3E6	109.480	93.897
20)	A Methoxychlor	7.505	6.770	600.3E6	2300.4E6	528.015	418.772
21)	B Endrin ke...	7.642	7.005	283.1E6	1289.3E6	116.216	98.137

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
Data File : PD086736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 22:19
Operator : AR\AJ
Sample : P4829-03MS
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:37:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

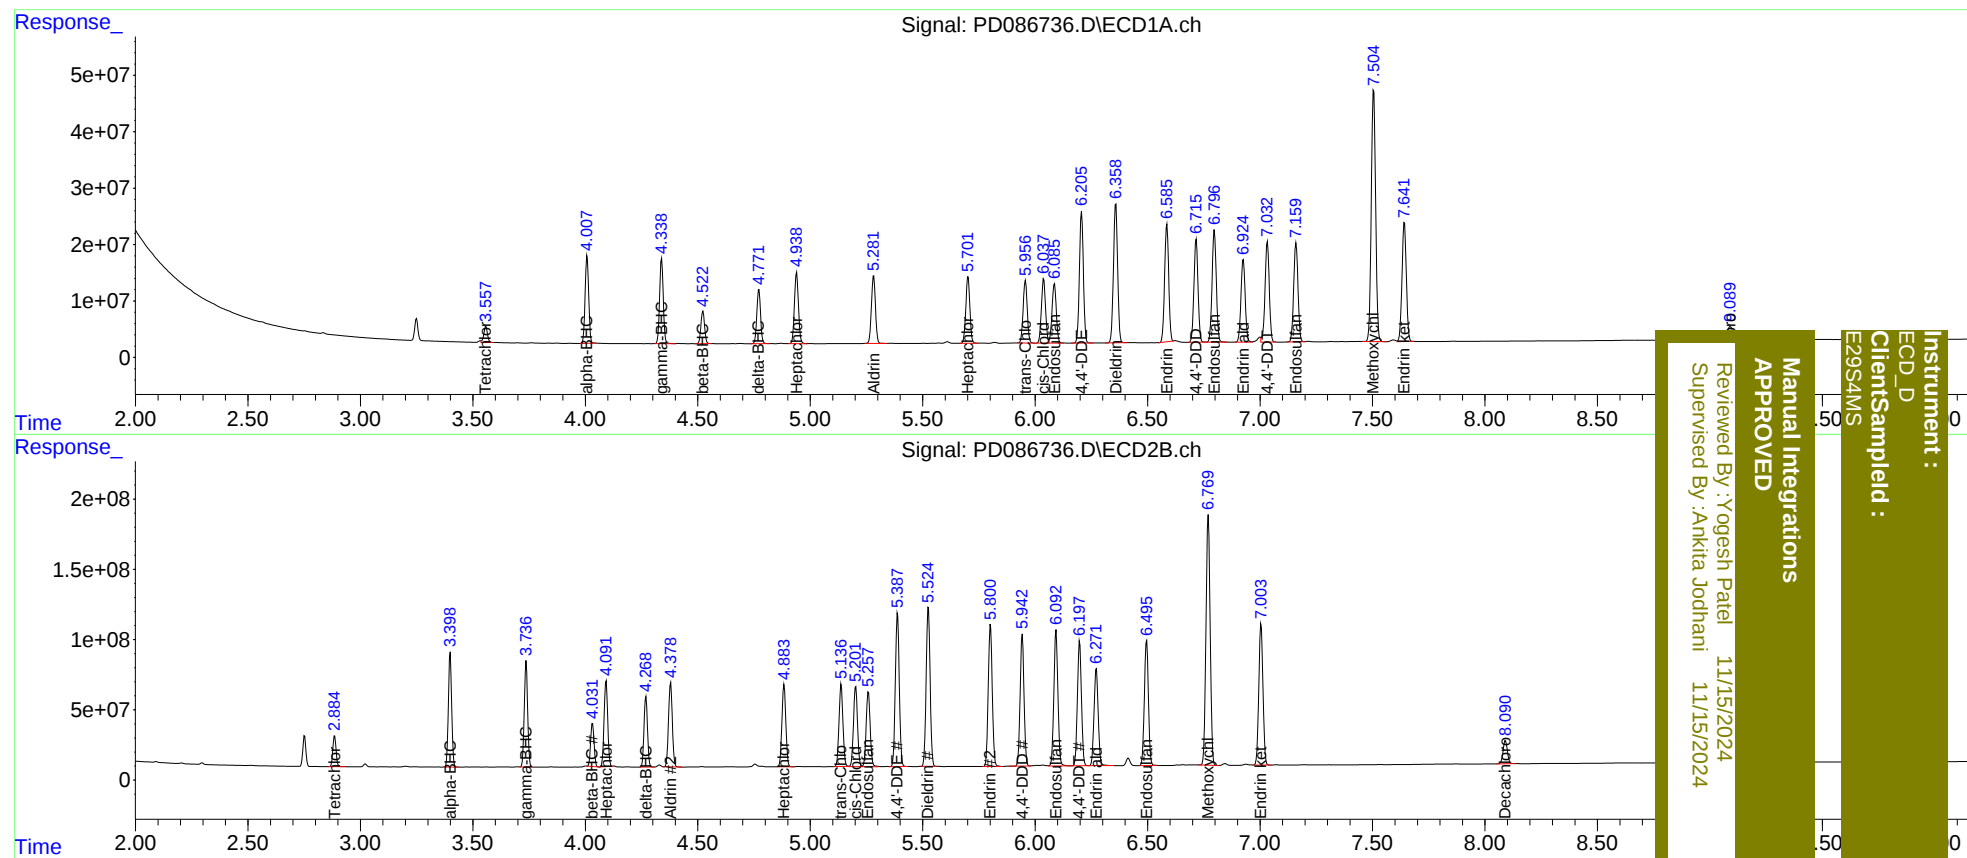

Instrument :
ECD_D
ClientSampled :
EZ9S4MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/15/2024
Supervised By : Ankita Jodhani 11/15/2024