

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
 Data File : PD086737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 22:33
 Operator : AR\AJ
 Sample : P4829-04MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29S4MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:37:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 03:38:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	32340162	220.6E6	21.535m	21.217
27)	SA Decachlor...	9.090	8.090	43305549	220.0E6	19.570	18.543
Target Compounds							
2)	A alpha-BHC	4.008	3.400	169.0E6	829.0E6	58.786	51.121
3)	MA gamma-BHC...	4.339	3.737	168.5E6	778.9E6	59.484	51.325
4)	MA Heptachlor	4.940	4.092	155.0E6	679.4E6	53.911	43.286
5)	MB Aldrin	5.282	4.379	147.7E6	697.7E6	54.902	47.367
6)	B beta-BHC	4.523	4.032	64564251	325.2E6	52.049	47.543
7)	B delta-BHC	4.771	4.269	110.8E6	533.2E6	39.201	34.961
8)	B Heptachlo...	5.701	4.884	146.3E6	699.7E6	57.704	50.744
9)	A Endosulfan I	6.084	5.258	136.3E6	660.7E6	56.320m	50.190m
10)	B trans-Chl...	5.956	5.138	138.5E6	700.7E6	55.841	48.395
11)	B cis-Chlor...	6.036	5.201	145.6E6	694.4E6	57.997m	49.140m
12)	B 4,4'-DDE	6.206	5.388	280.7E6	1325.5E6	117.383	99.598
13)	MA Dieldrin	6.358	5.525	313.6E6	1370.1E6	116.975	97.857
14)	MA Endrin	6.585	5.802	260.4E6	1249.7E6	116.173	97.370
15)	B Endosulfa...	6.796	6.093	255.6E6	1193.6E6	107.100	97.198
16)	A 4,4'-DDD	6.716	5.942	227.9E6	1112.8E6	117.193	99.174
17)	MA 4,4'-DDT	7.031	6.197	229.9E6	1100.0E6	113.214m	92.189
18)	B Endrin al...	6.925	6.271	190.8E6	883.3E6	109.468	93.061
19)	B Endosulfa...	7.160	6.495	231.0E6	1099.8E6	108.611	93.005
20)	A Methoxychlor	7.505	6.769	594.8E6	2281.5E6	523.192	415.340
21)	B Endrin ke...	7.641	7.004	280.8E6	1278.2E6	115.248	97.293

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111624\
Data File : PD086737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 22:33
Operator : AR\AJ
Sample : P4829-04MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:37:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 03:38:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

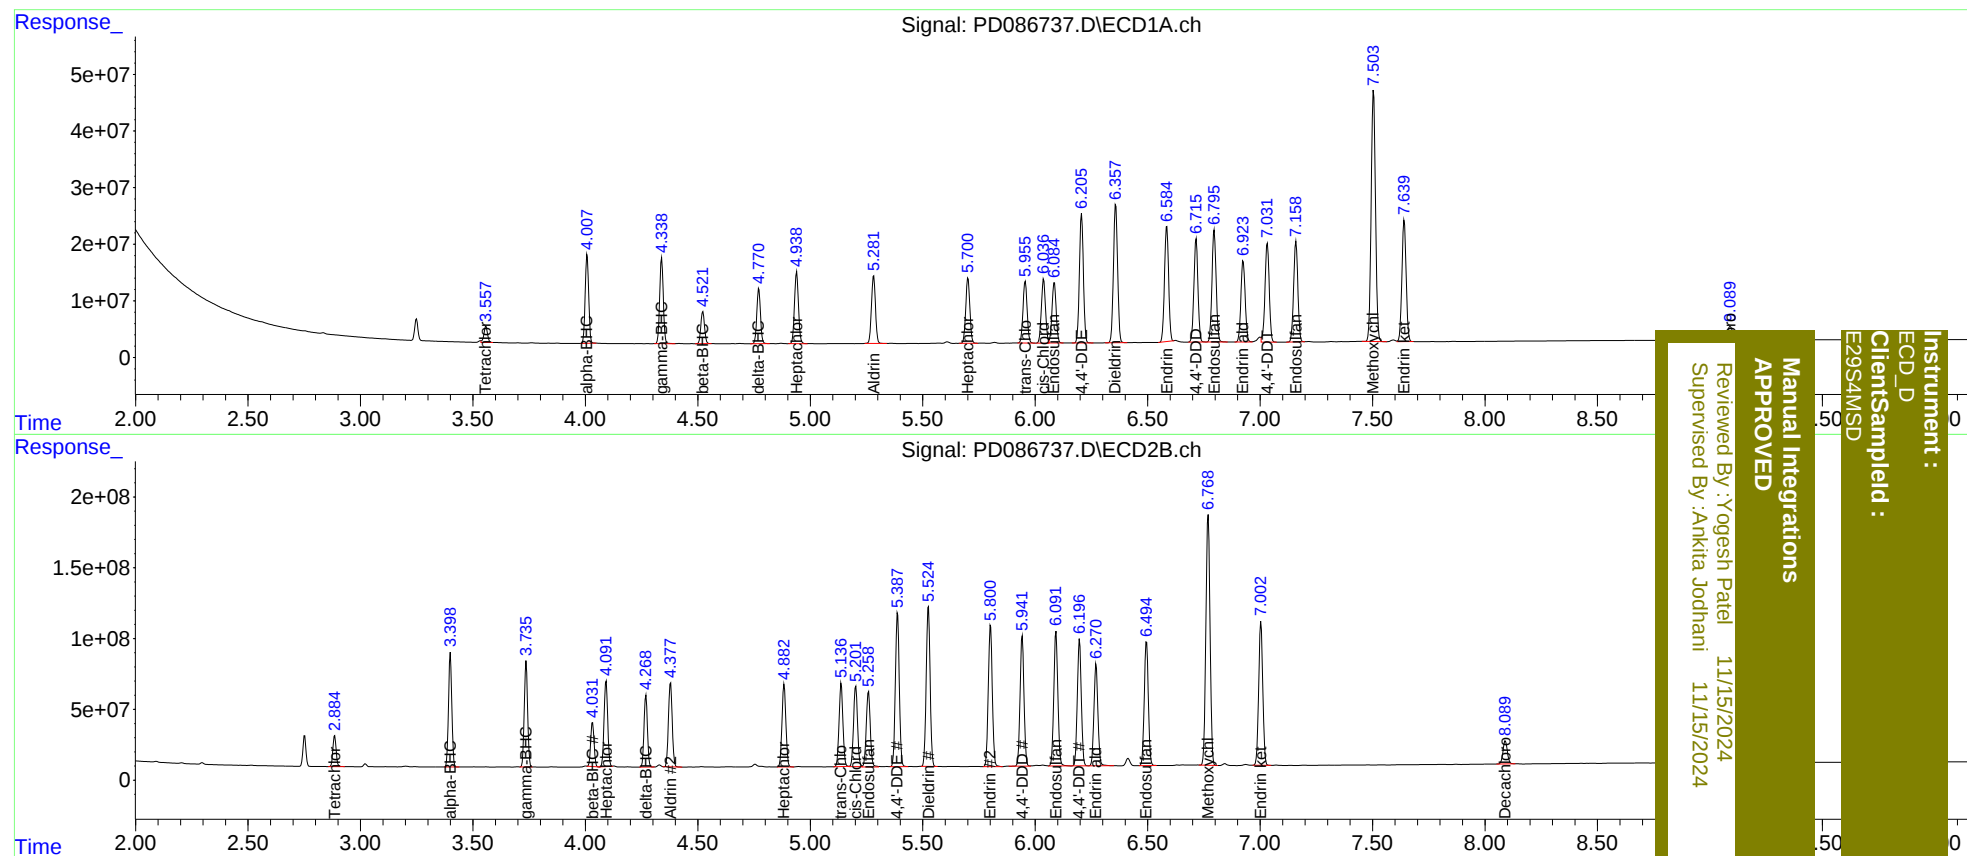

Instrument :
ECD_D
ClientSampled :
EZ9S4MSD

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/15/2024
Supervised By : Ankita Jodhani 11/15/2024