

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
 Data File : PD066986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 11:54
 Operator : AR\AJ
 Sample : PB140819BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS819

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/18/2021
 Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:18:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.967	34432859	169.2E6	17.812	19.542
27)	SA Decachlor...	8.163	9.025	37342218	199.5E6	31.871	38.249
Target Compounds							
2)	A alpha-BHC	3.874	4.360	11562463	50961611	3.950	4.661
3)	MA gamma-BHC...	4.156	4.645	11778411	49126750	4.254	4.861
4)	MA Heptachlor	4.449	5.145	12273902	47976770	4.314	4.895
5)	MB Aldrin	4.694	5.448	12269143	44215859	4.261	4.693
6)	B beta-BHC	4.404	4.823	5997155	25514389	4.775	5.178
7)	B delta-BHC	4.606	5.038	4141739	24710096	1.563	2.498 #
8)	B Heptachlo...	5.135	5.837	11722085	29561878	4.612	3.932
9)	A Endosulfan I	5.471	6.194	10703761	40357770	4.670	5.158
10)	B trans-Chl...	5.359	6.072	11765996	41595030	4.552	4.830
11)	B cis-Chlor...	5.416	6.143	11742022	42872563	4.609	4.996
12)	B 4,4'-DDE	5.581	6.303	21153126	79784632	9.261	10.477
13)	MA Dieldrin	5.713	6.453	21962905	81569820	8.801	10.225
14)	MA Endrin	5.970	6.671	18587892	62601622	8.786	9.225
15)	B Endosulfa...	6.242	6.886	18849070	71672102	9.078	9.995
16)	A 4,4'-DDD	6.095	6.798	16508316	66490715	9.120	10.299
17)	MA 4,4'-DDT	6.334	7.096	16071932	63675715	8.500	9.639
18)	B Endrin al...	6.410	7.011	16377720	62706840	11.242m	11.786
19)	B Endosulfa...	6.623	7.234	14710719	58759661	8.065	8.526
20)	A Methoxychlor	6.881	7.558	44396069	160.8E6	47.370	49.750
21)	B Endrin ke...	7.115	7.707	19541620	75399198	9.484	9.619

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
Data File : PD066986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 11:54
Operator : AR\AJ
Sample : PB140819BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:18:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

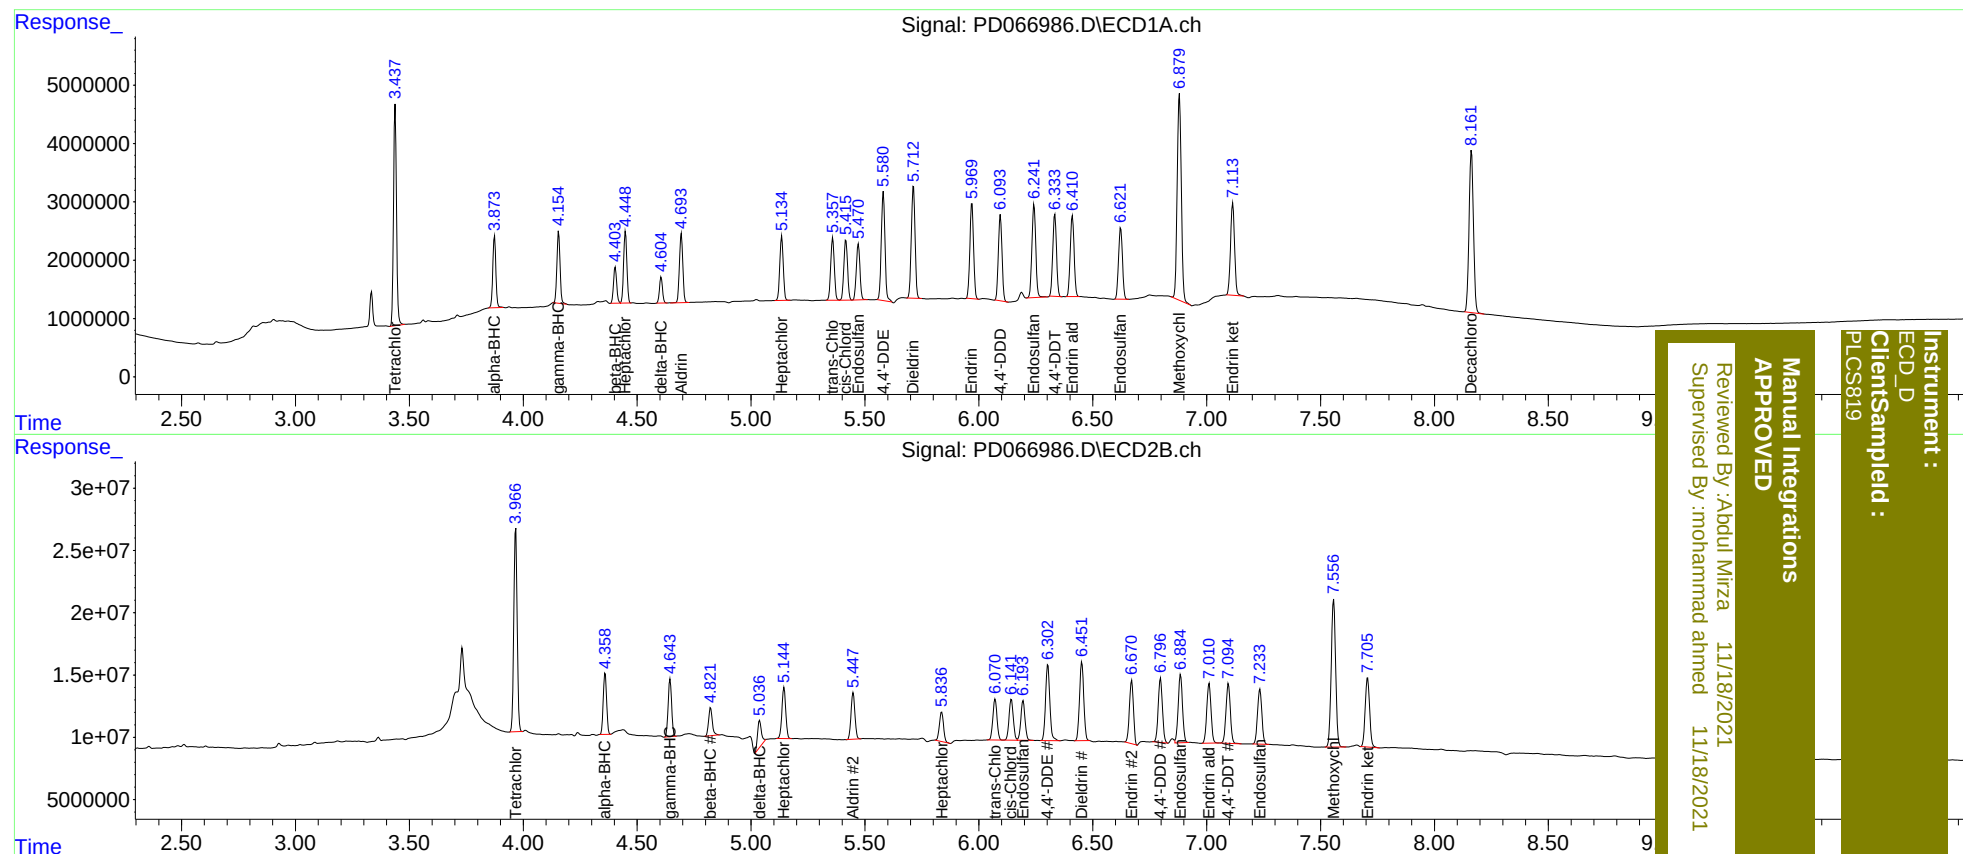

Instrument :
ECD_D
ClientSampled :
PLCS819

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/18/2021
Supervised By: mohammad ahmed 11/18/2021