

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
 Data File : PD066992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 14:45
 Operator : AR\AJ
 Sample : M4677-07MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0AB5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2021
 Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:19:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.967	36381007	211.7E6	18.820	24.439 #
27)	SA Decachlor...	8.163	9.025	31670696	186.3E6	27.030	35.718 #
Target Compounds							
2)	A alpha-BHC	3.875	4.358	129.1E6	470.7E6	44.111	43.053m
3)	MA gamma-BHC...	4.156	4.645	128.5E6	431.9E6	46.422	42.742
4)	MA Heptachlor	4.450	5.145	135.9E6	423.3E6	47.788	43.188
5)	MB Aldrin	4.695	5.448	142.4E6	350.1E6	49.471	37.161
6)	B beta-BHC	4.405	4.822	97002591	348.2E6	77.228	70.676
7)	B delta-BHC	4.607	5.036	46527334	111.9E6	17.554	11.313 #
8)	B Heptachlo...	5.136	5.837	162.6E6	448.3E6	63.975	59.627
9)	A Endosulfan I	5.472	6.195	114.5E6	358.3E6	49.943	45.788
10)	B trans-Chl...	5.359	6.071	135.8E6	326.3E6	52.545	37.891 #
11)	B cis-Chlor...	5.418	6.143	126.5E6	355.3E6	49.670	41.408
12)	B 4,4'-DDE	5.582	6.302	308.1E6	926.3E6	134.895	121.638
13)	MA Dieldrin	5.712	6.451	1483.0E6	4147.8E6	594.278m	519.922m
14)	MA Endrin	5.971	6.672	377.5E6	937.1E6	178.421	138.084
15)	B Endosulfa...	6.243	6.887	162.3E6	571.3E6	78.167	79.672
16)	A 4,4'-DDD	6.099	6.798	374.3E6	633.1E6	206.808	98.066 #
17)	MA 4,4'-DDT	6.335	7.096	197.5E6	700.8E6	104.479	106.088
18)	B Endrin al...	6.413	7.010	154.4E6	451.3E6	105.972	84.818
19)	B Endosulfa...	6.624	7.233	133.7E6	727.3E6	73.316	105.539 #
20)	A Methoxychlor	6.883	7.558	479.2E6	1427.5E6	511.290	441.715
21)	B Endrin ke...	7.114	7.706	384.9E6	1676.7E6	186.801m	213.914m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
Data File : PD066992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 14:45
Operator : AR\AJ
Sample : M4677-07MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:19:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

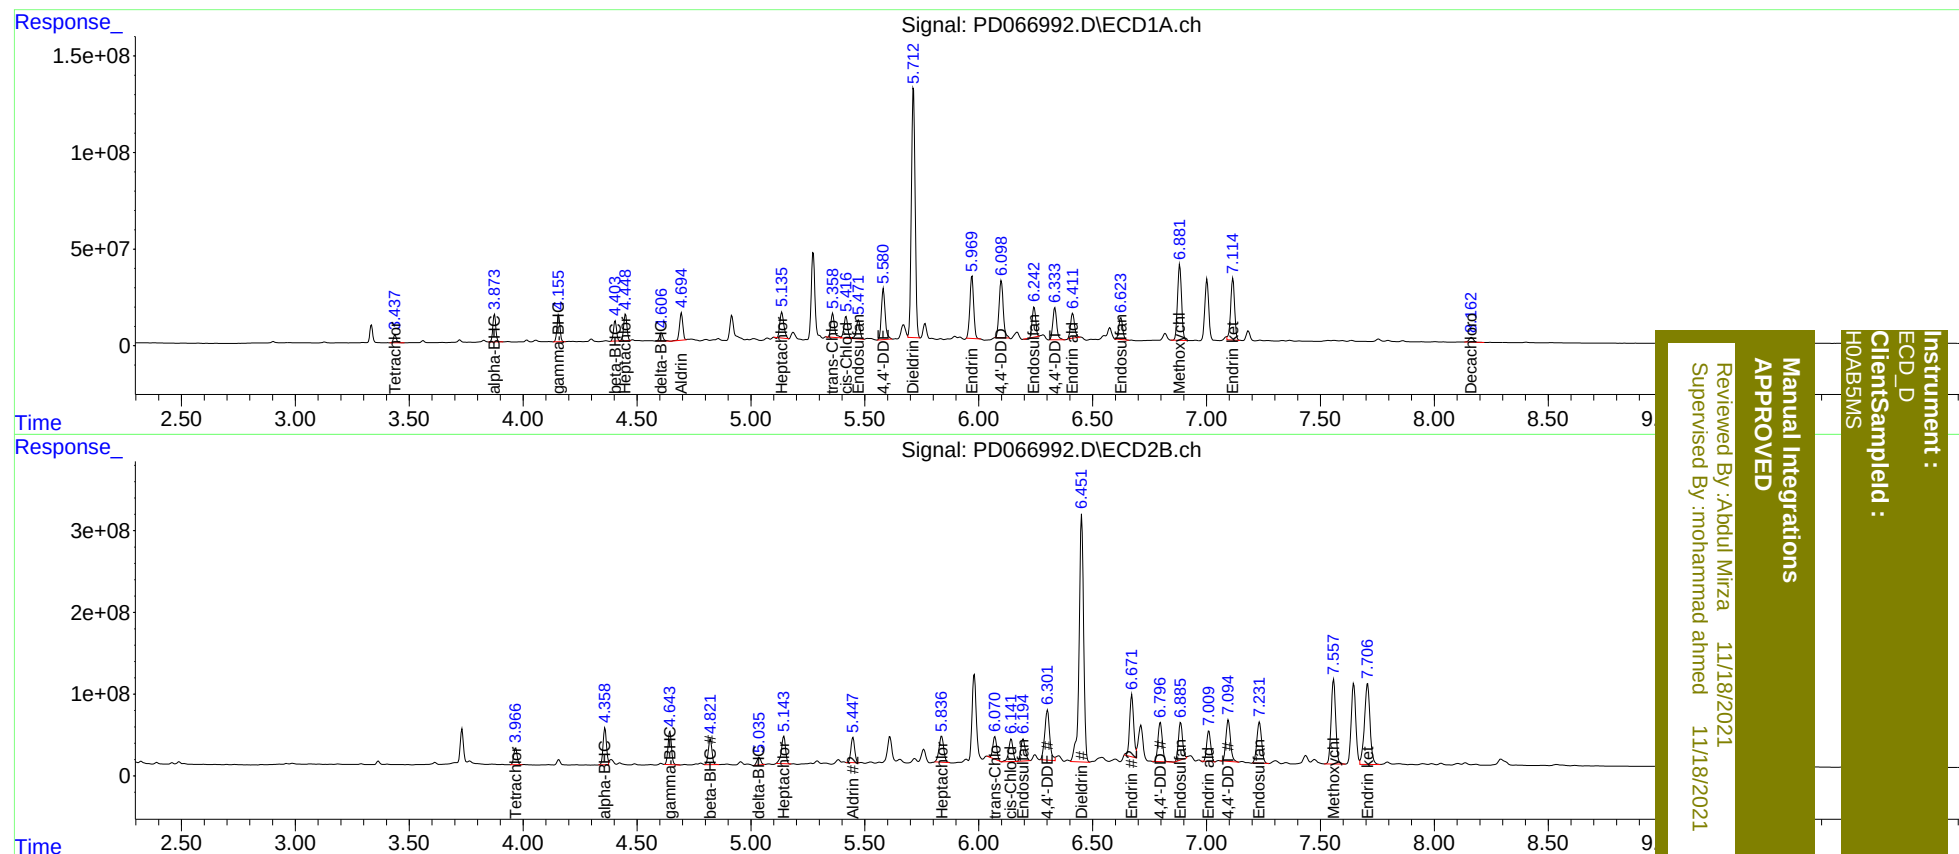

Reviewed By: Abdul Mirza 11/18/2021
Supervised By: mohammad ahmed 11/18/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
Client: Sampled :
HOABSMS