

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
 Data File : PD066993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2021 14:59
 Operator : AR\AJ
 Sample : M4677-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0AB5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2021
 Supervised By : mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:19:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.967	36540410	210.2E6	18.903	24.270 #
2)	SA Decachlor...	8.161	9.025	31806200	188.9E6	27.146	36.216 #
Target Compounds							
2)	A alpha-BHC	3.874	4.358	128.1E6	466.6E6	43.747	42.677m
3)	MA gamma-BHC...	4.155	4.644	128.1E6	426.5E6	46.262	42.203
4)	MA Heptachlor	4.449	5.144	135.9E6	423.3E6	47.759	43.192
5)	MB Aldrin	4.694	5.448	142.7E6	348.9E6	49.569	37.030 #
6)	B beta-BHC	4.404	4.822	96107893	344.7E6	76.516	69.953
7)	B delta-BHC	4.606	5.036	46398953	111.3E6	17.505	11.252 #
8)	B Heptachlo...	5.135	5.837	162.0E6	444.0E6	63.730	59.065
9)	A Endosulfan I	5.471	6.195	115.4E6	355.7E6	50.364	45.459
10)	B trans-Chl...	5.358	6.071	134.9E6	324.2E6	52.187	37.648 #
11)	B cis-Chlor...	5.416	6.142	126.9E6	356.0E6	49.826	41.490
12)	B 4,4'-DDE	5.580	6.301	307.4E6	924.9E6	134.572	121.462
13)	MA Dieldrin	5.711	6.451	1475.9E6	4135.8E6	591.443m	518.422m
14)	MA Endrin	5.969	6.672	372.6E6	926.0E6	176.100	136.448
15)	B Endosulfa...	6.242	6.886	163.2E6	578.9E6	78.577	80.732
16)	A 4,4'-DDD	6.098	6.797	377.2E6	635.6E6	208.393	98.453 #
17)	MA 4,4'-DDT	6.333	7.095	195.4E6	703.1E6	103.332	106.430
18)	B Endrin al...	6.411	7.010	160.1E6	453.5E6	109.899	85.235
19)	B Endosulfa...	6.622	7.232	132.1E6	725.2E6	72.437	105.237 #
20)	A Methoxychlor	6.881	7.558	480.0E6	1431.5E6	512.145	442.934
21)	B Endrin ke...	7.113	7.704	381.1E6	1656.2E6	184.979m	211.291m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111721\
Data File : PD066993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2021 14:59
Operator : AR\AJ
Sample : M4677-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:19:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

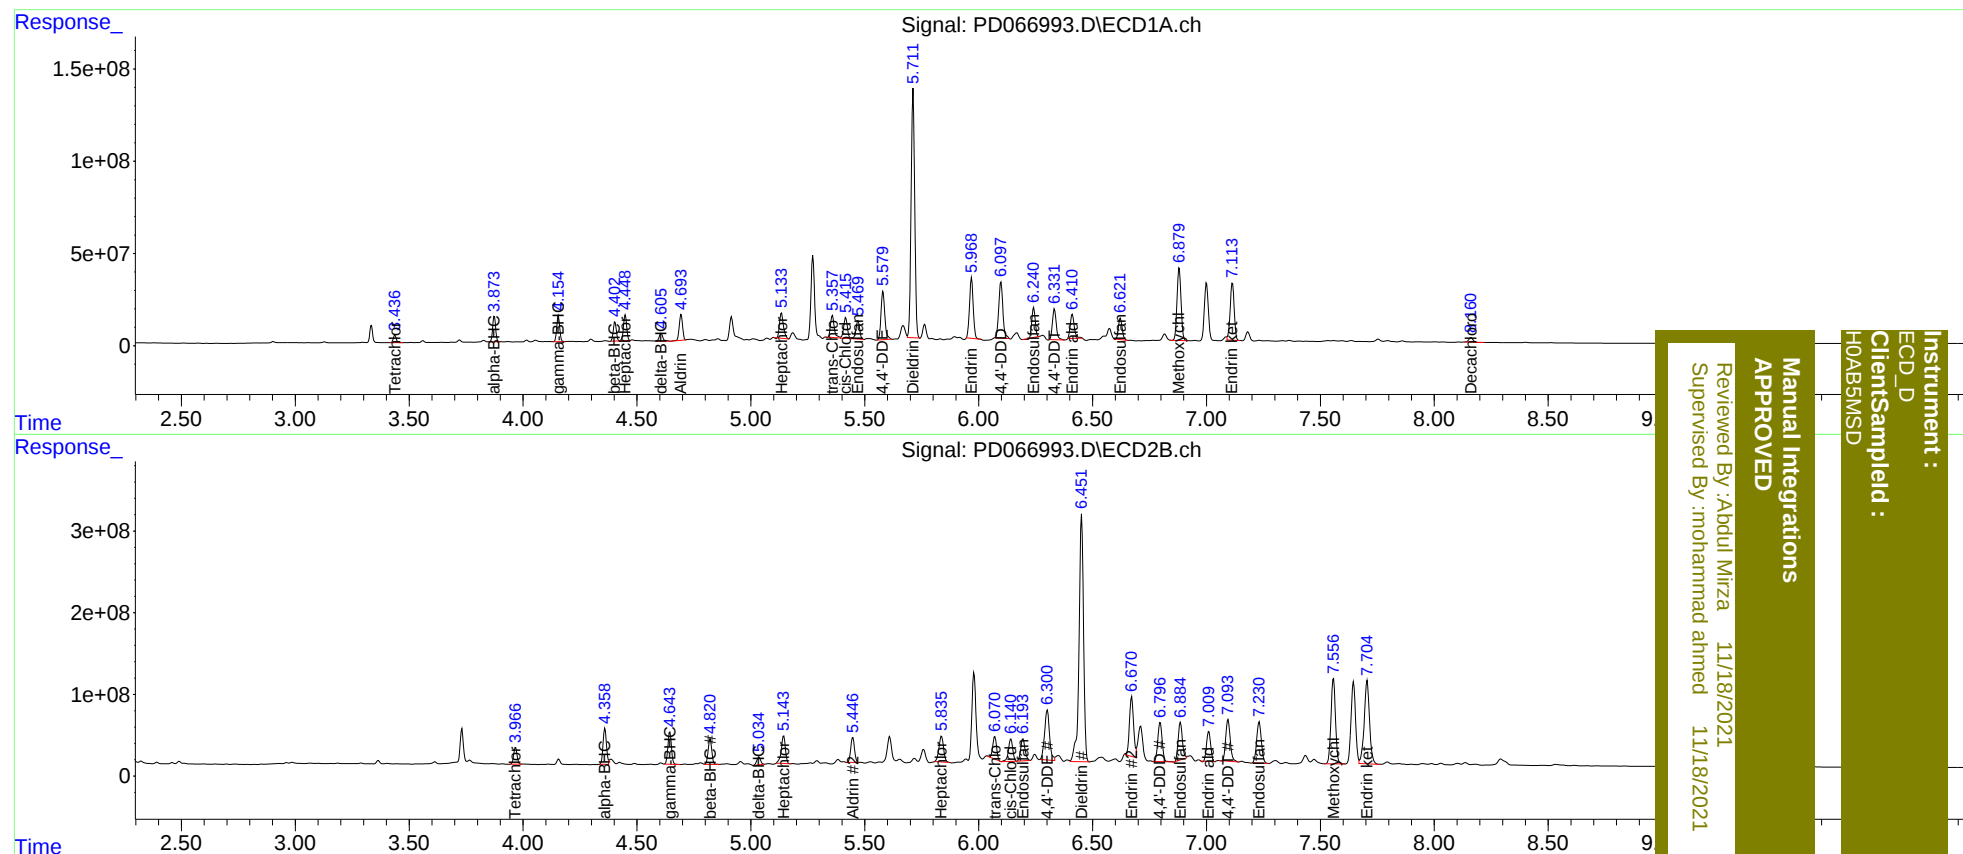

Instrument :
ECD_D
ClientSampled :
HOAB5MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/18/2021
Supervised By: mohammad ahmed 11/18/2021