

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 01:28
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:30:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.660f	3.441	160593	2180361	<MDL	<MDL #
27)	SA Decachlor...	7.832	0.000	264081	0	0.116	N.D. #
Target Compounds							
2)	A alpha-BHC	0.000	3.918	0	3800906	N.D.	<MDL
3)	MA gamma-BHC...	0.000	4.252	0	2284322	N.D.	<MDL
4)	MA Heptachlor	0.000	4.808	0	2929931	N.D.	<MDL
5)	MB Aldrin	0.000	5.159	0	2914560	N.D.	<MDL
6)	B beta-BHC	0.000	4.425f	0	1857331	N.D.	<MDL
7)	B delta-BHC	0.000	4.722	0	7523854	N.D.	0.138
8)	B Heptachlo...	4.630	5.594	280047	174.5E6	<MDL	5.161 #
10)	B trans-Chl...	4.891	5.863	1176404	18106925	0.382	0.573 #
11)	B cis-Chlor...	4.943	5.863f	2519280	18106925	0.805	0.570 #
12)	B 4,4'-DDE	5.144	6.106	3720961	317360	1.244	<MDL #
13)	MA Dieldrin	5.316	6.192f	177662	12640985	<MDL	0.419 #
15)	B Endosulfa...	5.863	0.000	472090	0	0.175	N.D. #
18)	B Endrin al...	6.085f	0.000	126444	0	<MDL	N.D. #
20)	A Methoxychlor	6.532	0.000	279973	0	0.224	N.D. #
22)	Toxaphene-1	0.000	5.759	0	46371411	N.D.	394.623
23)	Toxaphene-2	0.000	6.123	0	5722208	N.D.	26.702
24)	Toxaphene-3	5.863	0.000	472090	0	21.963	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 01:28
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:30:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

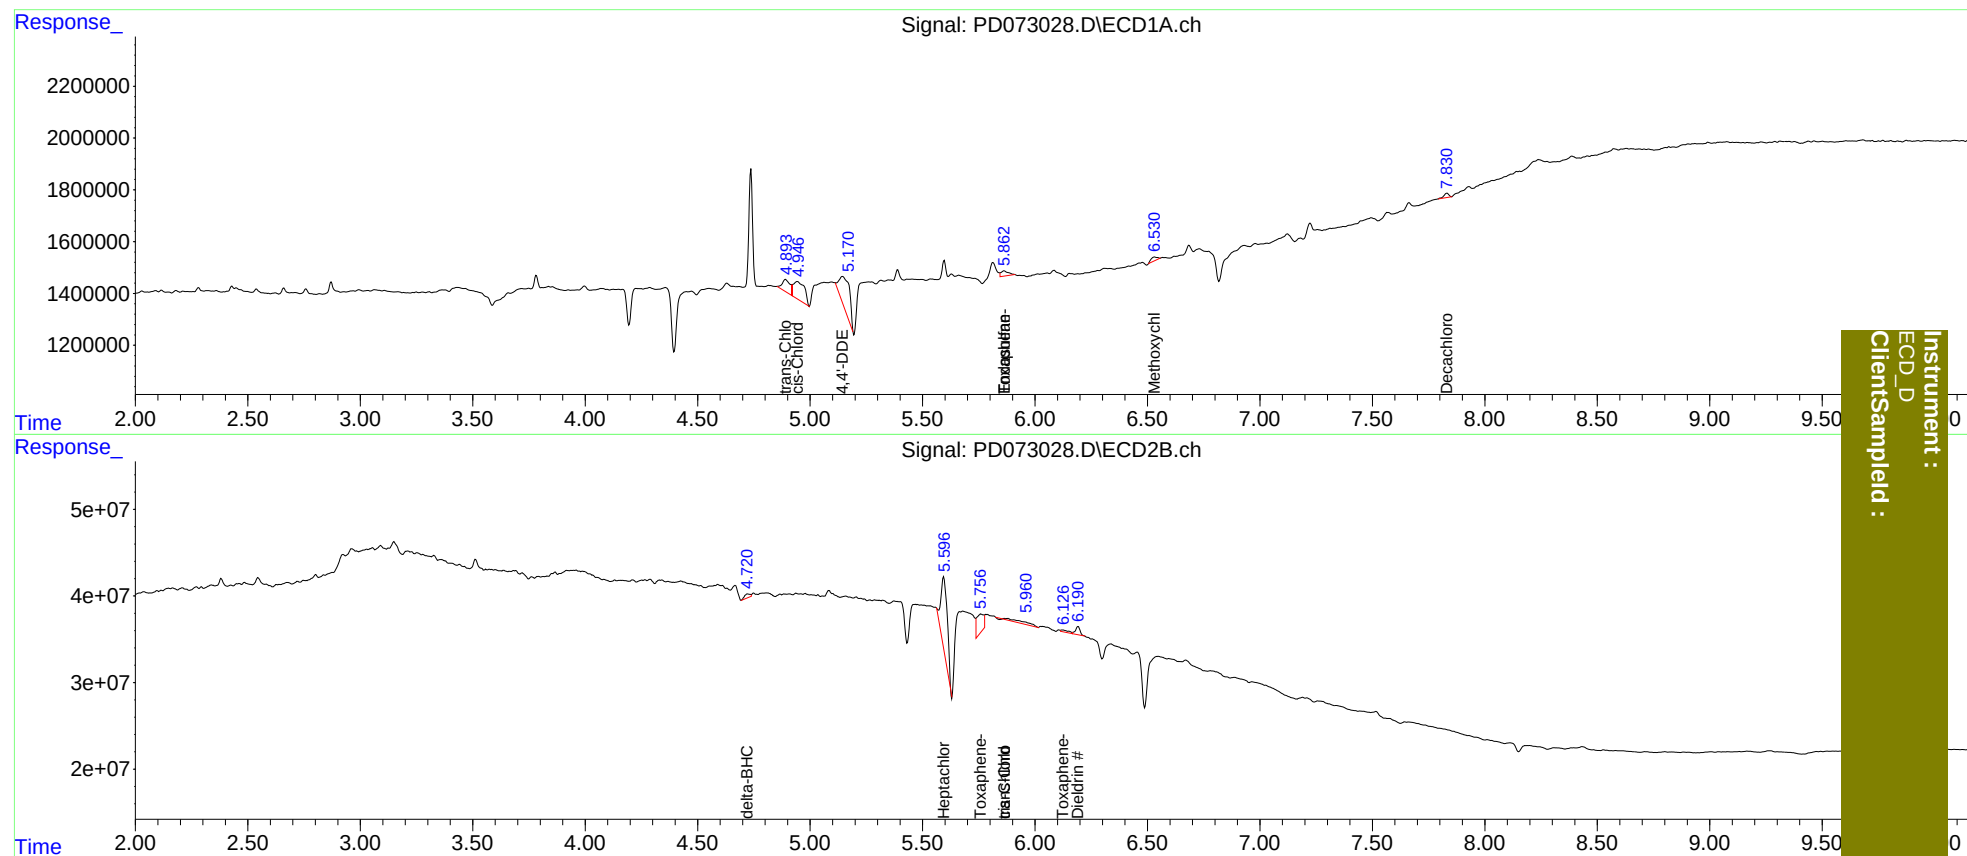


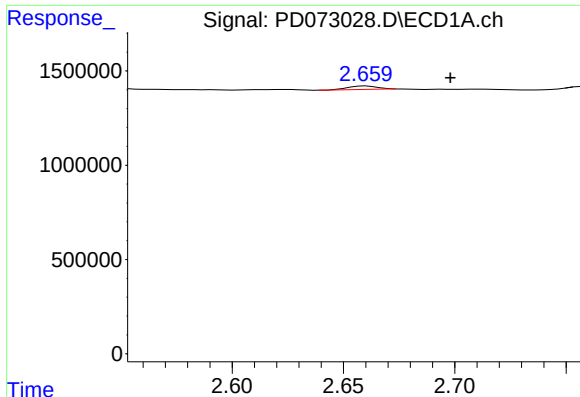

#1 Tetrachloro-m-xylene


R.T.: 2.660 min
Delta R.T.: -0.038 min
Response: 160593
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

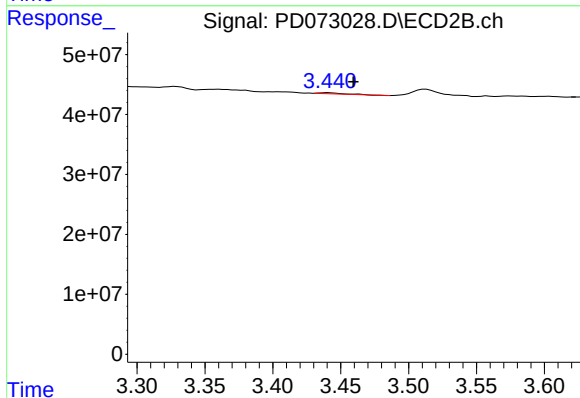


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: -0.018 min
Response: 2180361
Conc: N.D.

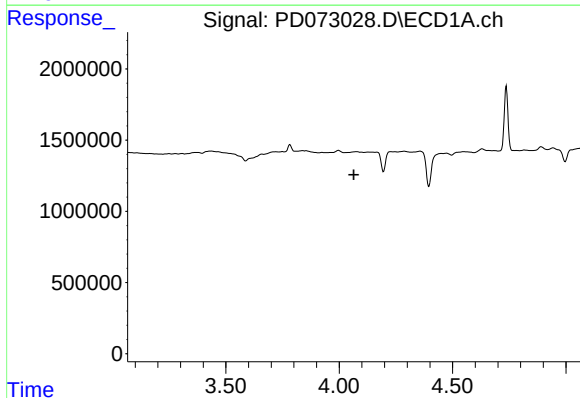


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.064 min
Response: 0
Conc: N.D.

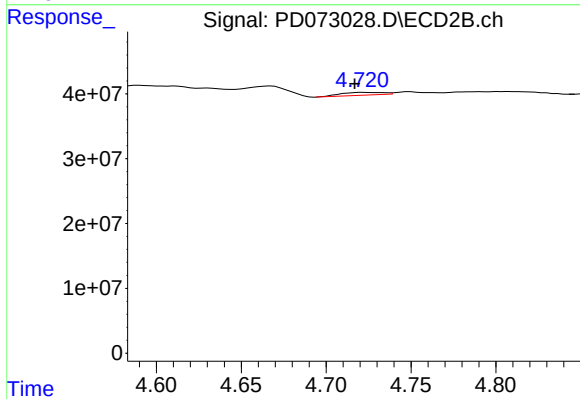

#7 delta-BHC


R.T.: 4.722 min
Delta R.T.: 0.005 min
Response: 7523854
Conc: 0.14 ng/ml

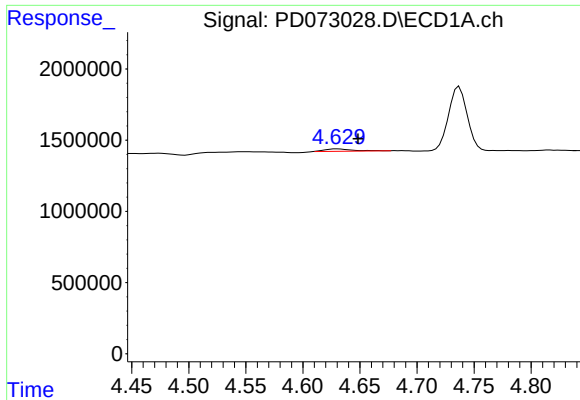

#8 Heptachlor epoxide


R.T.: 4.630 min
Delta R.T.: -0.018 min
Response: 280047
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

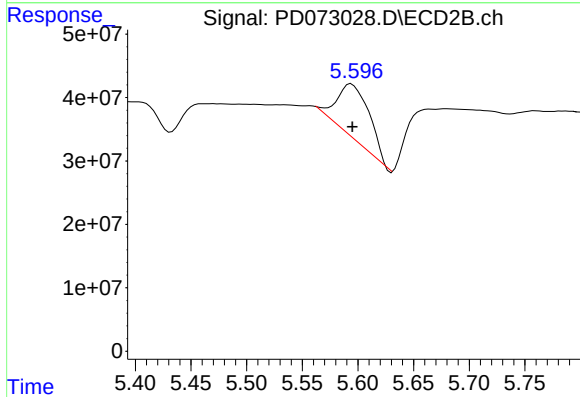


#8 Heptachlor epoxide

R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 174451033
Conc: 5.16 ng/ml

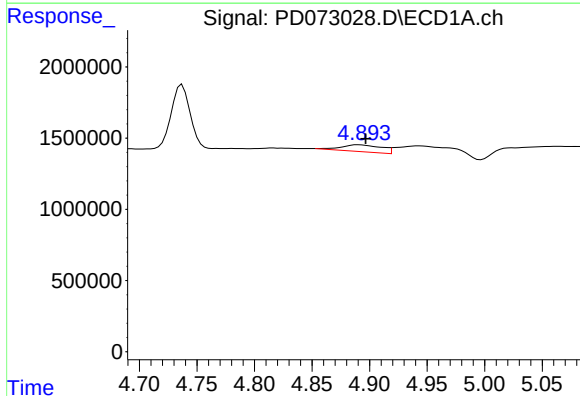


#10 trans-Chlordane

R.T.: 4.891 min
Delta R.T.: -0.006 min
Response: 1176404
Conc: 0.38 ng/ml

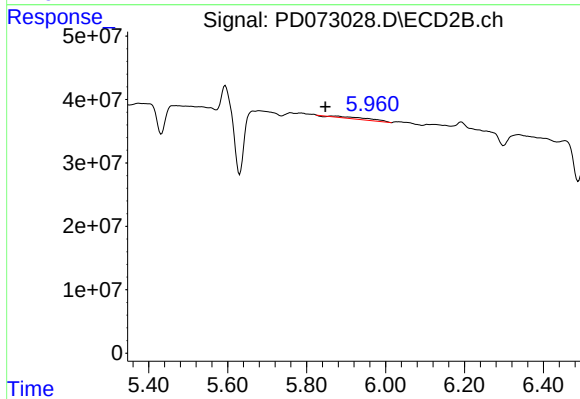

#10 trans-Chlordane


R.T.: 5.863 min
Delta R.T.: 0.015 min
Response: 18106925
Conc: 0.57 ng/ml

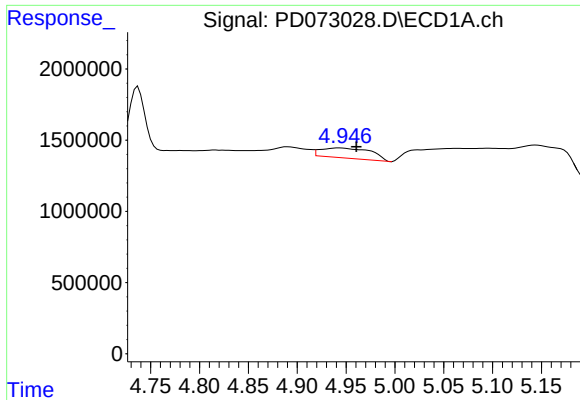

#11 cis-Chlordane


R.T.: 4.943 min
Delta R.T.: -0.017 min
Response: 2519280
Conc: 0.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

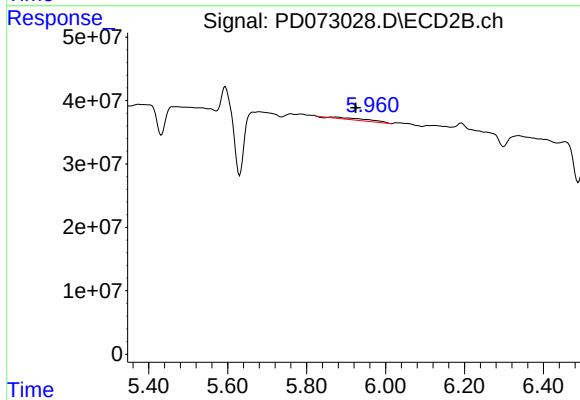


#11 cis-Chlordane

R.T.: 5.863 min
Delta R.T.: -0.061 min
Response: 18106925
Conc: 0.57 ng/ml

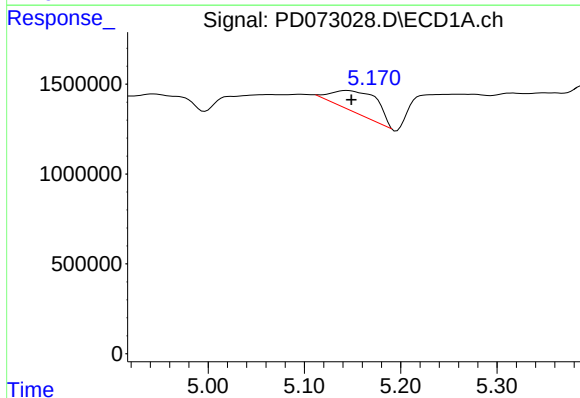


#12 4,4'-DDE

R.T.: 5.144 min
Delta R.T.: -0.004 min
Response: 3720961
Conc: 1.24 ng/ml

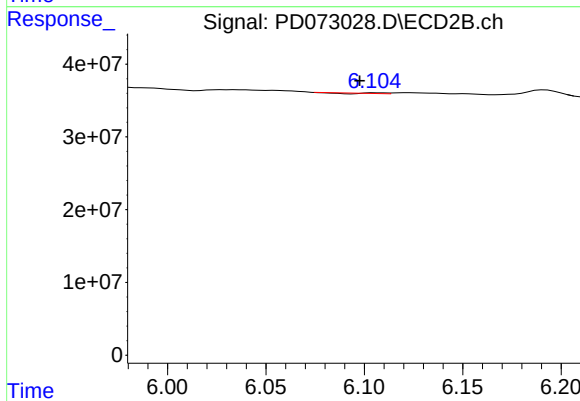

#12 4,4'-DDE


R.T.: 6.106 min
Delta R.T.: 0.008 min
Response: 317360
Conc: N.D.

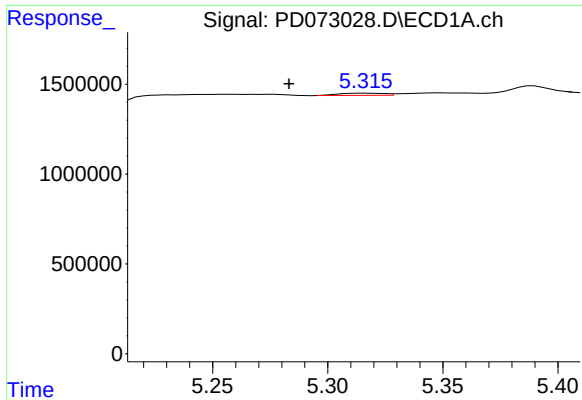

#13 Dieldrin


R.T.: 5.316 min
Delta R.T.: 0.033 min
Response: 177662
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

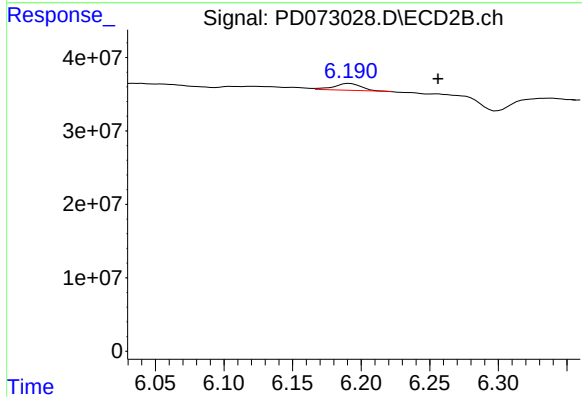


#13 Dieldrin

R.T.: 6.192 min
Delta R.T.: -0.064 min
Response: 12640985
Conc: 0.42 ng/ml

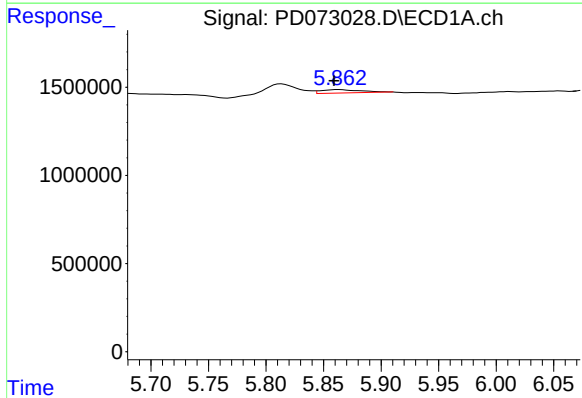


#15 Endosulfan II

R.T.: 5.863 min
Delta R.T.: 0.004 min
Response: 472090
Conc: 0.18 ng/ml

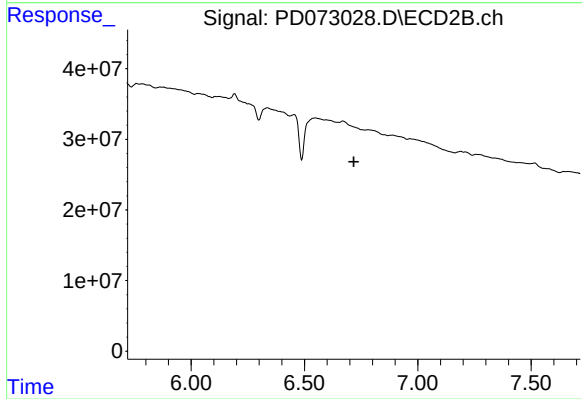

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.718 min
Response: 0
Conc: N.D.

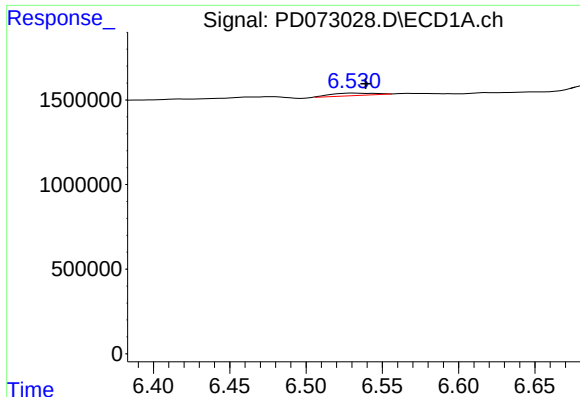

#20 Methoxychlor


R.T.: 6.532 min
Delta R.T.: -0.007 min
Response: 279973
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

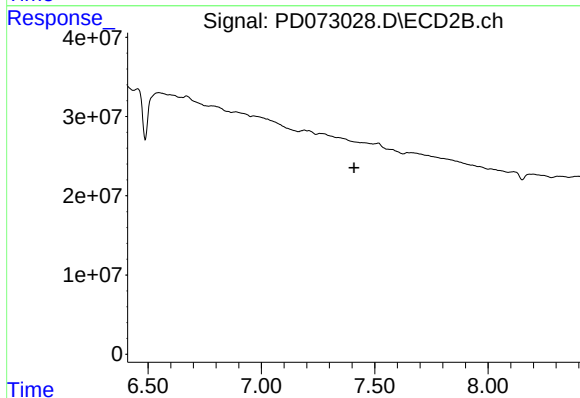


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.409 min
Response: 0
Conc: N.D.

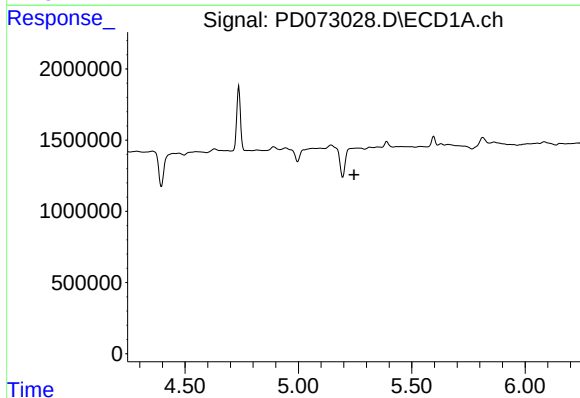


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.246 min
Response: 0
Conc: N.D.

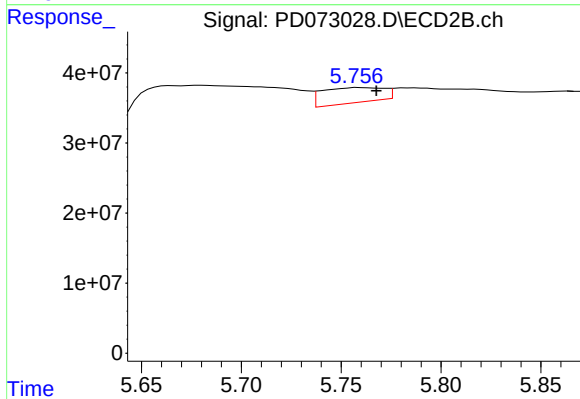

#22 Toxaphene-1


R.T.: 5.759 min
Delta R.T.: -0.009 min
Response: 46371411
Conc: 394.62 ng/ml

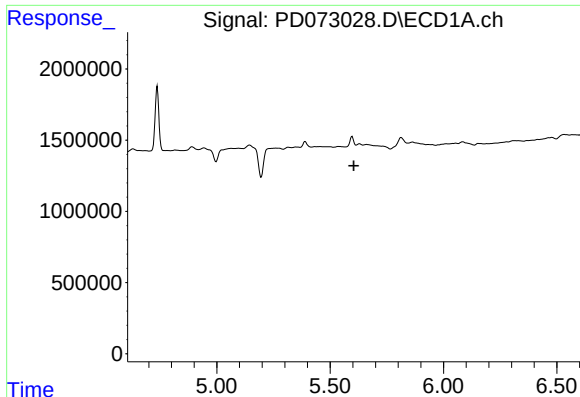

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 5.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

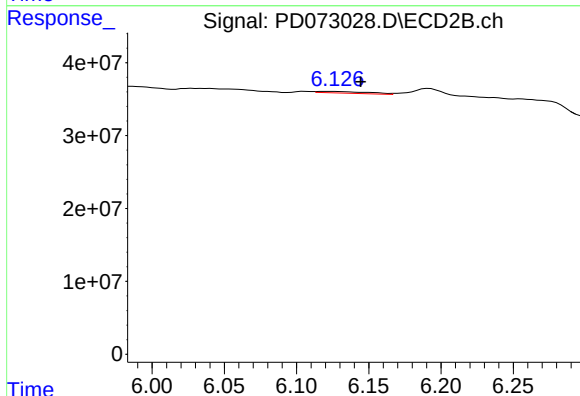


#23 Toxaphene-2

R.T.: 6.123 min
Delta R.T.: -0.021 min
Response: 5722208
Conc: 26.70 ng/ml

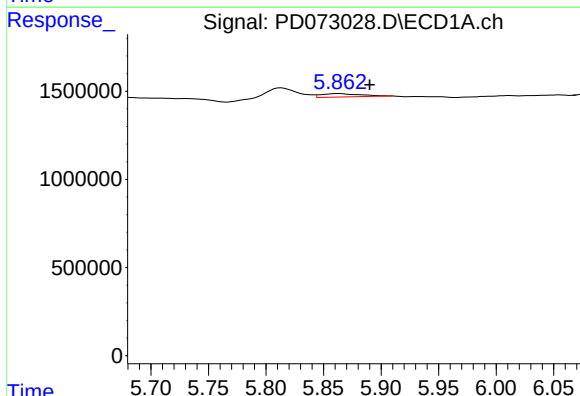


#24 Toxaphene-3

R.T.: 5.863 min
Delta R.T.: -0.027 min
Response: 472090
Conc: 21.96 ng/ml

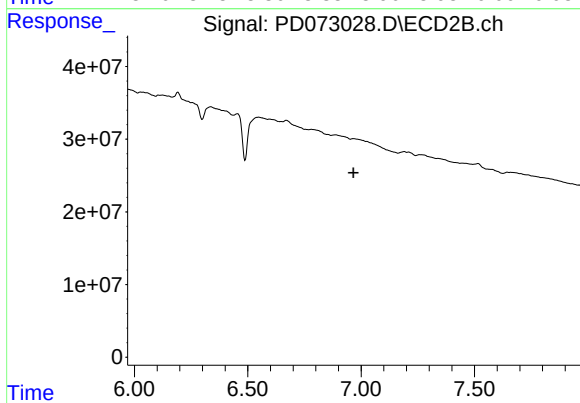

#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 6.966 min
Response: 0
Conc: N.D.

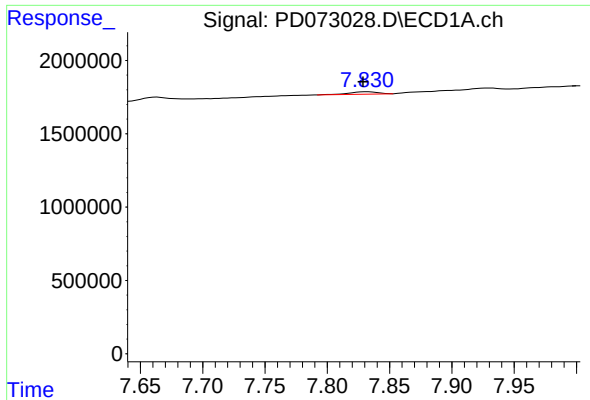


#27 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: 0.004 min
Response: 264081
Conc: 0.12 ng/ml

Instrument :

ECD_D

ClientSampleId :

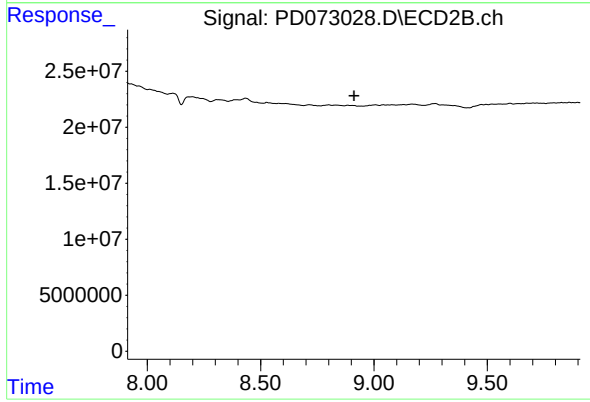

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.913 min
Response: 0
Conc: N.D.