

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 03:14
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:02:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:58:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	12783946	367.0E6	5.343	5.646
27)	SA Decachlor...	7.829	8.913	25632552	165.6E6	11.337	11.172
Target Compounds							
2)	A alpha-BHC	3.201	3.924	17447636	495.1E6	4.763	5.768
3)	MA gamma-BHC...	3.532	4.258	16181424	393.1E6	4.895	5.897
4)	MA Heptachlor	3.864	4.824	17078694	270.7E6	5.163	5.958
9)	A Endosulfan I	5.017	5.980	14795319	165.9E6	5.256	5.712
13)	MA Dieldrin	5.283	6.257	30306317	332.4E6	9.877	11.078
14)	MA Endrin	5.560	6.489	27643586	279.8E6	10.247	11.447
16)	A 4,4'-DDD	5.707	6.623	23811312	251.9E6	9.845	11.030
17)	MA 4,4'-DDT	5.955	6.931	20922526	229.0E6	9.384	10.709
20)	A Methoxychlor	6.539	7.411	65394953	521.2E6	51.770	55.636


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 03:14
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:02:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:58:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

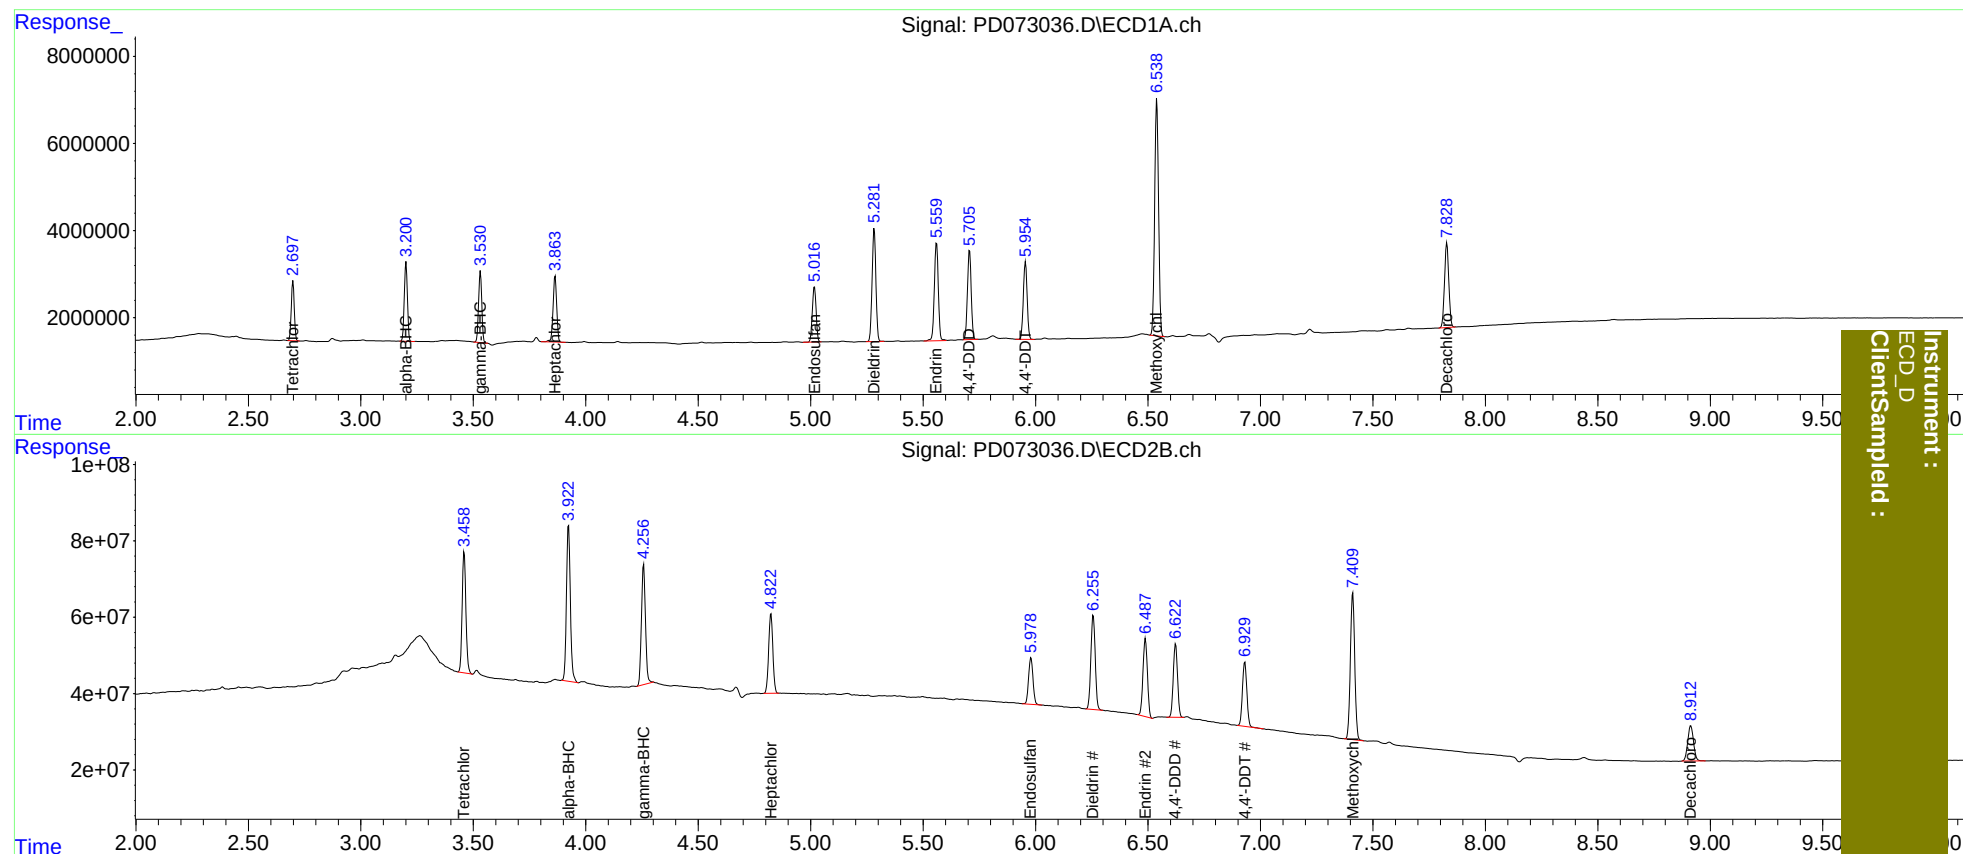


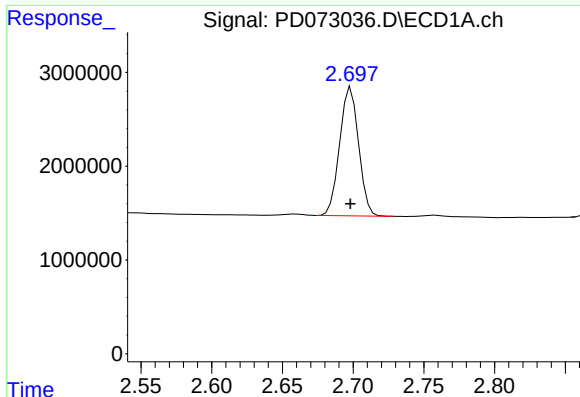

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 12783946
Conc: 5.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

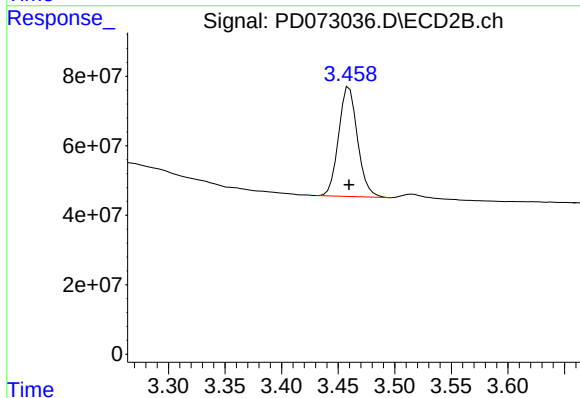


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 367005437
Conc: 5.65 ng/ml

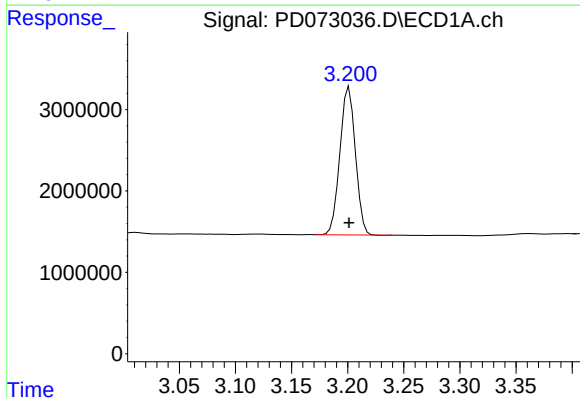


#2 alpha-BHC

R.T.: 3.201 min
Delta R.T.: 0.000 min
Response: 17447636
Conc: 4.76 ng/ml

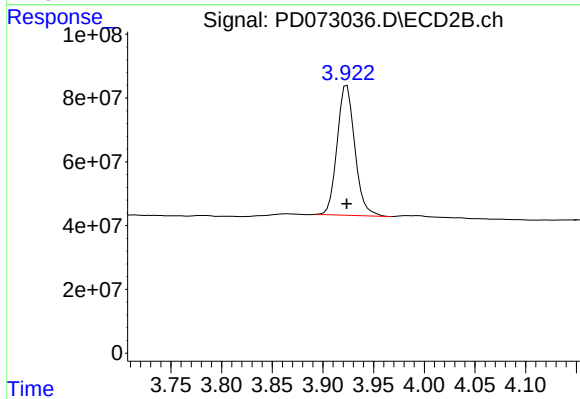

#2 alpha-BHC


R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 495111318
Conc: 5.77 ng/ml

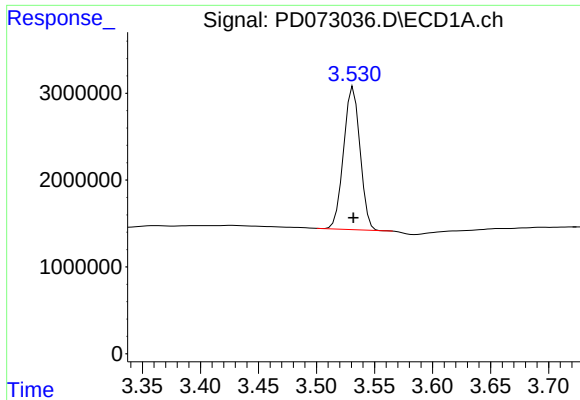

#3 gamma-BHC (Lindane)


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 16181424
Conc: 4.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

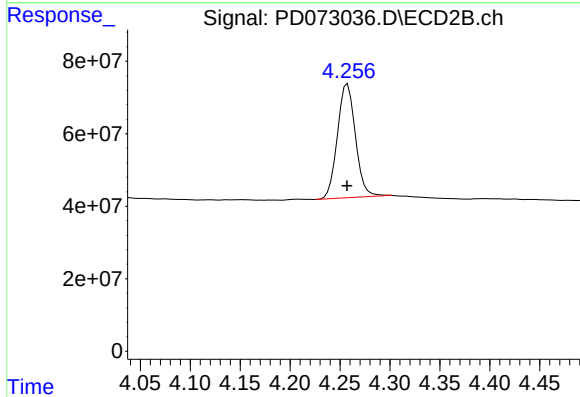


#3 gamma-BHC (Lindane)

R.T.: 4.258 min
Delta R.T.: 0.000 min
Response: 393119770
Conc: 5.90 ng/ml

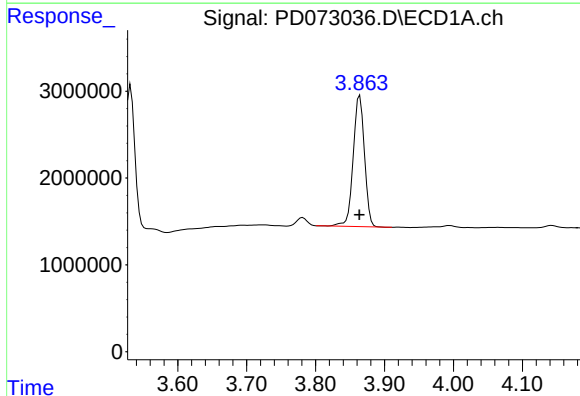


#4 Heptachlor

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 17078694
Conc: 5.16 ng/ml

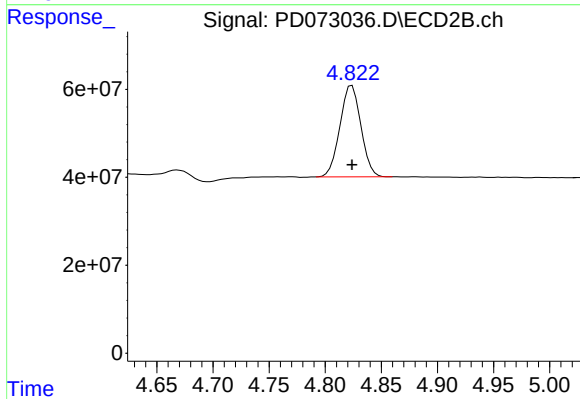

#4 Heptachlor


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 270659058
Conc: 5.96 ng/ml

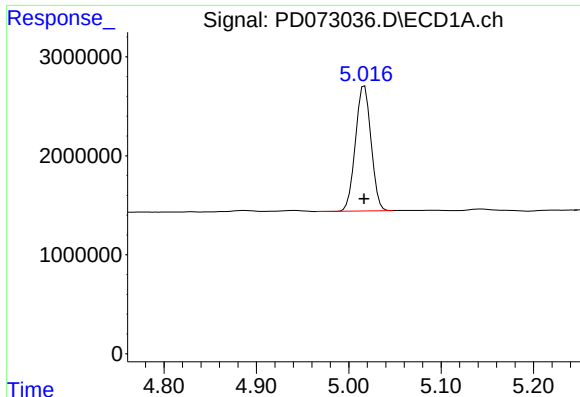

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 14795319
Conc: 5.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

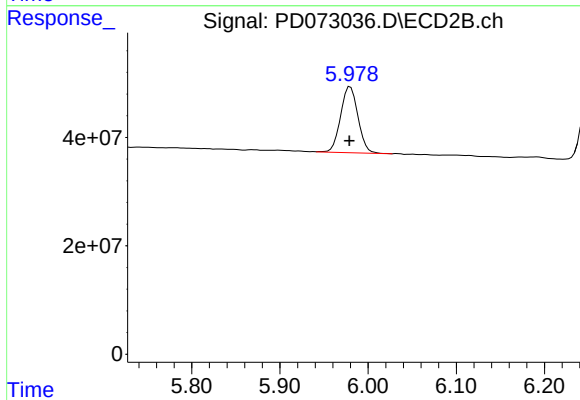


#9 Endosulfan I

R.T.: 5.980 min
Delta R.T.: 0.001 min
Response: 165908486
Conc: 5.71 ng/ml

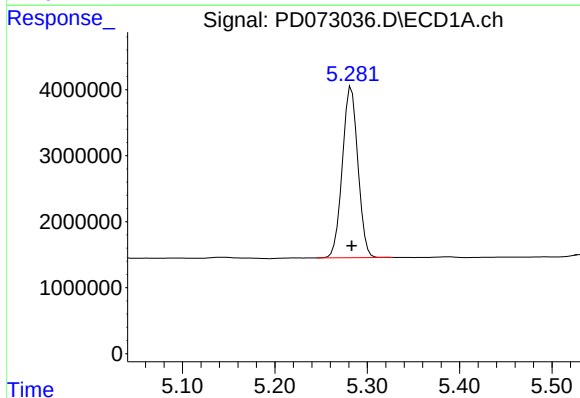


#13 Dieldrin

R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 30306317
Conc: 9.88 ng/ml

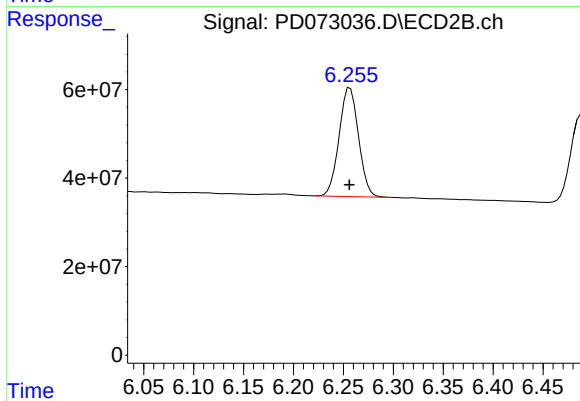

#13 Dieldrin


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 332402345
Conc: 11.08 ng/ml

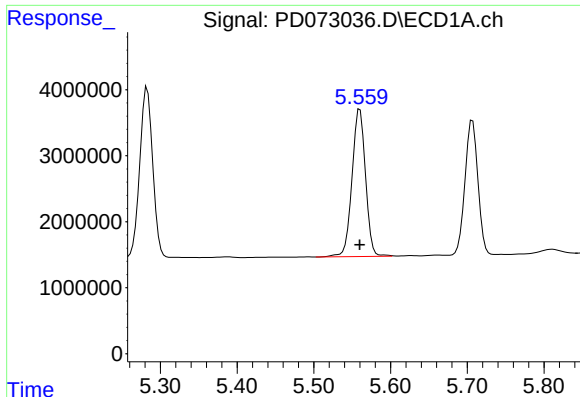

#14 Endrin


R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 27643586
Conc: 10.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

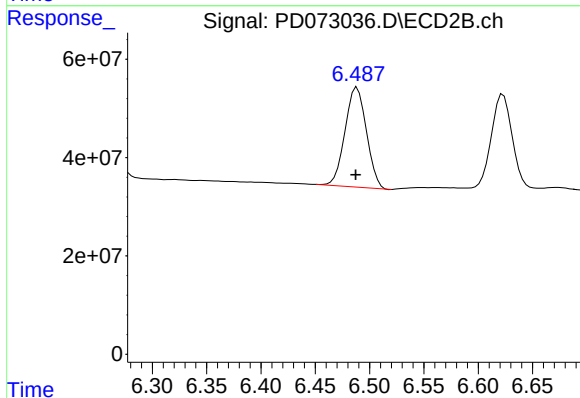


#14 Endrin

R.T.: 6.489 min
Delta R.T.: 0.001 min
Response: 279770243
Conc: 11.45 ng/ml

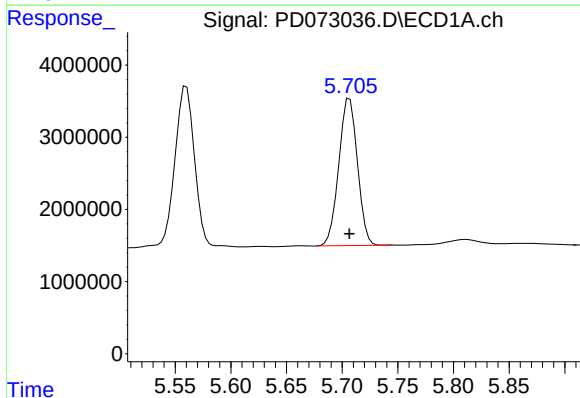


#16 4,4'-DDD

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 23811312
Conc: 9.85 ng/ml

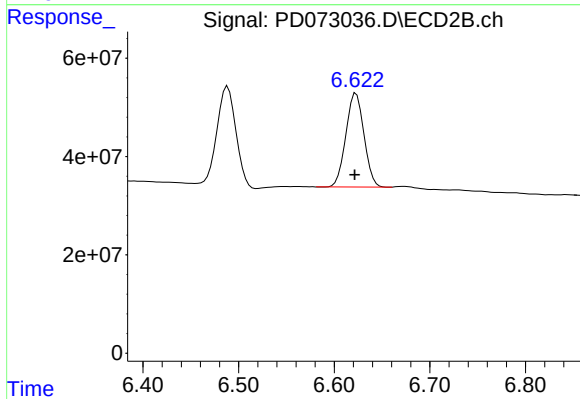

#16 4,4'-DDD


R.T.: 6.623 min
Delta R.T.: 0.001 min
Response: 251857188
Conc: 11.03 ng/ml

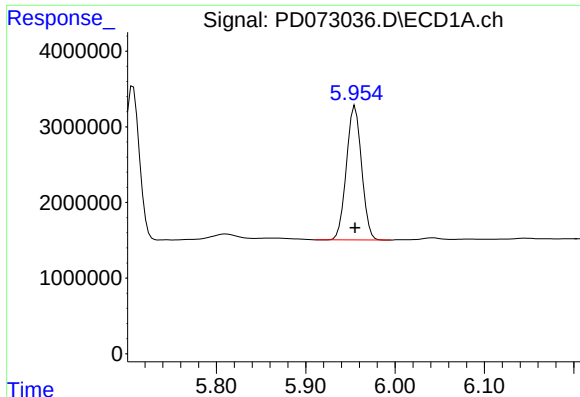

#17 4,4'-DDT


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 20922526
Conc: 9.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

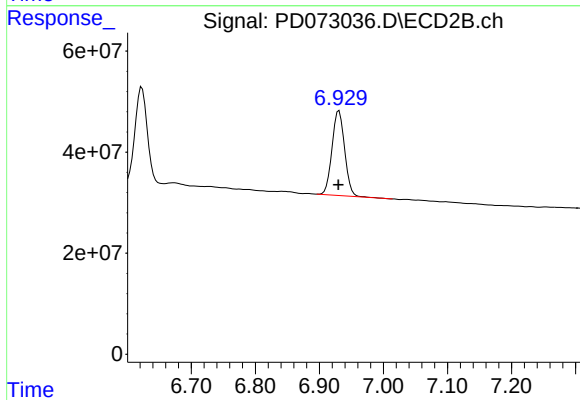


#17 4,4'-DDT

R.T.: 6.931 min
Delta R.T.: 0.001 min
Response: 229041148
Conc: 10.71 ng/ml

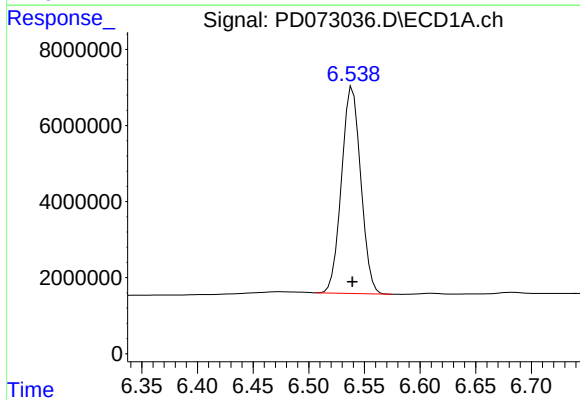


#20 Methoxychlor

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 65394953
Conc: 51.77 ng/ml

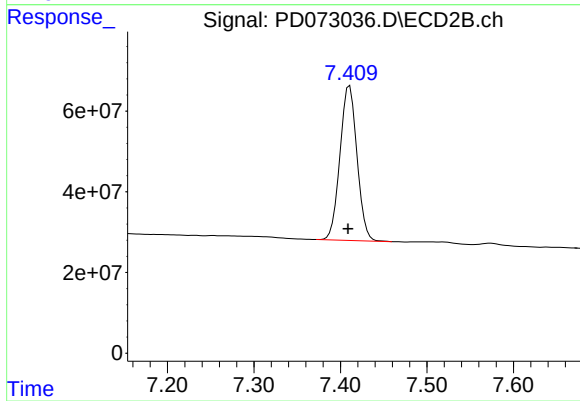

#20 Methoxychlor

R.T.: 7.411 min
Delta R.T.: 0.002 min
Response: 521249538
Conc: 55.64 ng/ml

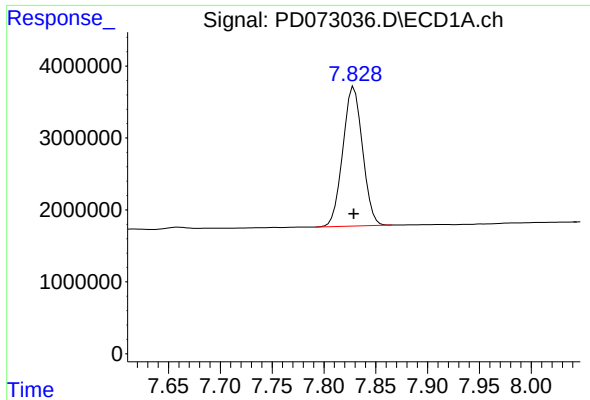

#27 Decachlorobiphenyl


R.T.: 7.829 min

Delta R.T.: 0.000 min

Response: 25632552

Conc: 11.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

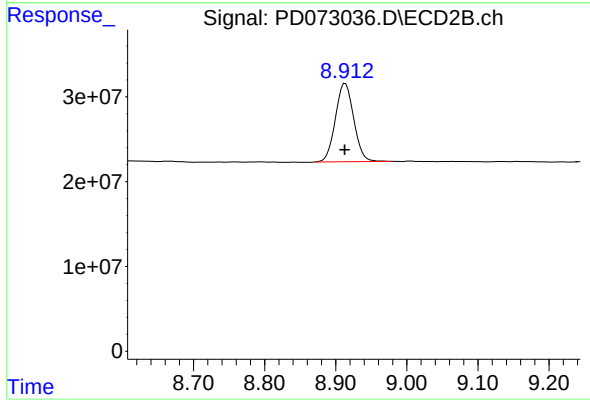

#27 Decachlorobiphenyl

R.T.: 8.913 min

Delta R.T.: 0.000 min

Response: 165583523

Conc: 11.17 ng/ml