

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 03:41
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:02:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:58:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	24093199	673.6E6	10.069	10.362
27)	SA Decachlor...	7.829	8.913	47667399	312.1E6	21.082	21.057
Target Compounds							
2)	A alpha-BHC	3.202	3.923	34773358	899.4E6	9.493	10.477
3)	MA gamma-BHC...	3.532	4.257	32024684	710.3E6	9.688	10.655
4)	MA Heptachlor	3.864	4.823	32731989	490.7E6	9.895	10.802
9)	A Endosulfan I	5.017	5.979	28401878	305.9E6	10.089	10.532
13)	MA Dieldrin	5.283	6.256	59715483	627.5E6	19.461	20.913
14)	MA Endrin	5.560	6.488	53561122	515.2E6	19.854	21.080
16)	A 4,4'-DDD	5.707	6.622	47259212	479.7E6	19.540	21.010
17)	MA 4,4'-DDT	5.956	6.930	42016236	441.9E6	18.845	20.661
20)	A Methoxychlor	6.540	7.410	126.6E6	981.0E6	100.234	104.705

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 03:41
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:02:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:58:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

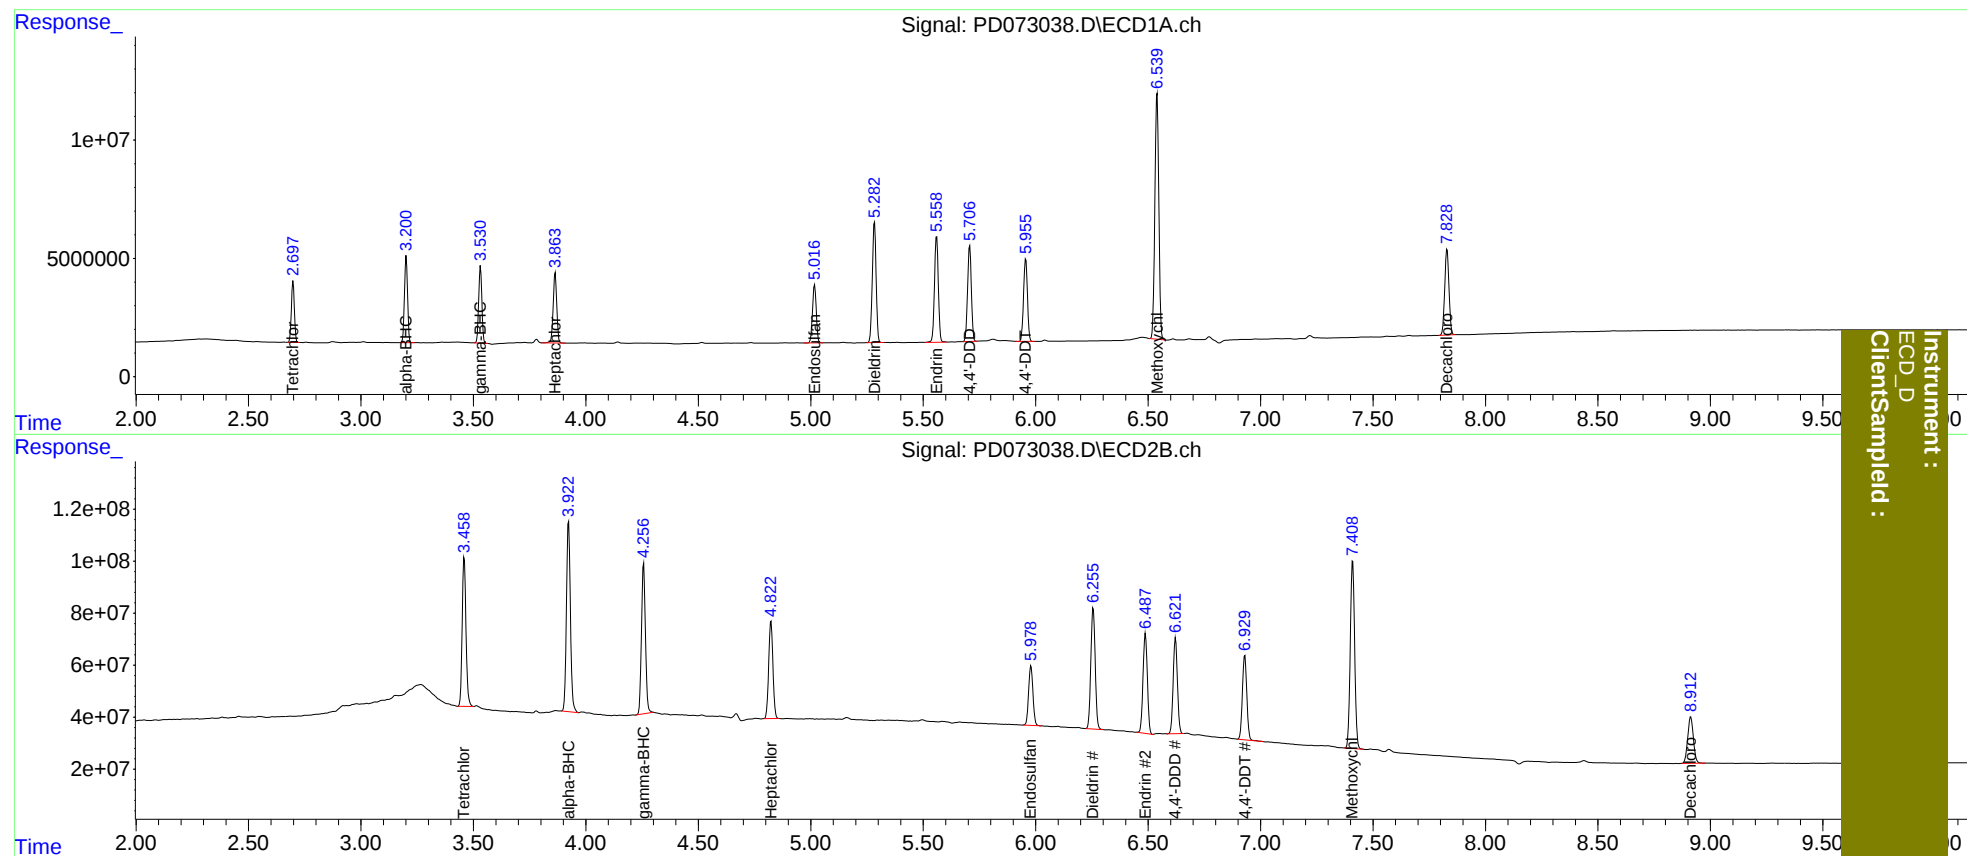


Instrument :
ECD_D
ClientSampled :
0

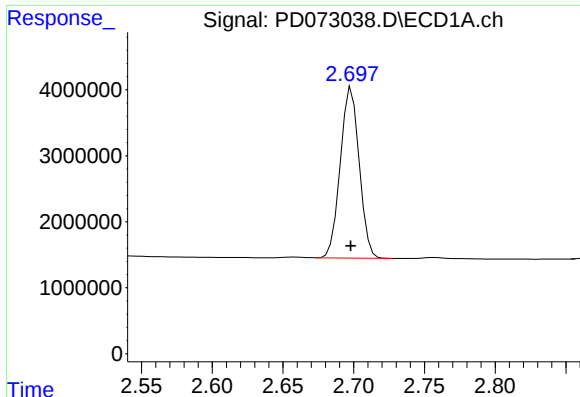

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 24093199
Conc: 10.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

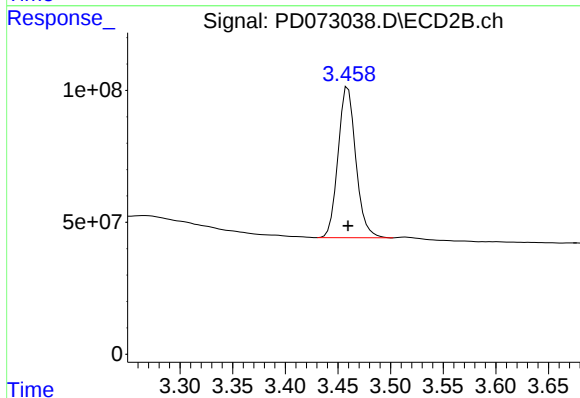


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 673564762
Conc: 10.36 ng/ml

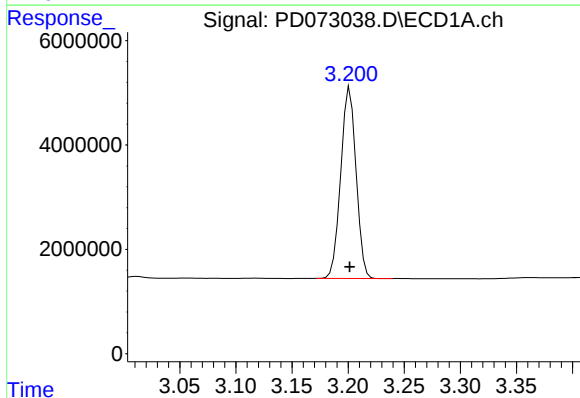


#2 alpha-BHC

R.T.: 3.202 min
Delta R.T.: 0.000 min
Response: 34773358
Conc: 9.49 ng/ml

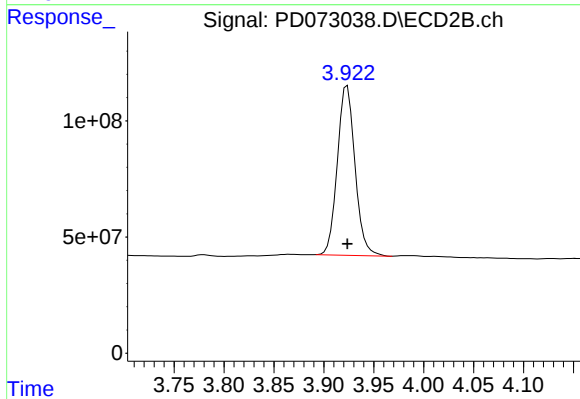

#2 alpha-BHC


R.T.: 3.923 min
Delta R.T.: 0.000 min
Response: 899373778
Conc: 10.48 ng/ml

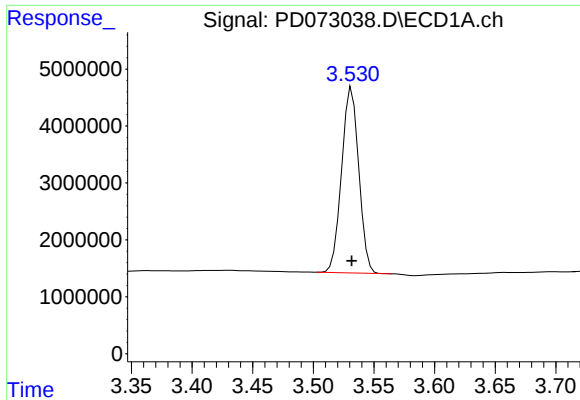

#3 gamma-BHC (Lindane)


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 32024684
Conc: 9.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

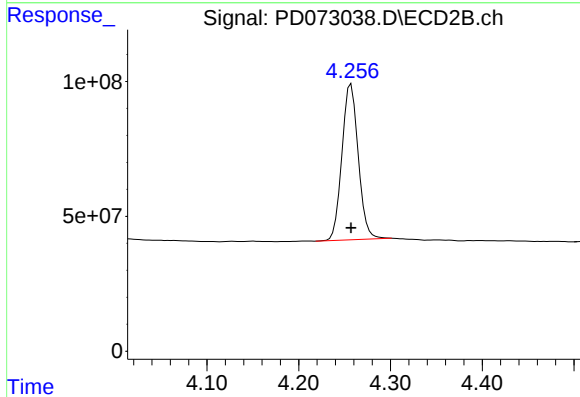


#3 gamma-BHC (Lindane)

R.T.: 4.257 min
Delta R.T.: 0.000 min
Response: 710265953
Conc: 10.65 ng/ml

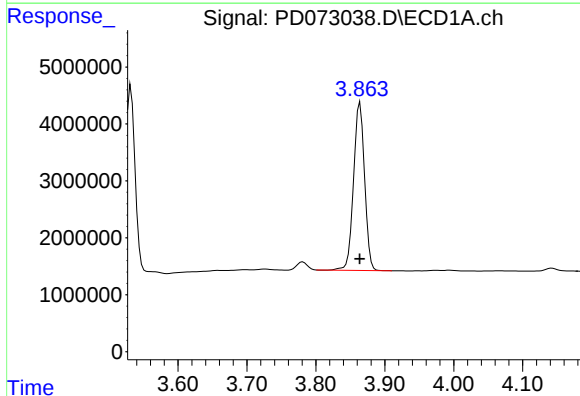


#4 Heptachlor

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 32731989
Conc: 9.89 ng/ml

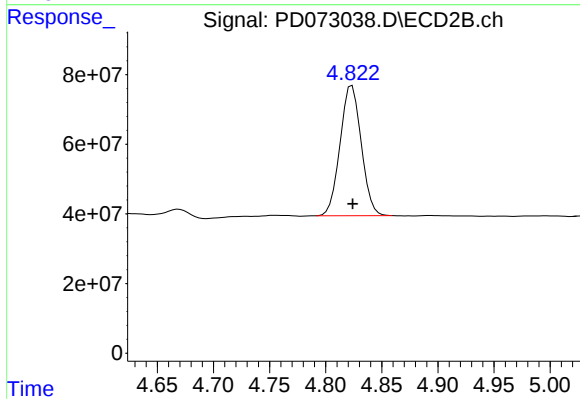

#4 Heptachlor


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 490723883
Conc: 10.80 ng/ml

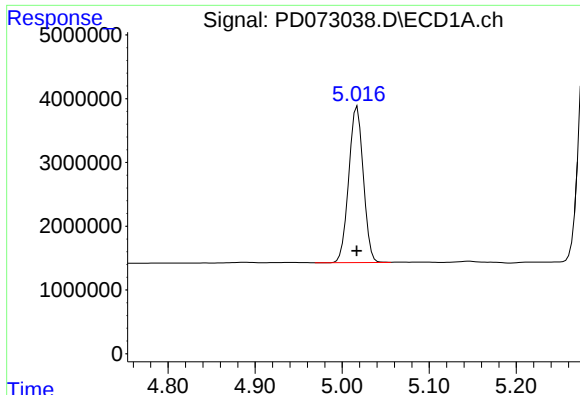

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 28401878
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

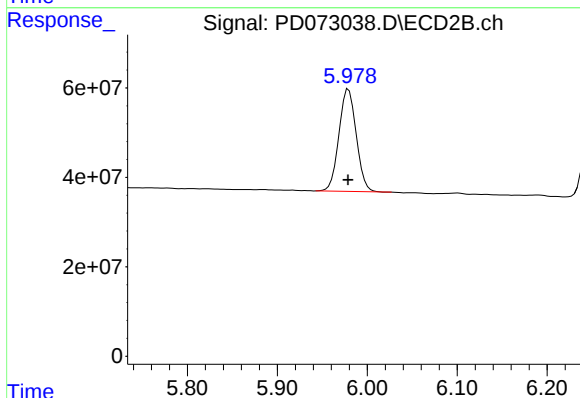


#9 Endosulfan I

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 305938756
Conc: 10.53 ng/ml

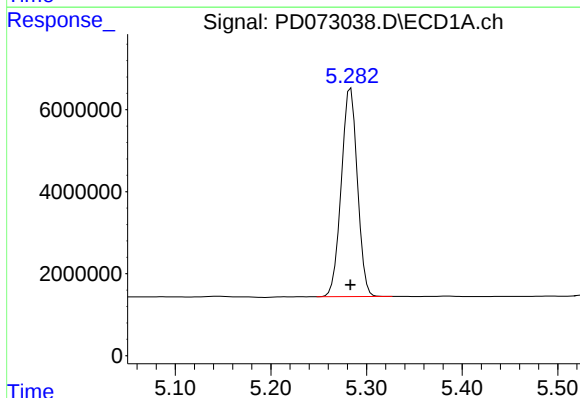


#13 Dieldrin

R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 59715483
Conc: 19.46 ng/ml

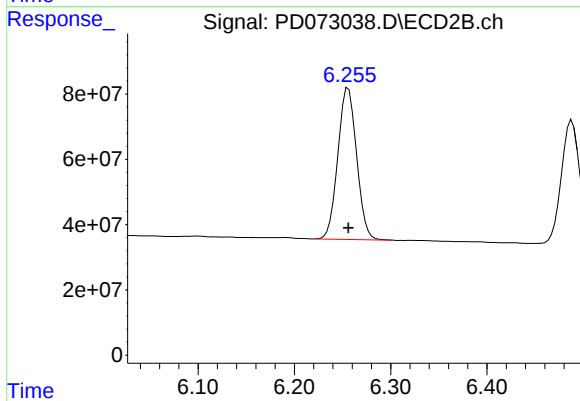

#13 Dieldrin


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 627486750
Conc: 20.91 ng/ml

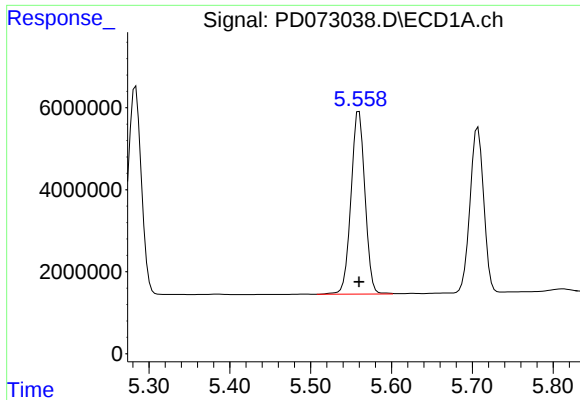

#14 Endrin


R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 53561122
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

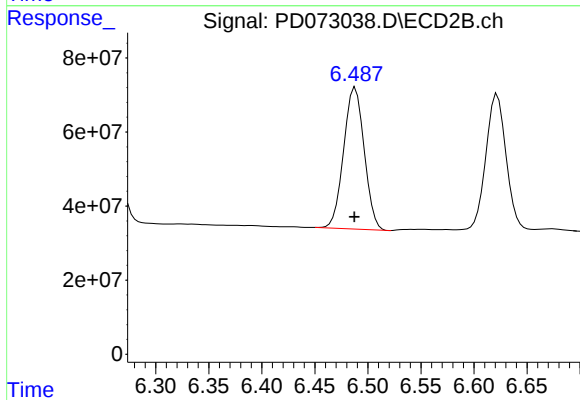


#14 Endrin

R.T.: 6.488 min
Delta R.T.: 0.001 min
Response: 515187561
Conc: 21.08 ng/ml

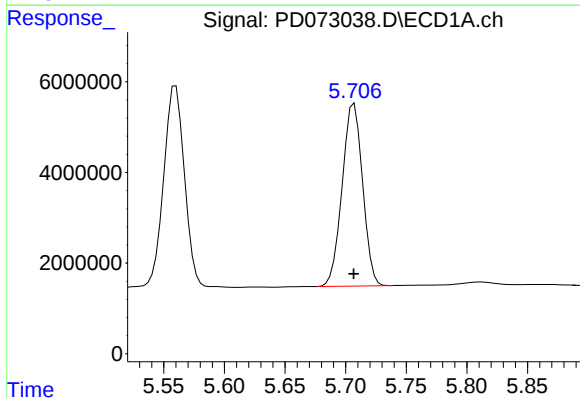


#16 4,4'-DDD

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 47259212
Conc: 19.54 ng/ml

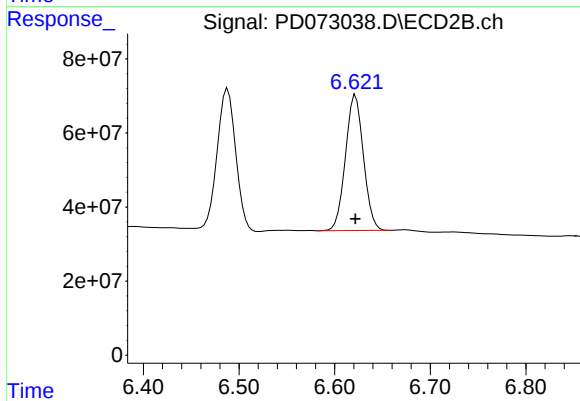

#16 4,4'-DDD


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 479718441
Conc: 21.01 ng/ml

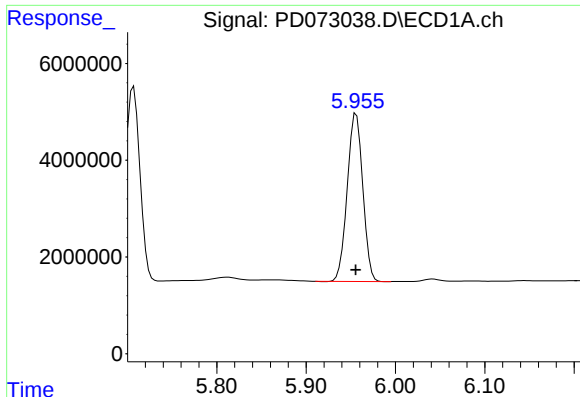

#17 4,4'-DDT


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 42016236
Conc: 18.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

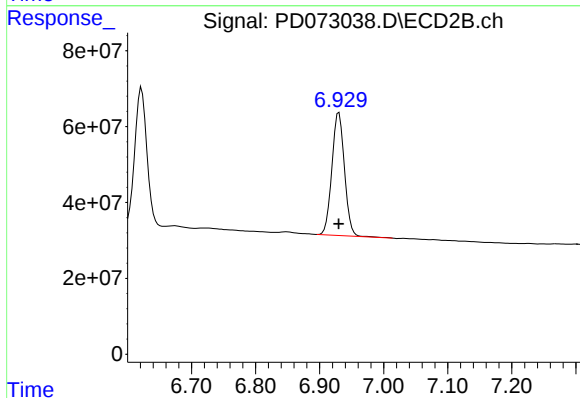


#17 4,4'-DDT

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 441882086
Conc: 20.66 ng/ml

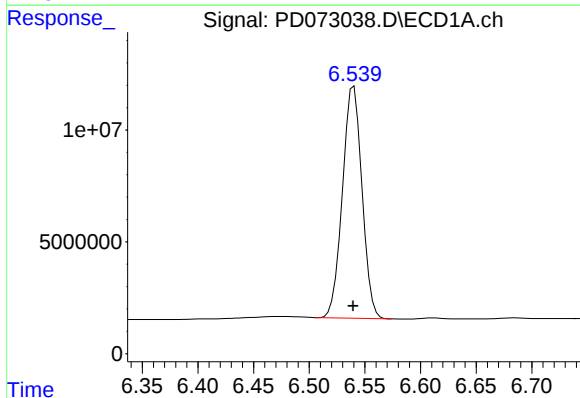


#20 Methoxychlor

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 126613666
Conc: 100.23 ng/ml

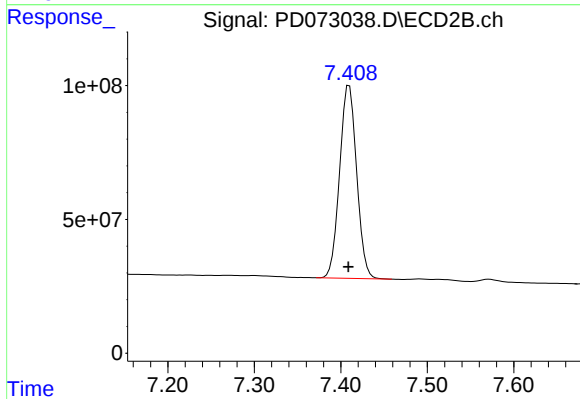

#20 Methoxychlor


R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 980965895
Conc: 104.71 ng/ml

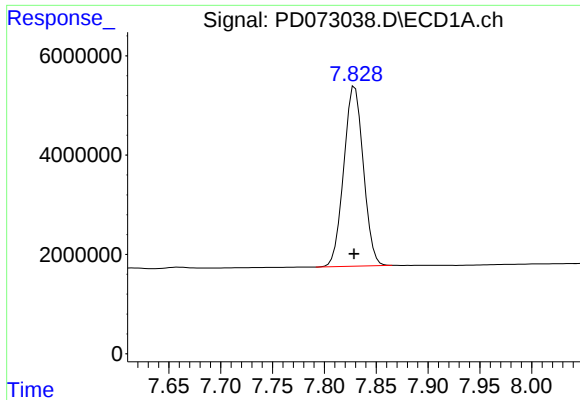

#27 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 47667399
Conc: 21.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

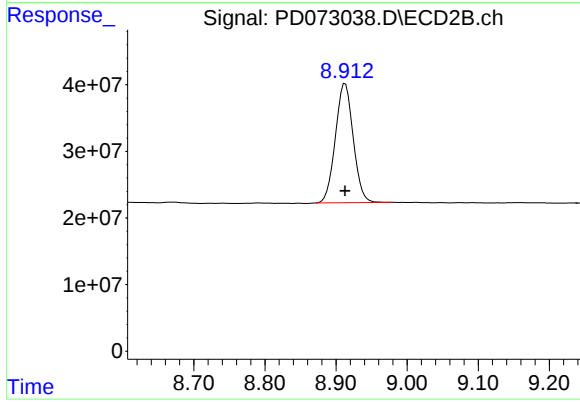

#27 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 312100366
Conc: 21.06 ng/ml