

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 04:08
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:02:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:58:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	47856202	1300.1E6	20.000	20.000
27)	SA Decachlor...	7.829	8.913	90440692	592.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.201	3.924	73262274	1716.8E6	20.000	20.000
3)	MA gamma-BHC...	3.532	4.257	66114748	1333.2E6	20.000	20.000
4)	MA Heptachlor	3.864	4.824	66160377	908.6E6	20.000	20.000
9)	A Endosulfan I	5.017	5.979	56301662	580.9E6	20.000	20.000
13)	MA Dieldrin	5.283	6.256	122.7E6	1200.2E6	40.000	40.000
14)	MA Endrin	5.560	6.487	107.9E6	977.6E6	40.000	40.000
16)	A 4,4'-DDD	5.707	6.622	96742456	913.3E6	40.000	40.000
17)	MA 4,4'-DDT	5.955	6.930	89182502	855.5E6	40.000	40.000
20)	A Methoxychlor	6.539	7.409	252.6E6	1873.8E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 04:08
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:02:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:58:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

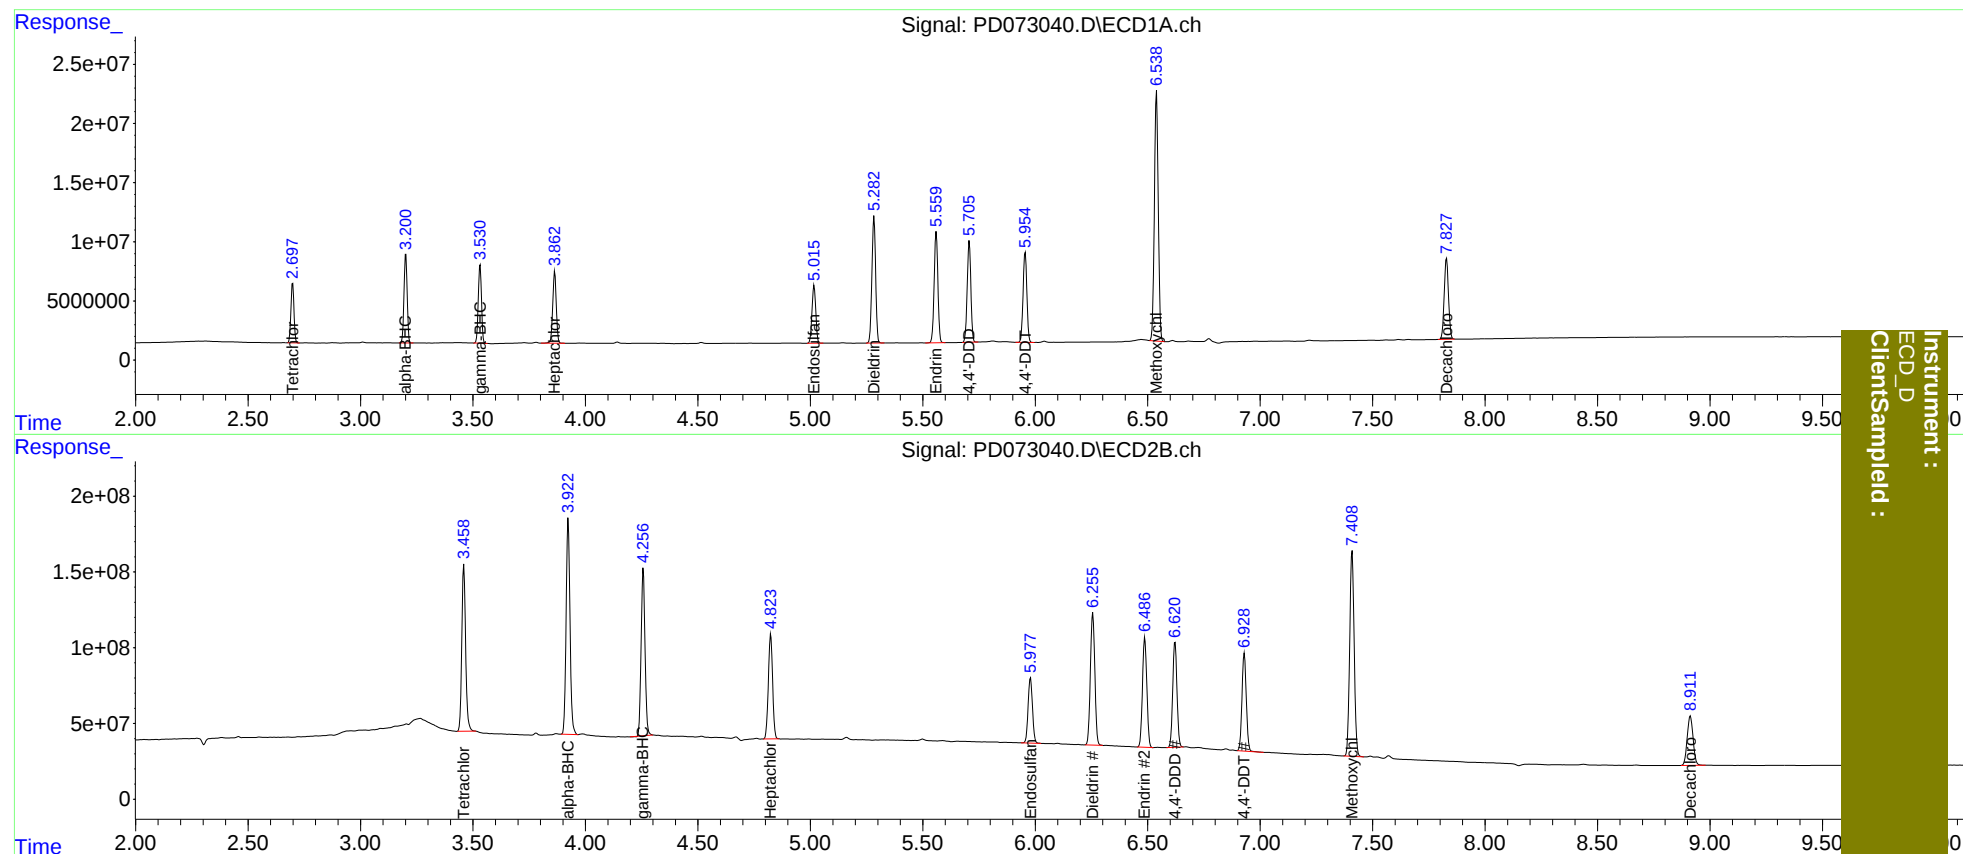


Instrument :
ECD_D
ClientSampled :

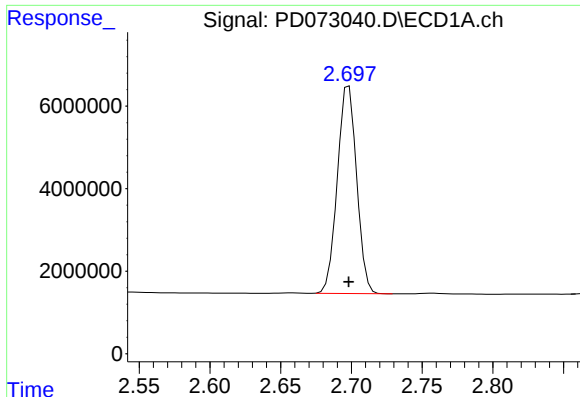

#1 Tetrachloro-m-xylene


R.T.: 2.698 min
Delta R.T.: 0.000 min
Response: 47856202
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

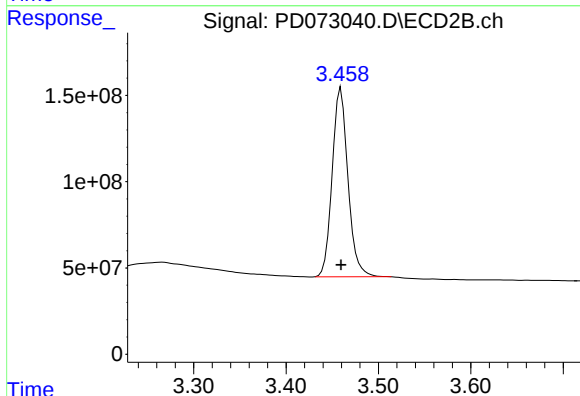


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 1300109542
Conc: 20.00 ng/ml

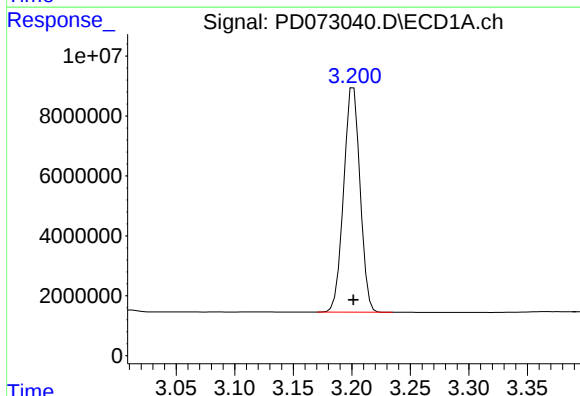


#2 alpha-BHC

R.T.: 3.201 min
Delta R.T.: 0.000 min
Response: 73262274
Conc: 20.00 ng/ml

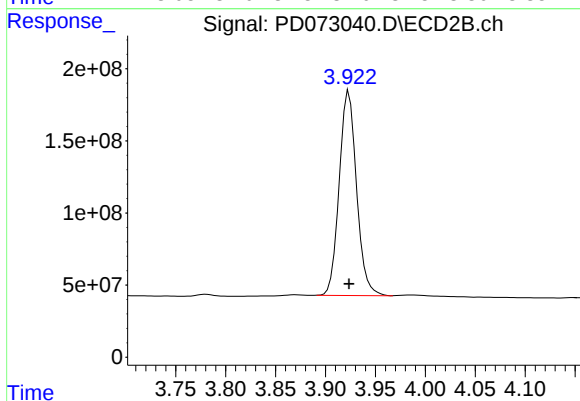

#2 alpha-BHC


R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 1716781217
Conc: 20.00 ng/ml

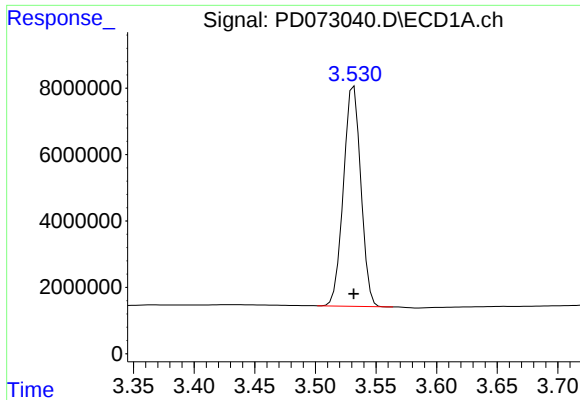

#3 gamma-BHC (Lindane)


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 66114748
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

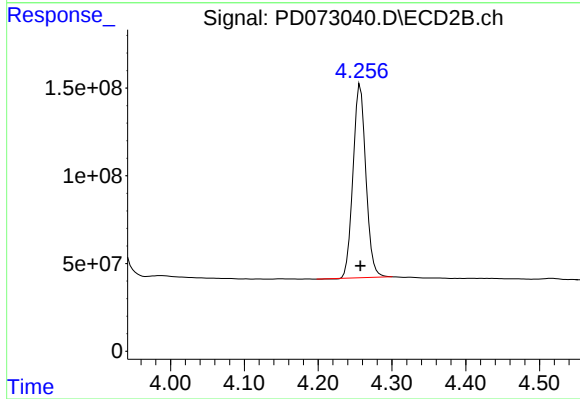


#3 gamma-BHC (Lindane)

R.T.: 4.257 min
Delta R.T.: 0.000 min
Response: 1333224391
Conc: 20.00 ng/ml

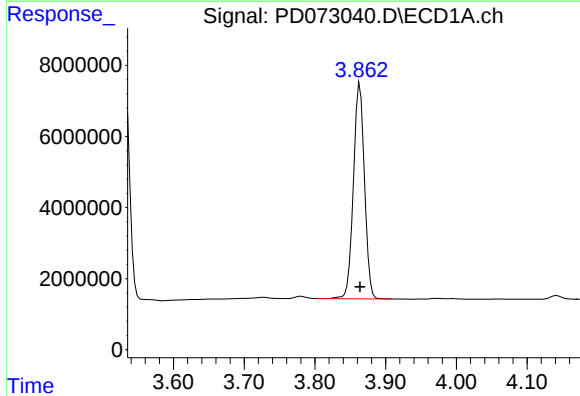


#4 Heptachlor

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 66160377
Conc: 20.00 ng/ml

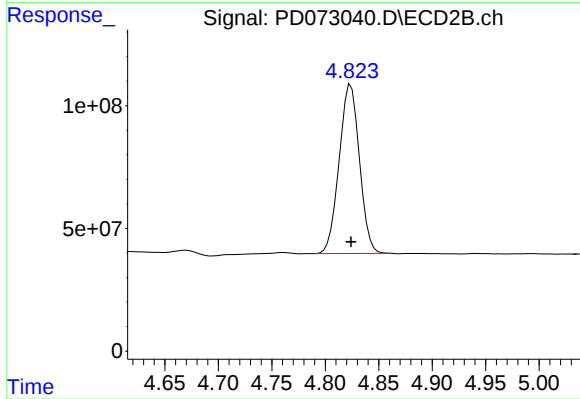

#4 Heptachlor


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 908554050
Conc: 20.00 ng/ml

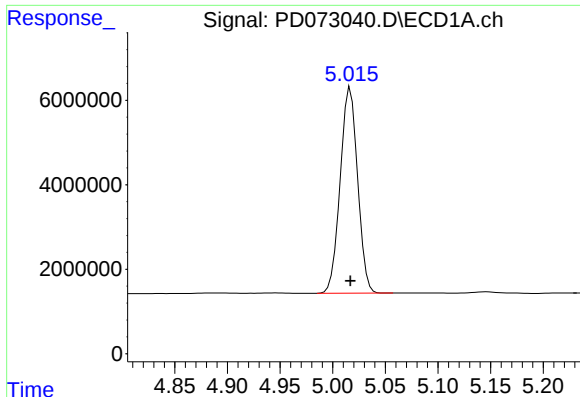

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 56301662
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

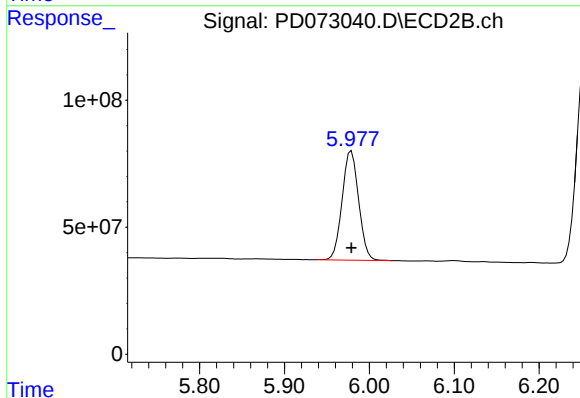


#9 Endosulfan I

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 580942840
Conc: 20.00 ng/ml

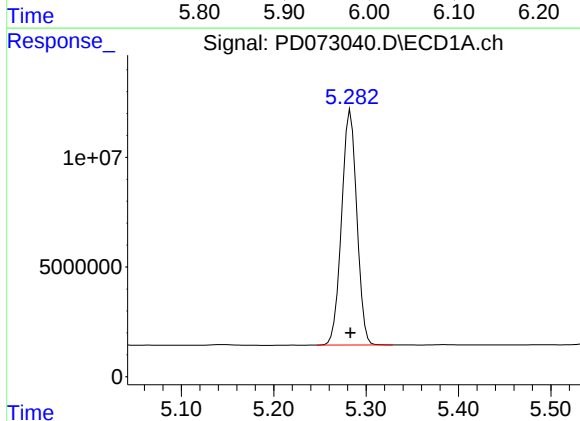


#13 Dieldrin

R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 122737131
Conc: 40.00 ng/ml

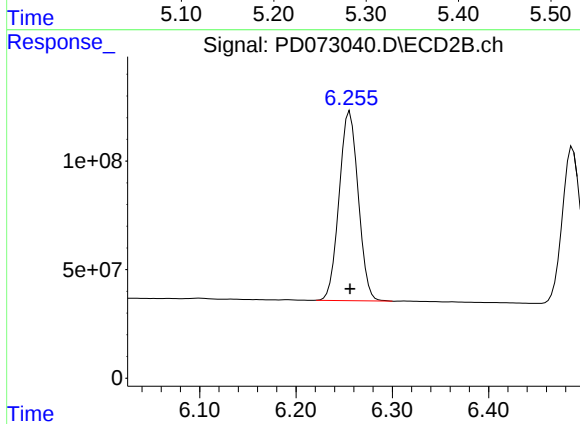

#13 Dieldrin


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 1200211417
Conc: 40.00 ng/ml

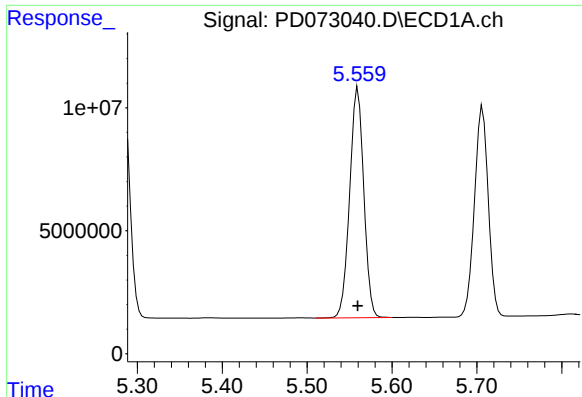

#14 Endrin


R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 107909721
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

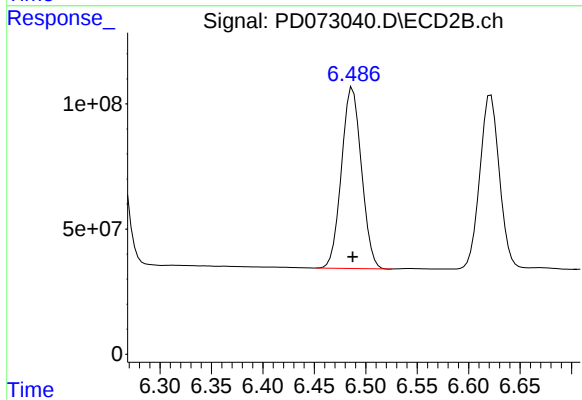


#14 Endrin

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 977605213
Conc: 40.00 ng/ml

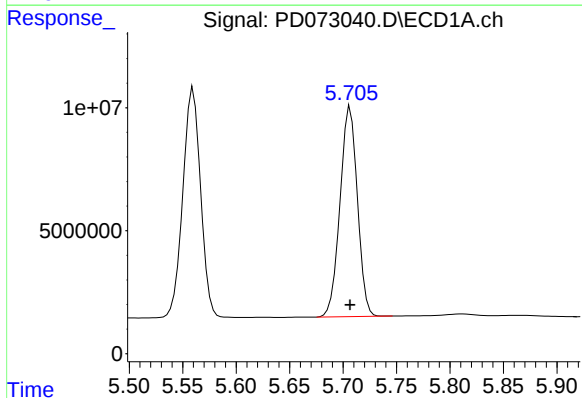


#16 4,4'-DDD

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 96742456
Conc: 40.00 ng/ml

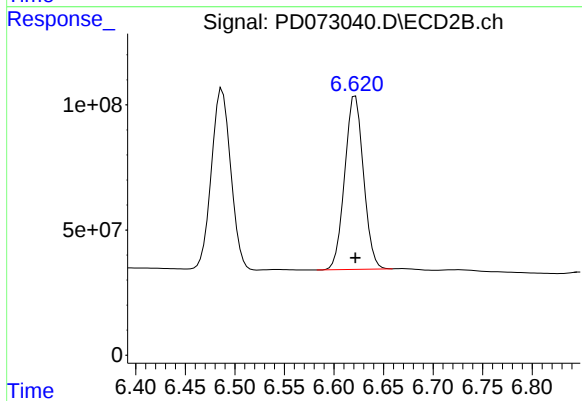

#16 4,4'-DDD


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 913319299
Conc: 40.00 ng/ml

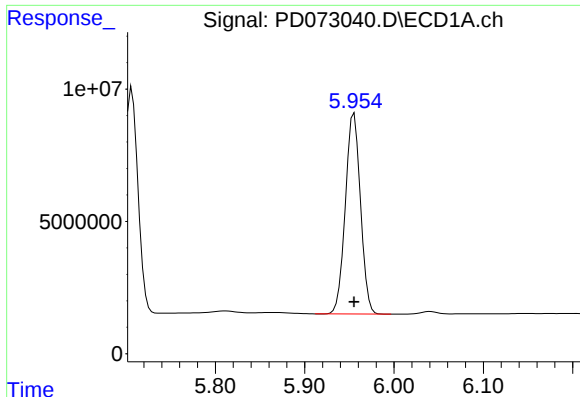

#17 4,4'-DDT


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 89182502
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

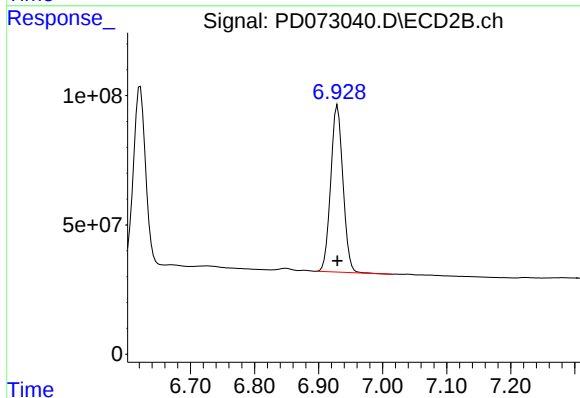


#17 4,4'-DDT

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 855477942
Conc: 40.00 ng/ml

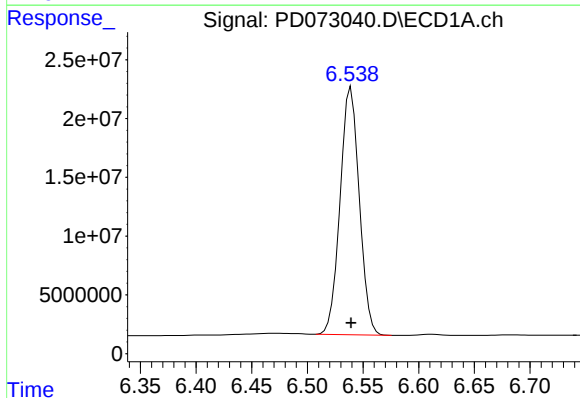


#20 Methoxychlor

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 252637285
Conc: 200.00 ng/ml

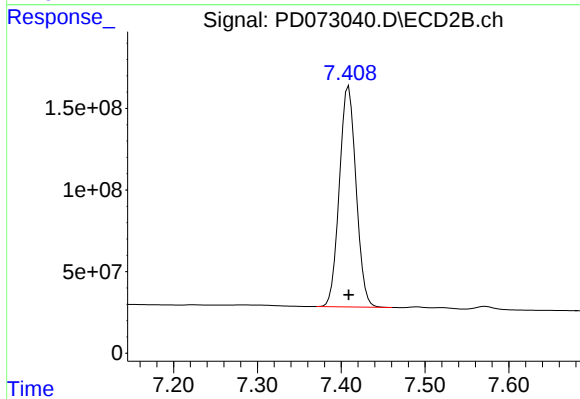

#20 Methoxychlor


R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 1873768684
Conc: 200.00 ng/ml

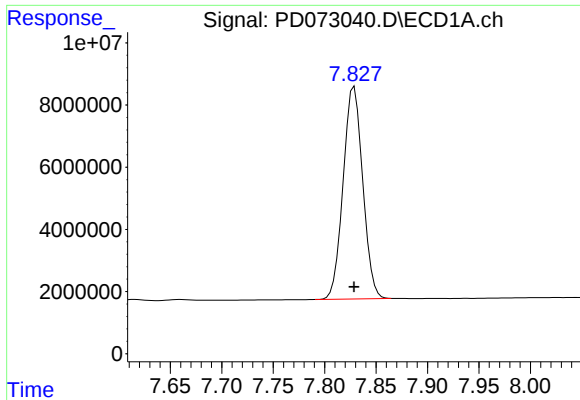

#27 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 90440692
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

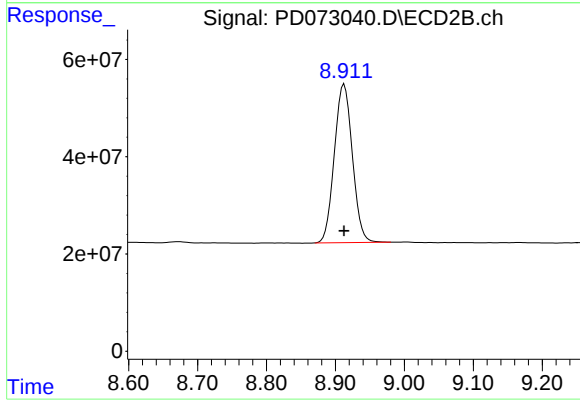

#27 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 592868444
Conc: 40.00 ng/ml