

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 04:34
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:03:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:58:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	91969677	2397.9E6	38.436	36.888
27)	SA Decachlor...	7.829	8.912	169.8E6	1098.6E6	75.090	74.123
Target Compounds							
2)	A alpha-BHC	3.202	3.924	148.7E6	3182.5E6	40.597	37.076
3)	MA gamma-BHC...	3.532	4.257	133.5E6	2456.9E6	40.378	36.856
4)	MA Heptachlor	3.864	4.824	131.9E6	1649.5E6	39.867	36.311
9)	A Endosulfan I	5.017	5.979	109.1E6	1068.9E6	38.764	36.797
13)	MA Dieldrin	5.283	6.256	245.7E6	2253.4E6	80.088	75.100
14)	MA Endrin	5.560	6.488	214.2E6	1822.7E6	79.410	74.579
16)	A 4,4'-DDD	5.707	6.622	192.7E6	1719.3E6	79.695	75.300
17)	MA 4,4'-DDT	5.956	6.930	185.7E6	1640.3E6	83.307	76.695
20)	A Methoxychlor	6.540	7.410	489.5E6	3495.8E6	387.484	373.131

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 04:34
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:03:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:58:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

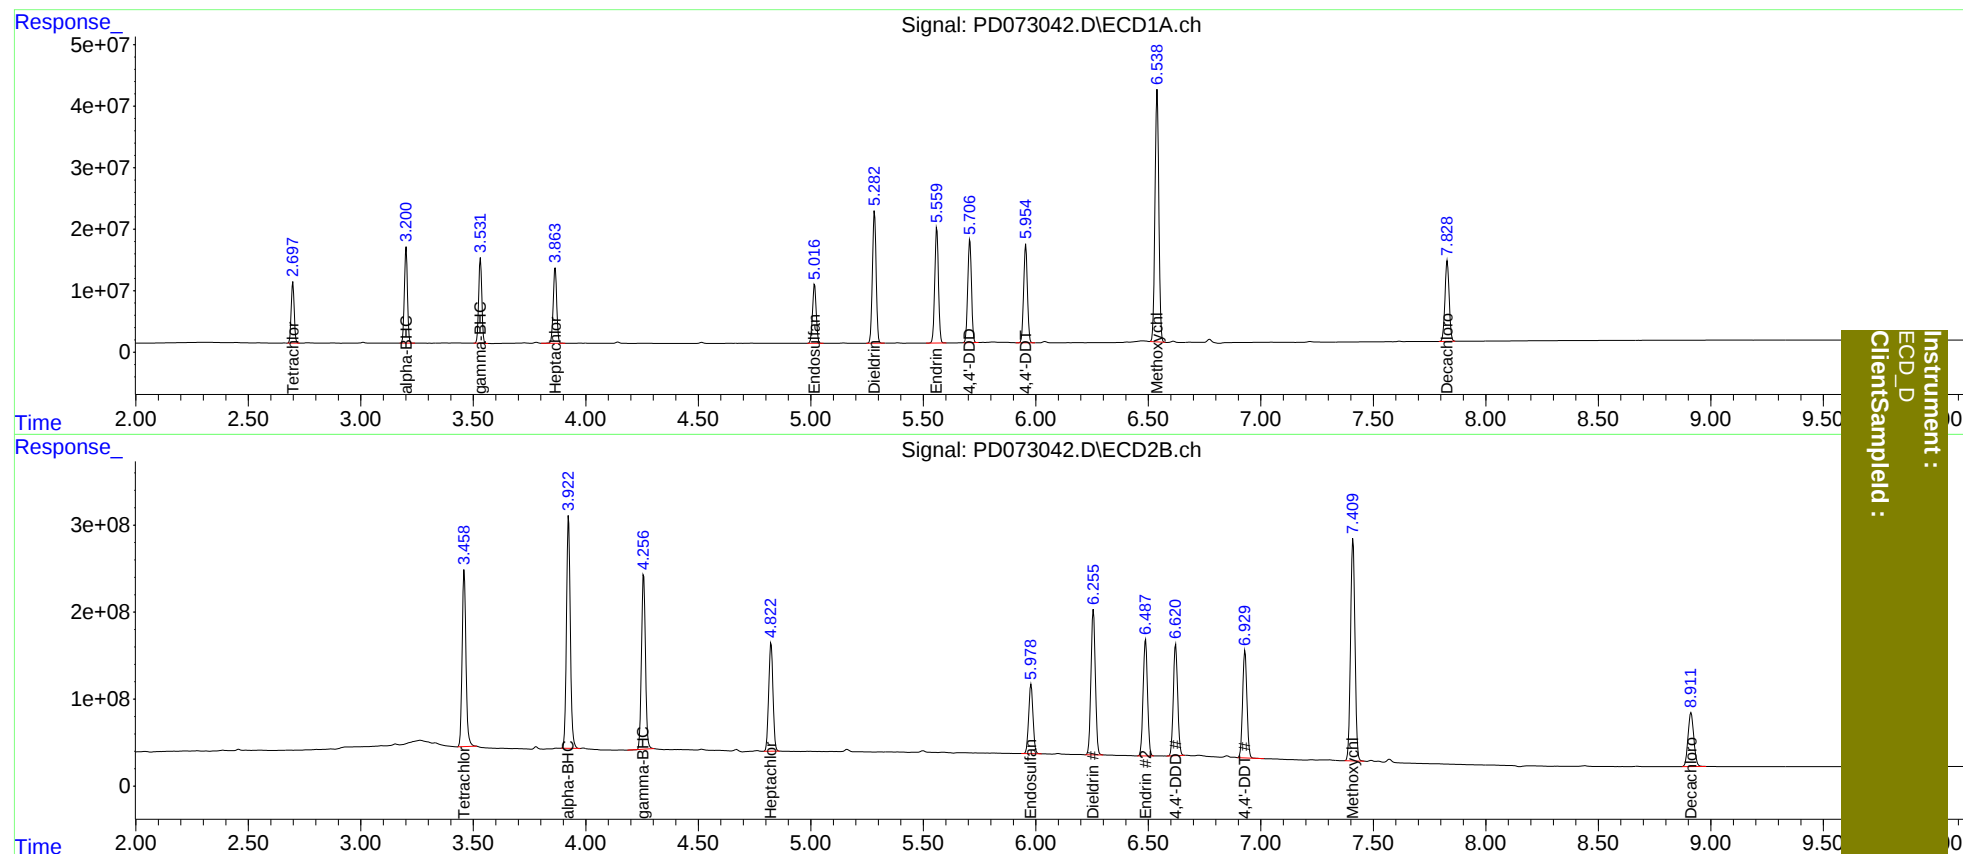


Instrument :
ECD_D
ClientSampled :
INDA401

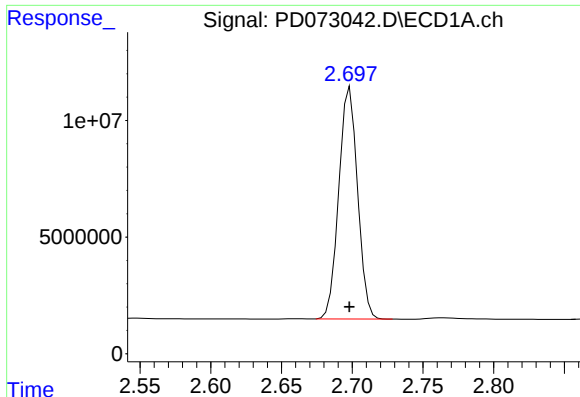

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 91969677
Conc: 38.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

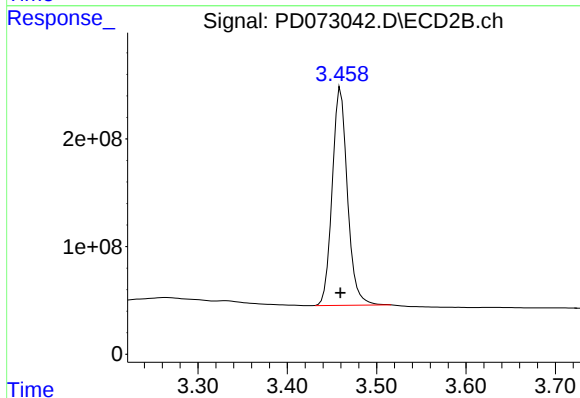


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 2397902656
Conc: 36.89 ng/ml

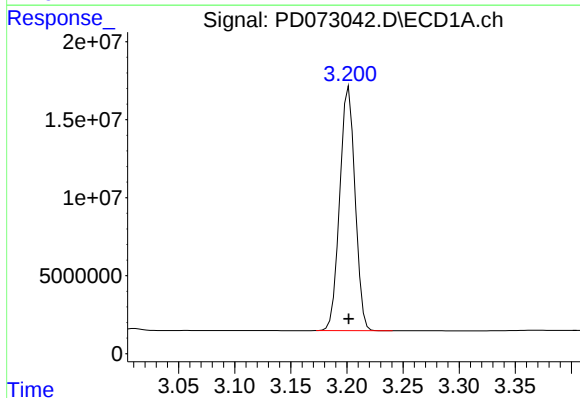


#2 alpha-BHC

R.T.: 3.202 min
Delta R.T.: 0.000 min
Response: 148710045
Conc: 40.60 ng/ml

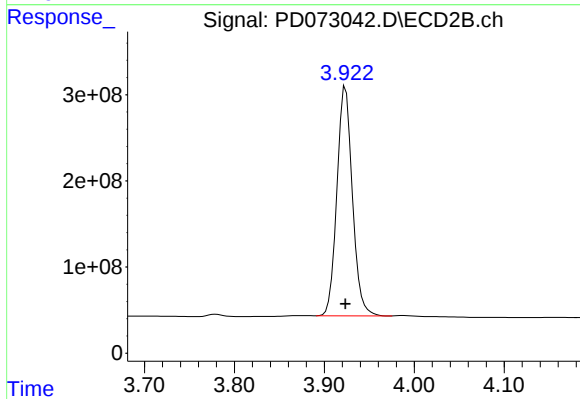

#2 alpha-BHC


R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 3182540761
Conc: 37.08 ng/ml

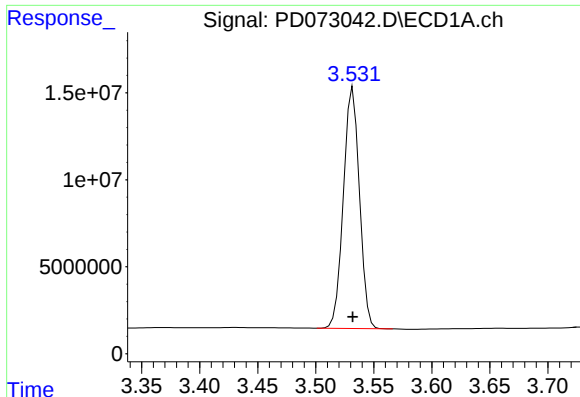

#3 gamma-BHC (Lindane)


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 133478335
Conc: 40.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

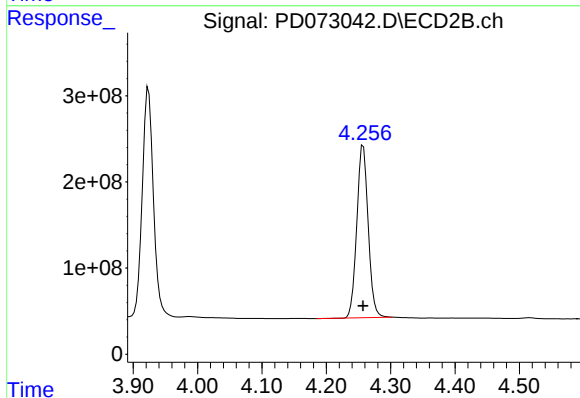


#3 gamma-BHC (Lindane)

R.T.: 4.257 min
Delta R.T.: 0.000 min
Response: 2456896728
Conc: 36.86 ng/ml

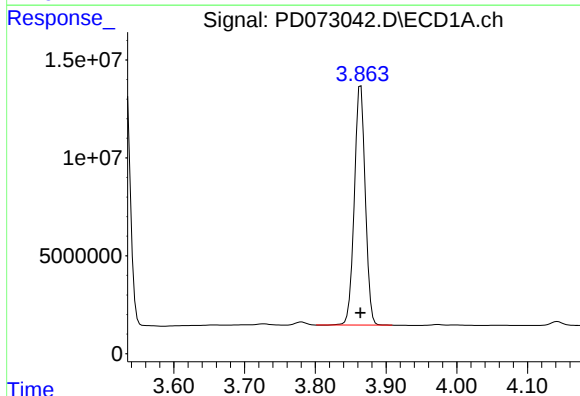


#4 Heptachlor

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 131881261
Conc: 39.87 ng/ml

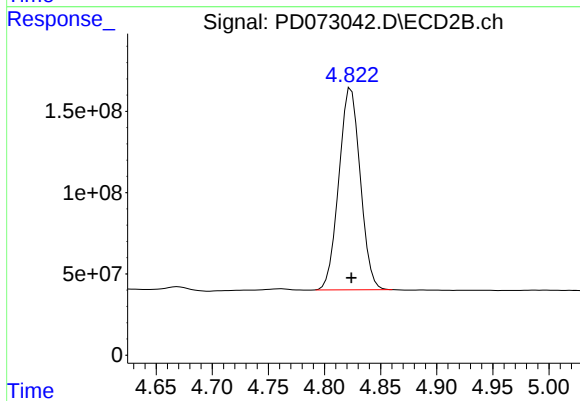

#4 Heptachlor


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 1649541686
Conc: 36.31 ng/ml

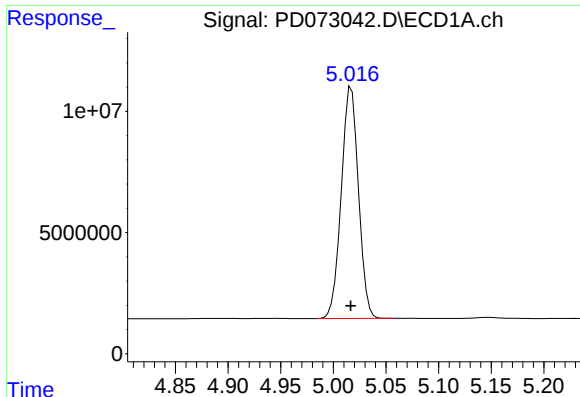

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 109123603
Conc: 38.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

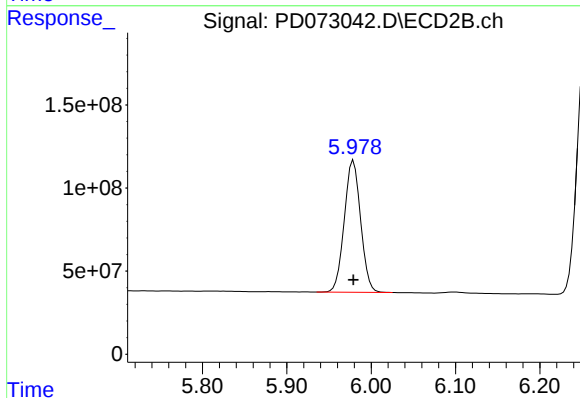


#9 Endosulfan I

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 1068859490
Conc: 36.80 ng/ml

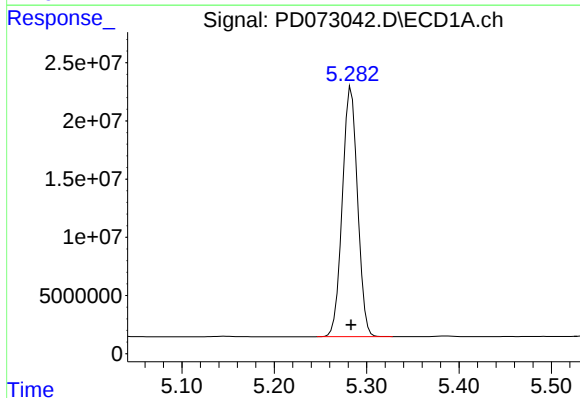


#13 Dieldrin

R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 245744159
Conc: 80.09 ng/ml

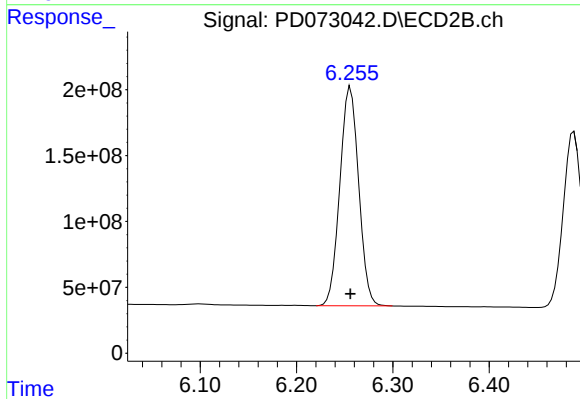

#13 Dieldrin


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 2253382654
Conc: 75.10 ng/ml

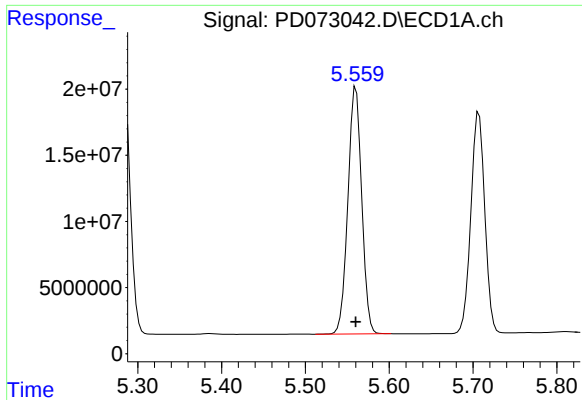

#14 Endrin


R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 214228916
Conc: 79.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

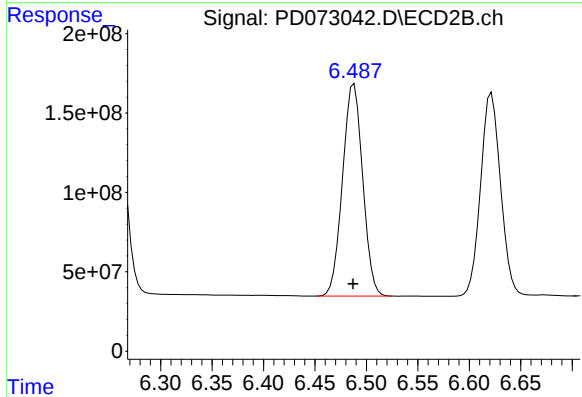


#14 Endrin

R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 1822726227
Conc: 74.58 ng/ml

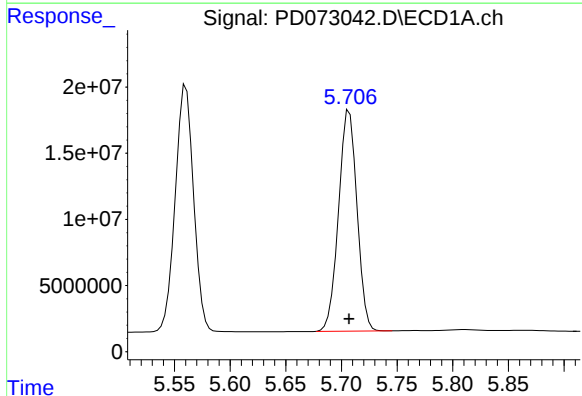


#16 4,4'-DDD

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 192747313
Conc: 79.70 ng/ml

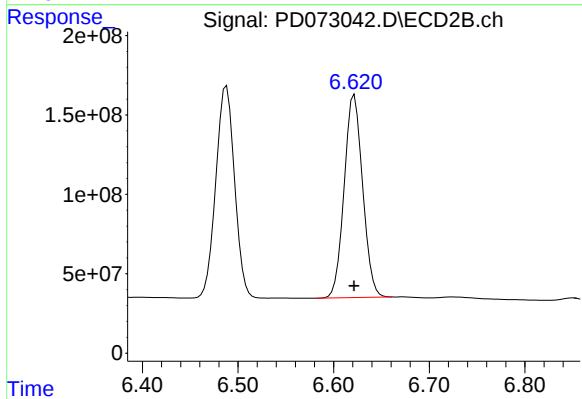

#16 4,4'-DDD


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 1719331177
Conc: 75.30 ng/ml

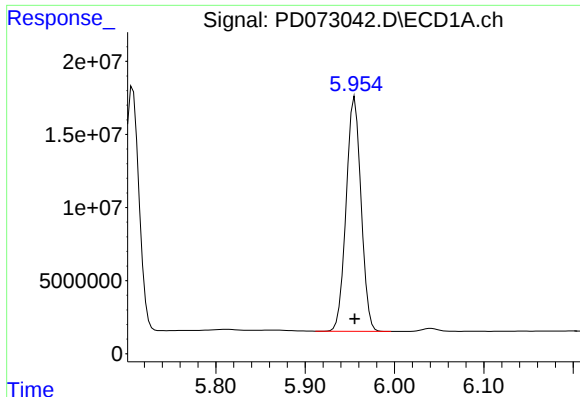

#17 4,4'-DDT


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 185738380
Conc: 83.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

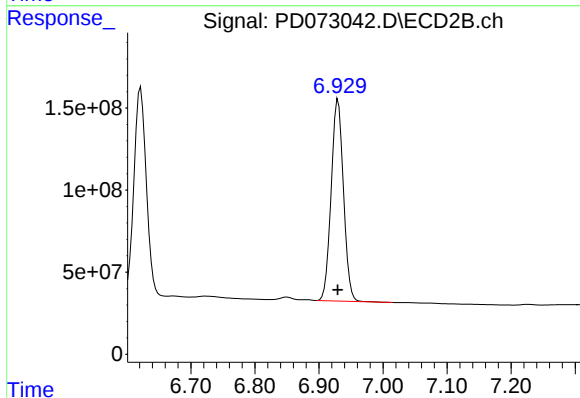


#17 4,4'-DDT

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 1640263204
Conc: 76.69 ng/ml

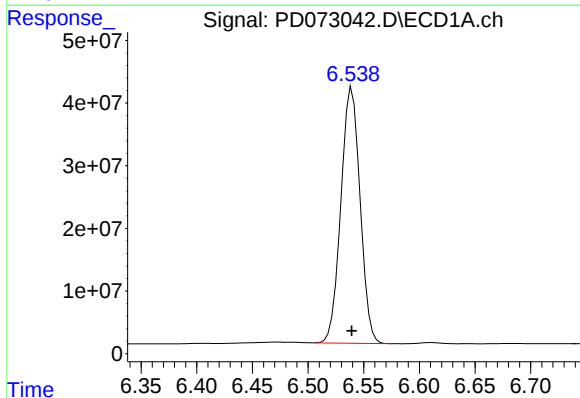


#20 Methoxychlor

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 489464888
Conc: 387.48 ng/ml

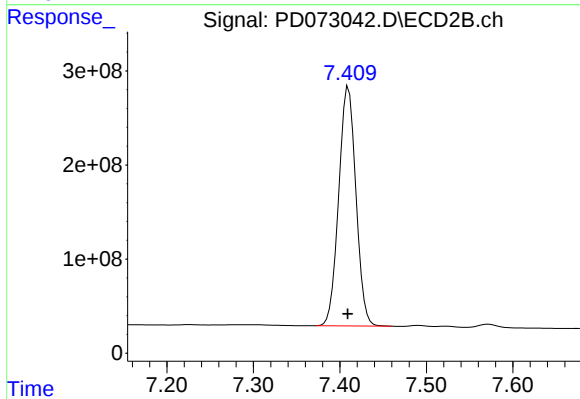

#20 Methoxychlor


R.T.: 7.410 min
Delta R.T.: 0.001 min
Response: 3495803822
Conc: 373.13 ng/ml

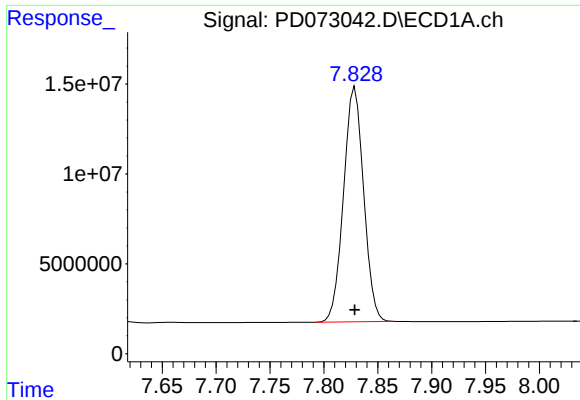

#27 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 169779932
Conc: 75.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

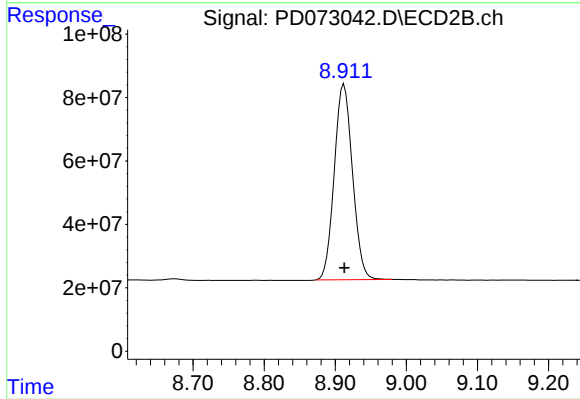

#27 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.000 min
Response: 1098634092
Conc: 74.12 ng/ml